

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
 Data File : BG050015.D
 Acq On : 28 Aug 2021 3:56
 Operator : CG/JU
 Sample : PB138564BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK564

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050016.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	44	49	53	rVB5	6340	10120	1.10%	0.110%
2	3.751	118	121	136	rBV	77287	160349	17.38%	1.739%
3	4.021	165	167	170	rBV3	1437	1687	0.18%	0.018%
4	4.085	175	178	179	rBV3	1335	1309	0.14%	0.014%
5	5.378	396	398	401	rBV2	1394	1418	0.15%	0.015%
6	5.437	405	408	412	rBV3	1503	1589	0.17%	0.017%
7	5.883	482	484	487	rBV2	1879	1487	0.16%	0.016%
8	5.942	491	494	497	rBV	1297	1846	0.20%	0.020%
9	7.134	690	697	706	rBV	145671	251654	27.27%	2.729%
10	7.287	714	723	732	rBV	94611	162165	17.58%	1.758%
11	7.498	750	759	769	rBV	139147	248891	26.97%	2.699%
12	7.704	792	794	797	rBV	1138	1376	0.15%	0.015%
13	7.963	831	838	846	rBV2	89275	152824	16.56%	1.657%
14	8.685	954	961	971	rBV2	172178	315977	34.25%	3.426%
15	8.756	971	973	975	rVV2	2367	2177	0.24%	0.024%
16	8.803	979	981	985	rVB	1397	1731	0.19%	0.019%
17	9.137	1031	1038	1048	rBV	142227	250717	27.17%	2.719%
18	9.860	1154	1161	1169	rBV	125861	234555	25.42%	2.543%
19	10.412	1248	1255	1265	rBV2	173010	321109	34.80%	3.482%
20	10.612	1287	1289	1291	rBV	1305	1395	0.15%	0.015%
21	10.782	1311	1318	1327	rVB	122762	217696	23.59%	2.361%
22	10.923	1335	1342	1357	rBV	171370	318166	34.48%	3.450%
23	11.076	1365	1368	1371	rBV	921	1302	0.14%	0.014%
24	12.380	1585	1590	1594	rVB2	2946	4315	0.47%	0.047%
25	14.025	1863	1870	1877	rBV	351656	506058	54.85%	5.488%
26	14.319	1913	1920	1930	rBV	366216	575674	62.39%	6.243%
27	14.624	1966	1972	1980	rVB	201472	314407	34.08%	3.409%
28	14.847	2005	2010	2022	rBV2	110704	219173	23.75%	2.377%
29	15.118	2054	2056	2060	rVB	1192	1361	0.15%	0.015%
30	15.217	2070	2073	2077	rBV	869	1376	0.15%	0.015%
31	15.617	2135	2141	2152	rVB	469562	713412	77.32%	7.736%
32	15.752	2159	2164	2177	rBV	145112	230224	24.95%	2.497%
33	15.852	2179	2181	2186	rVB3	3819	5344	0.58%	0.058%
34	17.038	2375	2383	2385	rBV2	834	1336	0.14%	0.014%
35	17.379	2435	2441	2448	rVV	259995	392650	42.56%	4.258%
36	17.479	2451	2458	2466	rVB2	531612	802337	86.96%	8.700%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
 Data File : BG050015.D
 Acq On : 28 Aug 2021 3:56
 Operator : CG/JU
 Sample : PB138564BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK564

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	18.789	2679	2681	2683	rBV	1715	1624	0.18%	0.018%
38	18.901	2697	2700	2701	rBV	999	1264	0.14%	0.014%
39	19.200	2749	2751	2756	rBV	1135	1935	0.21%	0.021%
40	19.329	2770	2773	2778	rBV2	7368	9257	1.00%	0.100%
41	19.406	2782	2786	2788	rBV2	5836	8573	0.93%	0.093%
42	19.482	2798	2799	2800	rBV	2872	1595	0.17%	0.017%
43	19.541	2807	2809	2813	rBV5	2746	3239	0.35%	0.035%
44	19.770	2841	2848	2855	rBV	637180	922686	100.00%	10.005%
45	19.993	2883	2886	2888	rVB2	1795	1785	0.19%	0.019%
46	20.029	2891	2892	2894	rBV2	1811	1356	0.15%	0.015%
47	20.070	2897	2899	2901	rBV	1471	1415	0.15%	0.015%
48	20.222	2923	2925	2928	rBV2	1548	1659	0.18%	0.018%
49	20.669	2999	3001	3008	rVB6	2691	4846	0.53%	0.053%
50	21.121	3077	3078	3080	rBV2	2493	1255	0.14%	0.014%
51	21.368	3117	3120	3123	rBV4	5339	5895	0.64%	0.064%
52	21.650	3162	3168	3175	rVB	265697	431645	46.78%	4.681%
53	22.508	3312	3314	3315	rBV2	3810	2366	0.26%	0.026%
54	23.912	3547	3553	3559	rBV10	9676	19924	2.16%	0.216%
55	24.652	3669	3679	3691	rVB	333045	891993	96.67%	9.673%
56	24.875	3707	3717	3729	rVB2	159590	453904	49.19%	4.922%
57	25.979	3900	3905	3906	rBV5	8623	13580	1.47%	0.147%
58	26.919	4064	4065	4067	rVB2	4079	1786	0.19%	0.019%
59	27.736	4202	4204	4205	rBV2	2809	1440	0.16%	0.016%
60	30.068	4599	4601	4603	rBV3	4725	4482	0.49%	0.049%
61	30.837	4730	4732	4734	rBV3	3962	3091	0.34%	0.034%




Sum of corrected areas: 9221802

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
Data File : BG050015.D
Acq On : 28 Aug 2021 3:56
Operator : CG/JU
Sample : PB138564BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK564

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

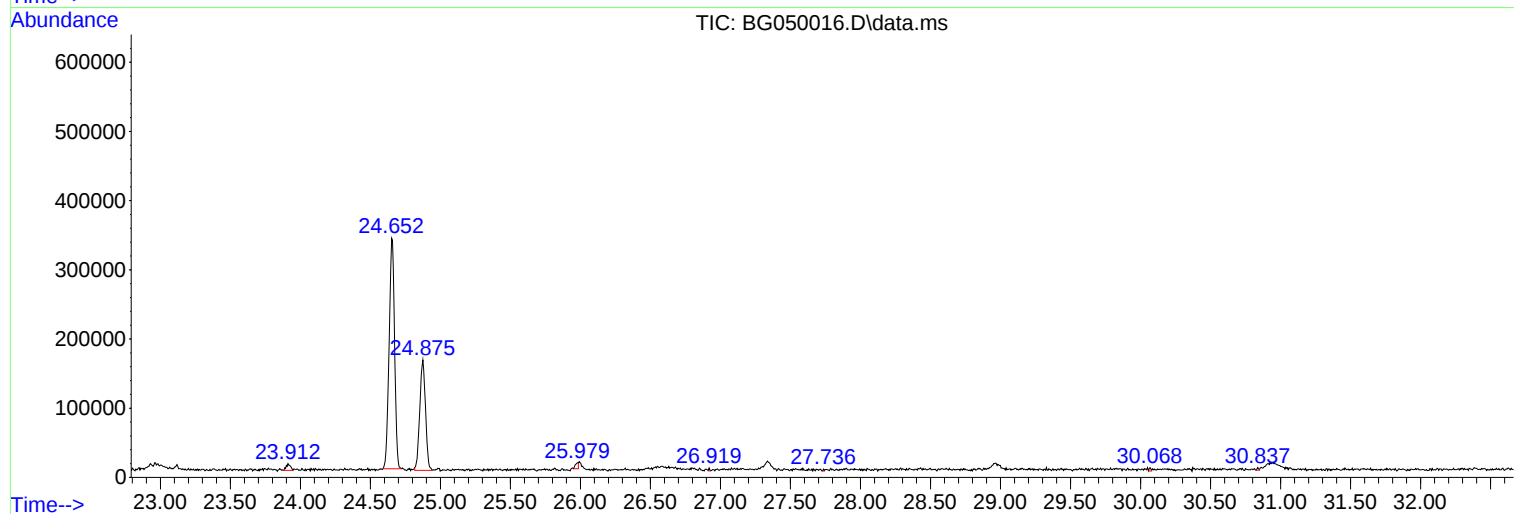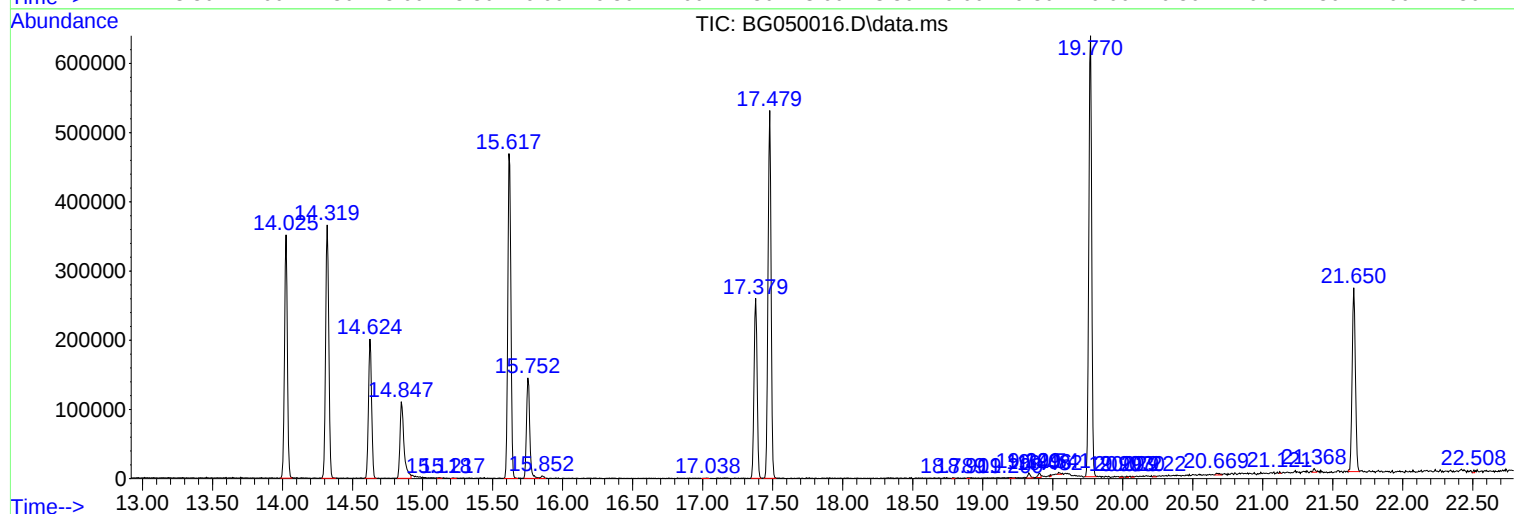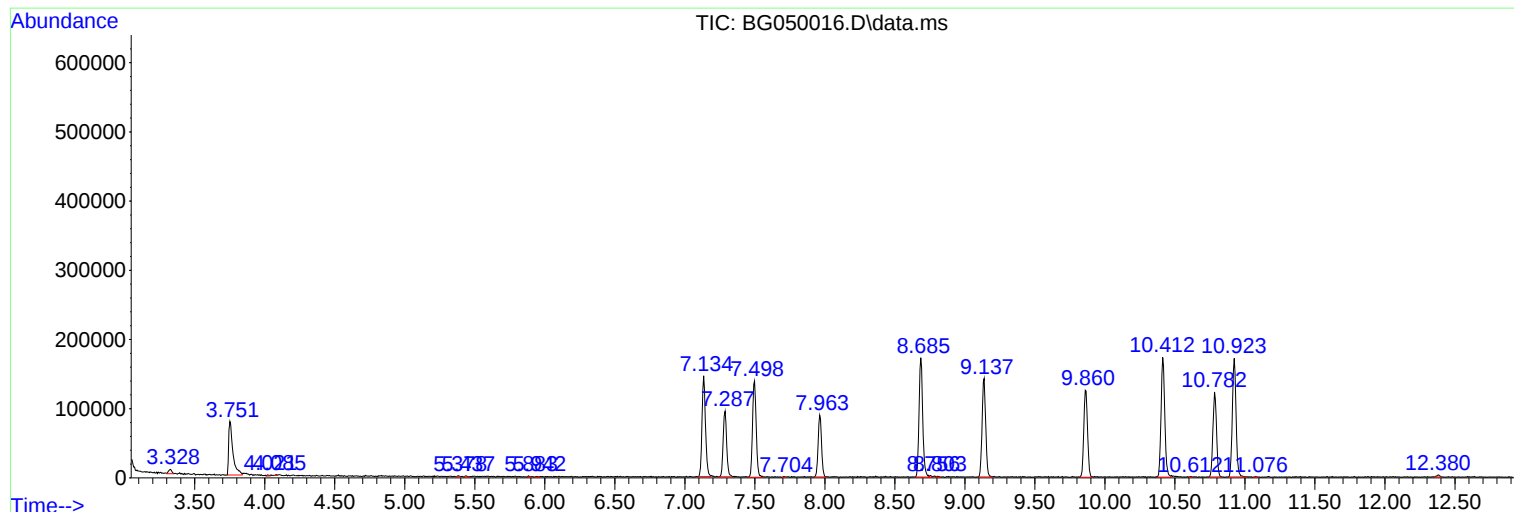

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
Data File : BG050015.D
Acq On : 28 Aug 2021 3:56
Operator : CG/JU
Sample : PB138564BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK564

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
Data File : BG050015.D
Acq On : 28 Aug 2021 3:56
Operator : CG/JU
Sample : PB138564BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK564

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
