
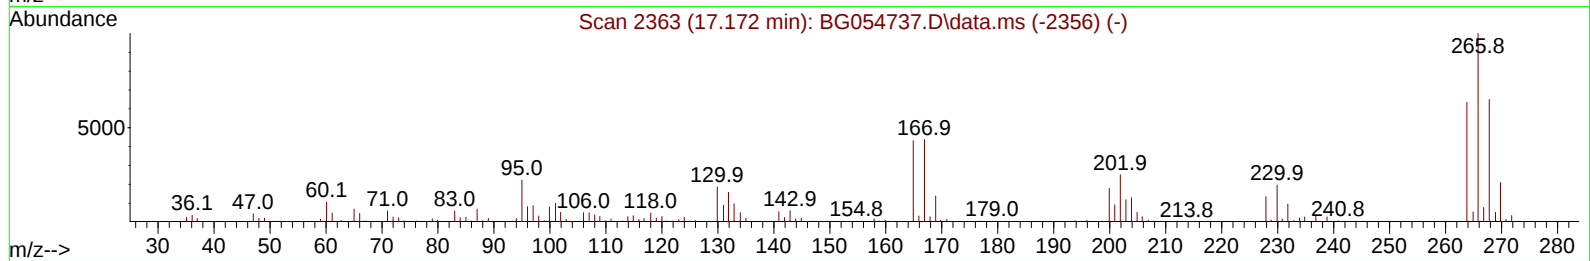
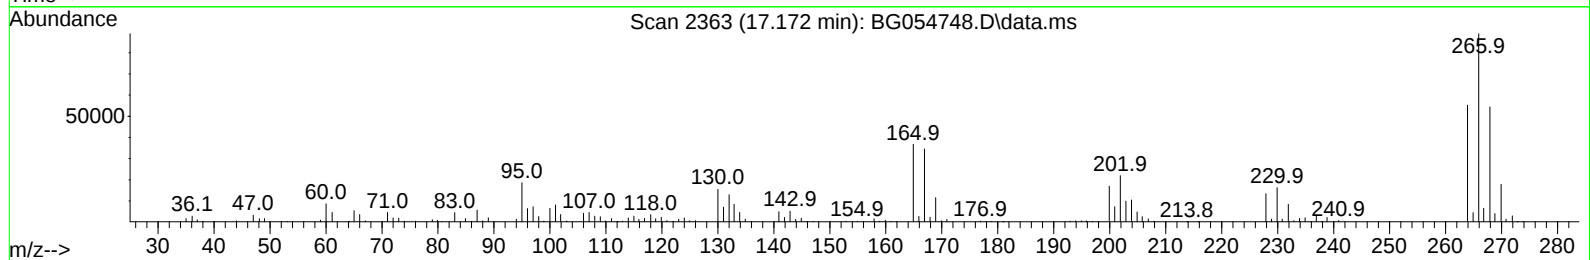


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082622\
Data File : BG054748.D
Acq On : 26 Aug 2022 9:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 27 04:40:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

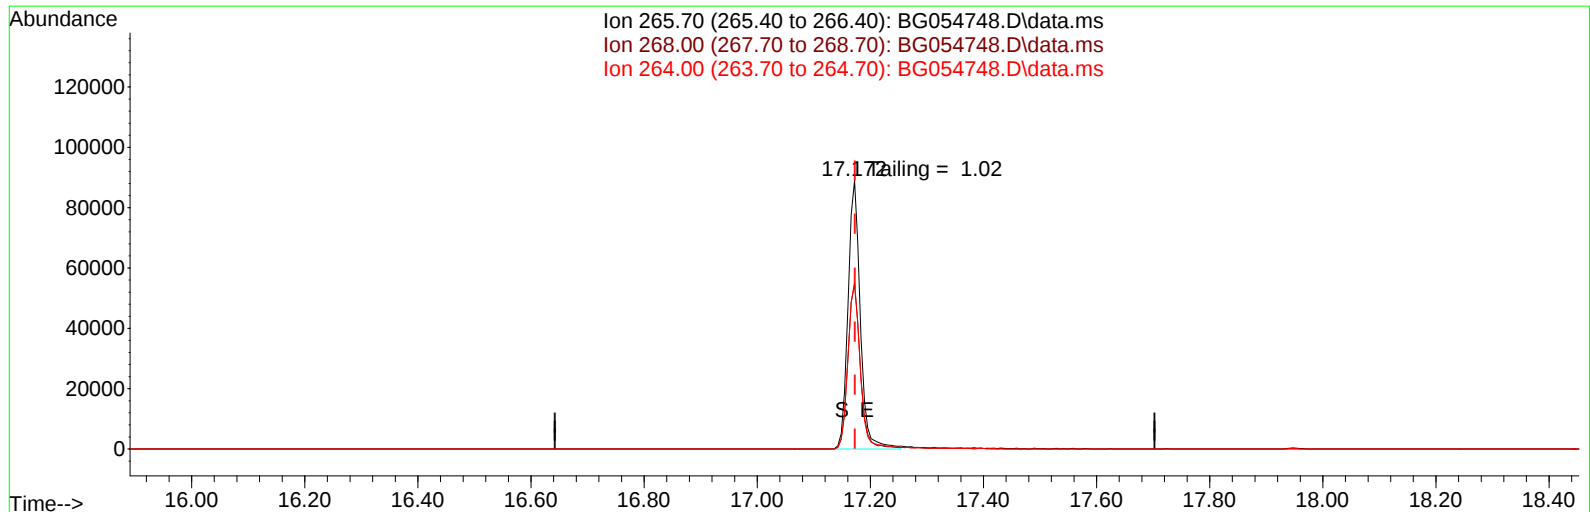

TIC: BG054748.D\data.ms

(70) Pentachlorophenol (C)




17.172min (-0.001) 28333.13 ng

response 136803

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	61.18
264.00	61.70	62.10
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082622\  
Data File : BG054748.D  
Acq On    : 26 Aug 2022    9:07  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Aug 27 04:40:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

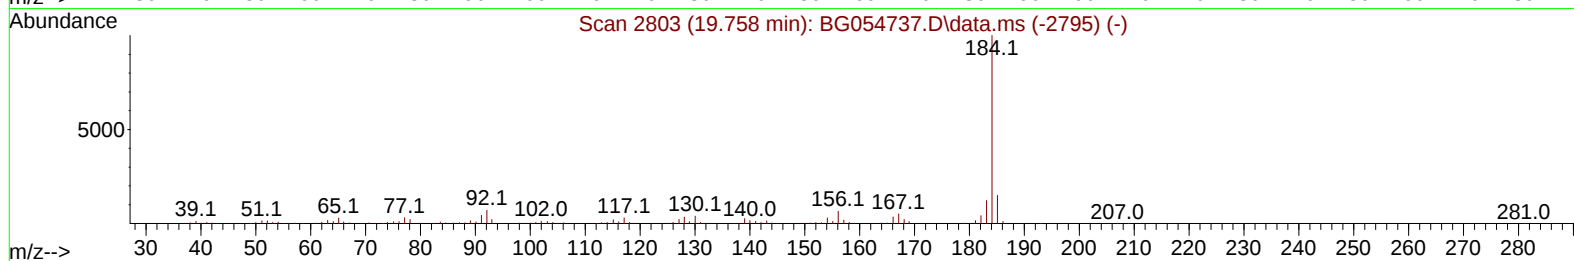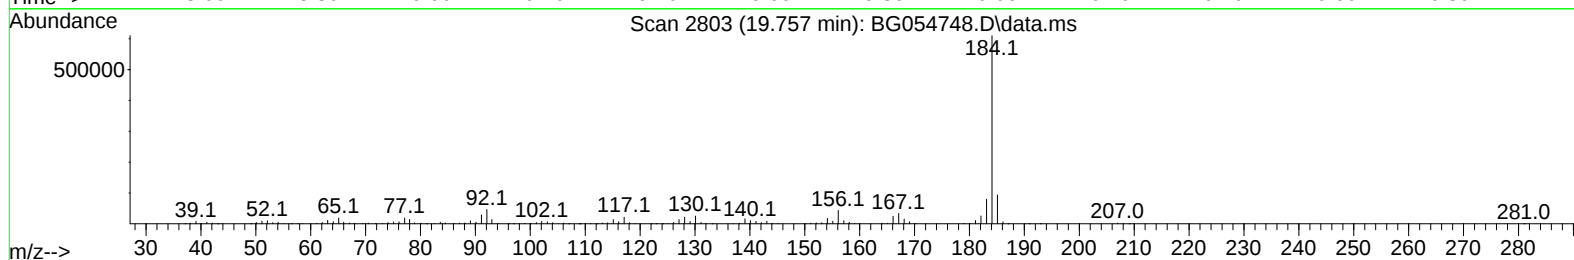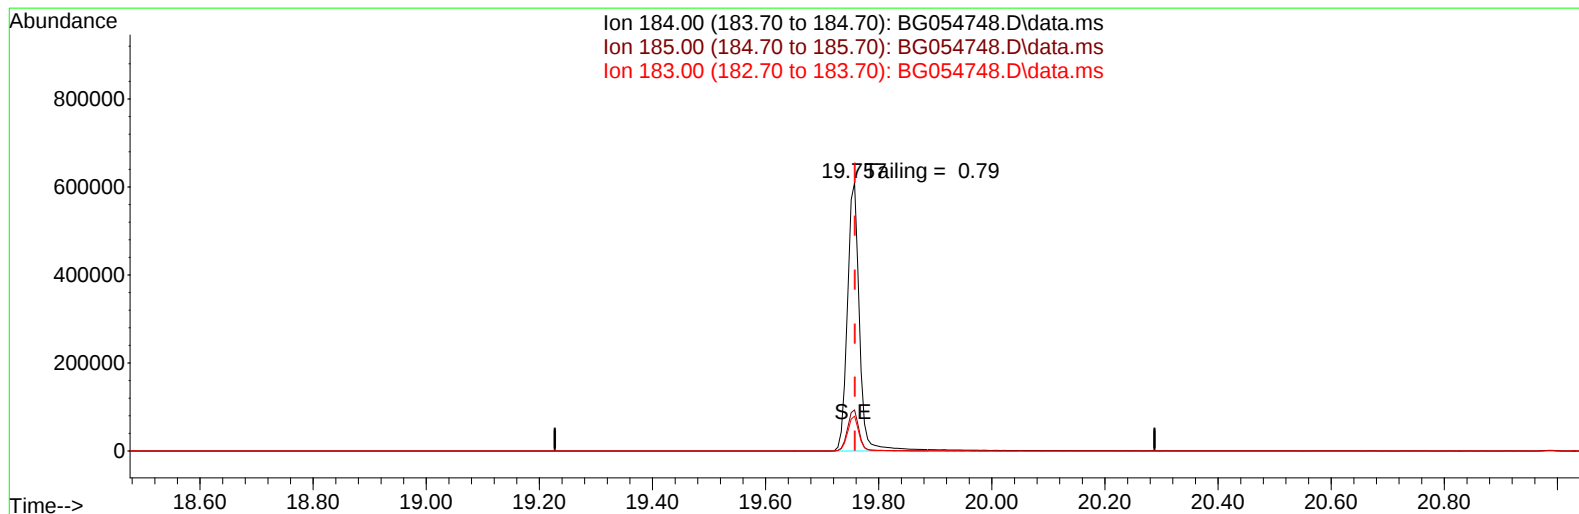

TIC: BG054748.D\data.ms

(77) Benzidine

19.757min (-0.001) 97898.72 ng

response **919011**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	15.33
183.00	12.30	13.04
0.00	0.00	0.00