
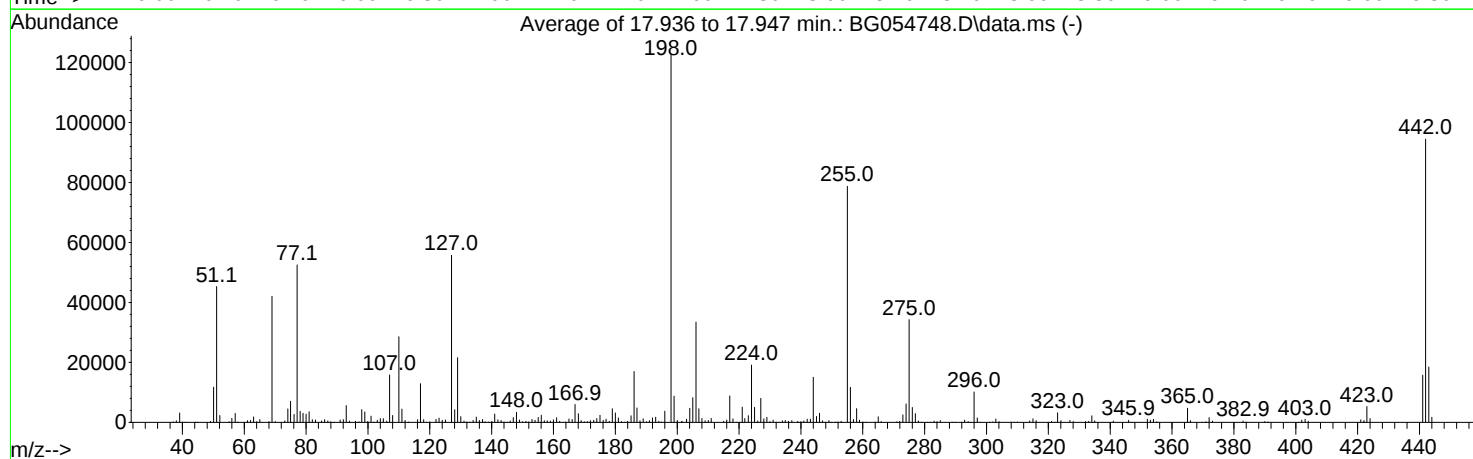


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082622\
 Data File : BG054748.D
 Acq On : 26 Aug 2022 9:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 25 17:50:55 2022

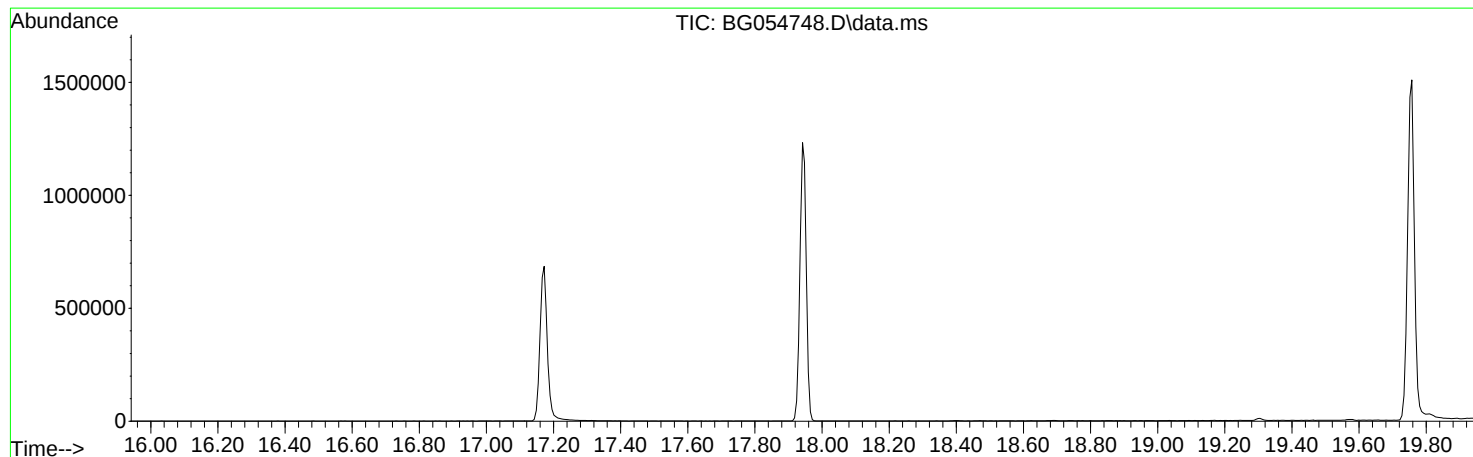

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	45304	PASS
68	69	0.00	2	0.6	251	PASS
69	198	0.00	100	34.3	42048	PASS
70	69	0.00	2	0.6	263	PASS
127	198	10	80	45.4	55720	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	122693	PASS
199	198	5	9	7.2	8774	PASS
275	198	10	60	27.9	34291	PASS
365	198	1	100	3.9	4724	PASS
441	198	0.01	100	12.8	15741	PASS
442	442	50	100	100.0	94477	PASS
443	442	15	24	19.5	18465	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/26/2022	BNA_G	<u>BG054748.D</u>
Compound Name	Response	Retention Time
DDT	444898	20.985
DDD	5498	20.538
DDE	76	20.033
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5574	450472	1.24

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082622\
Data File : BG054748.D
Acq On : 26 Aug 2022 9:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 27 04:40:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

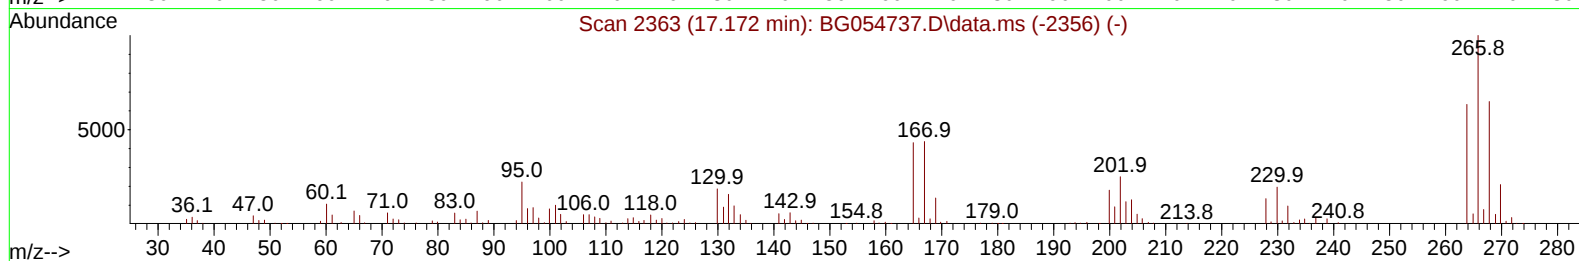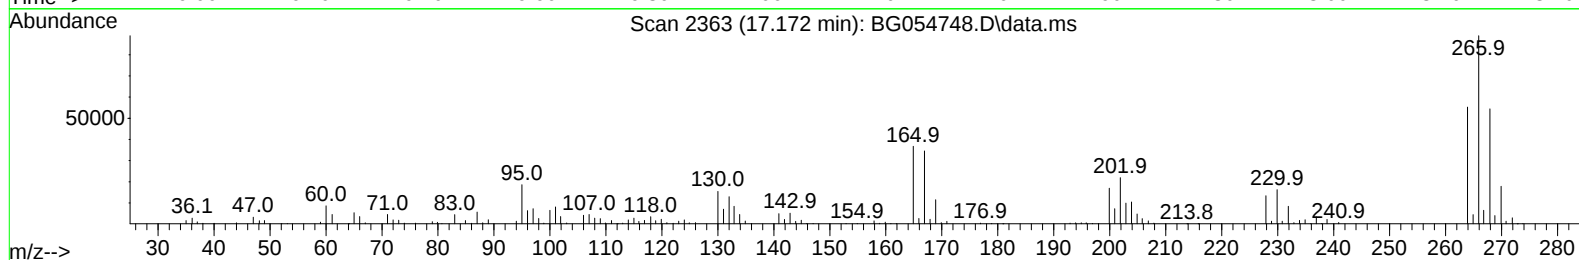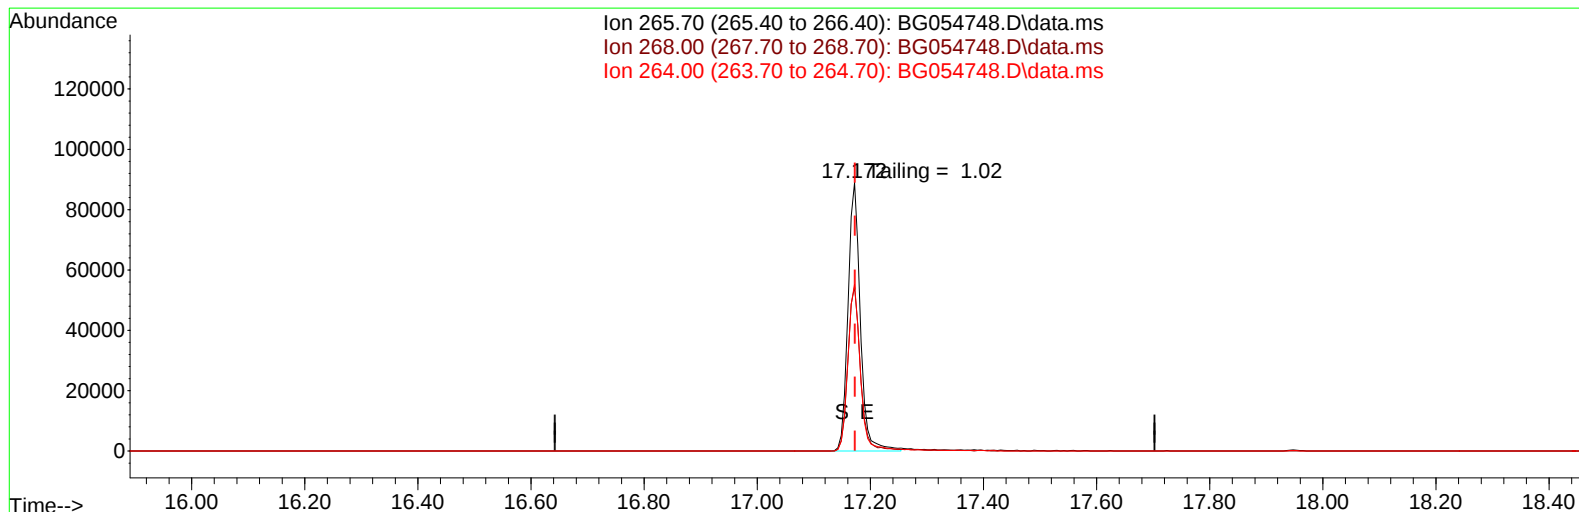

TIC: BG054748.D\data.ms

(70) Pentachlorophenol (C)

17.172min (-0.001) 28333.13 ng




response 136803

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	61.18
264.00	61.70	62.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082622\
 Data File : BG054748.D
 Acq On : 26 Aug 2022 9:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Aug 27 04:40:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 25 17:50:55 2022
 Response via : Initial Calibration

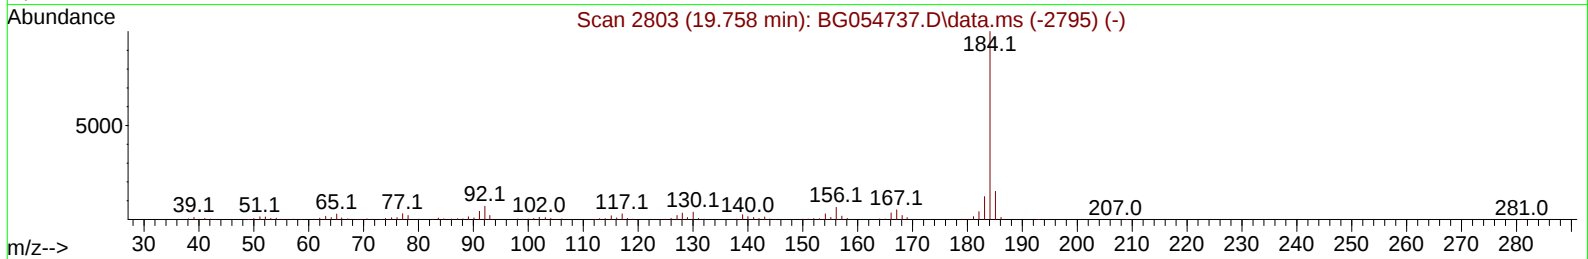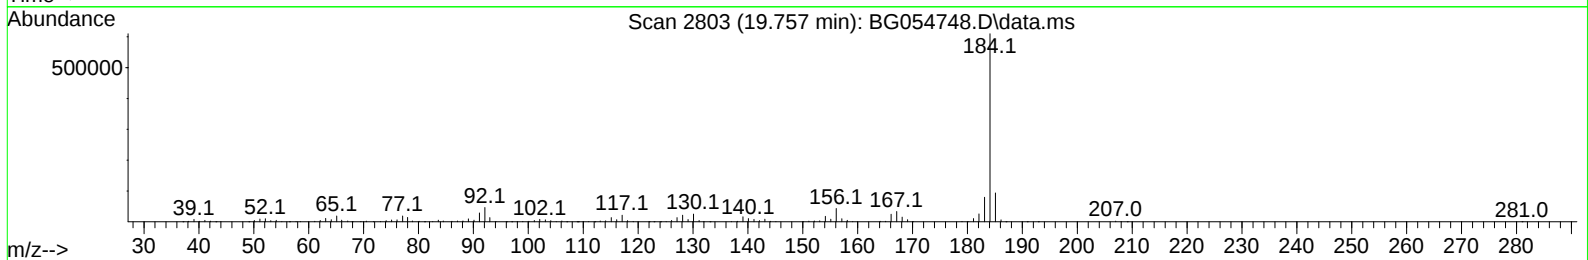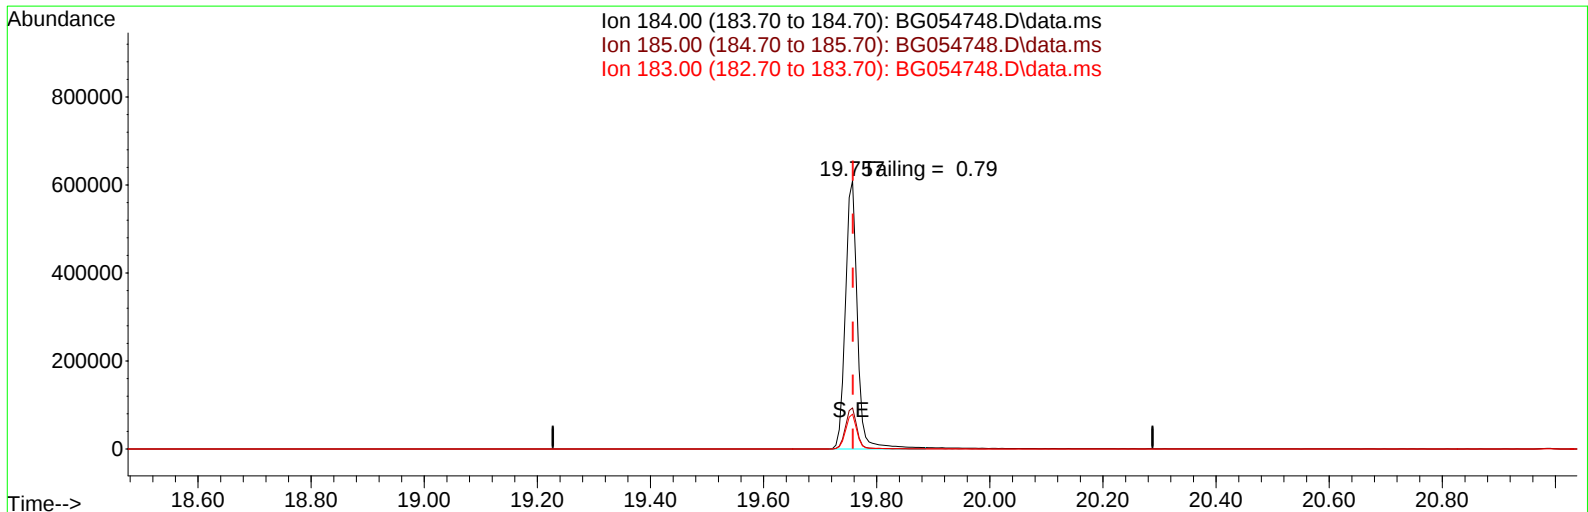

TIC: BG054748.D\data.ms

(77) Benzidine

19.757min (-0.001) 97898.72 ng

response 919011

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	15.33
183.00	12.30	13.04
0.00	0.00	0.00