
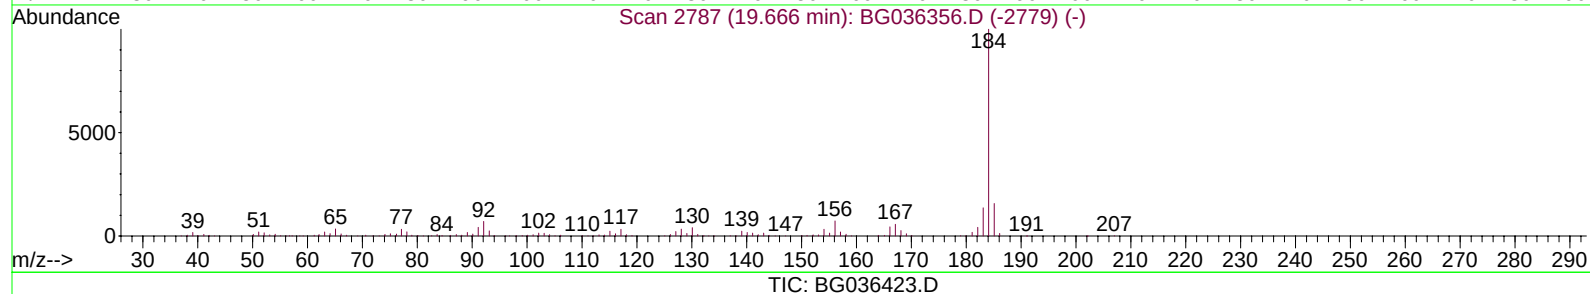
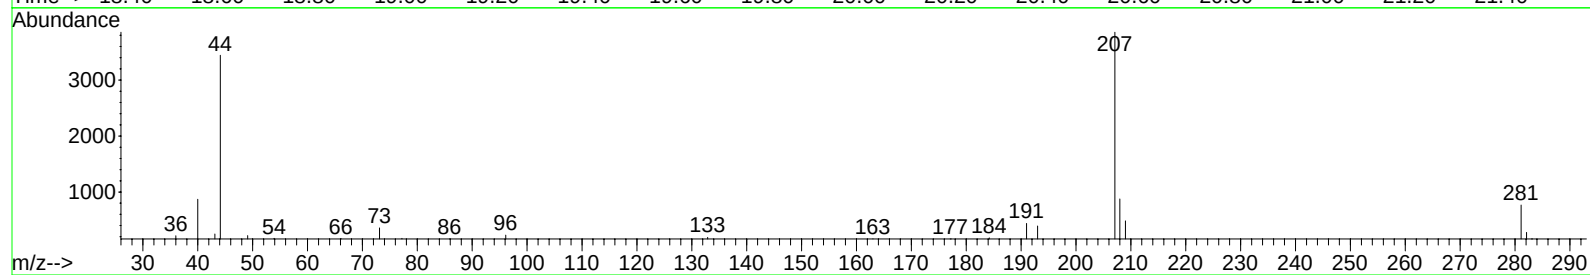


```
Data Path   : Z:\svoasrv\HPCHEM1\BNA G\Data\BG082718\  
Data File  : BG036423.D  
Acq On     : 27 Aug 2018    9:35  
Operator   : JU/SJ  
Sample     : DFTPP  
Misc       :  
ALS Vial   : 1      Sample Multiplier: 1
```

Quant Time: Aug 27 15:05:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 23 12:07:02 2018
Response via : Initial Calibration

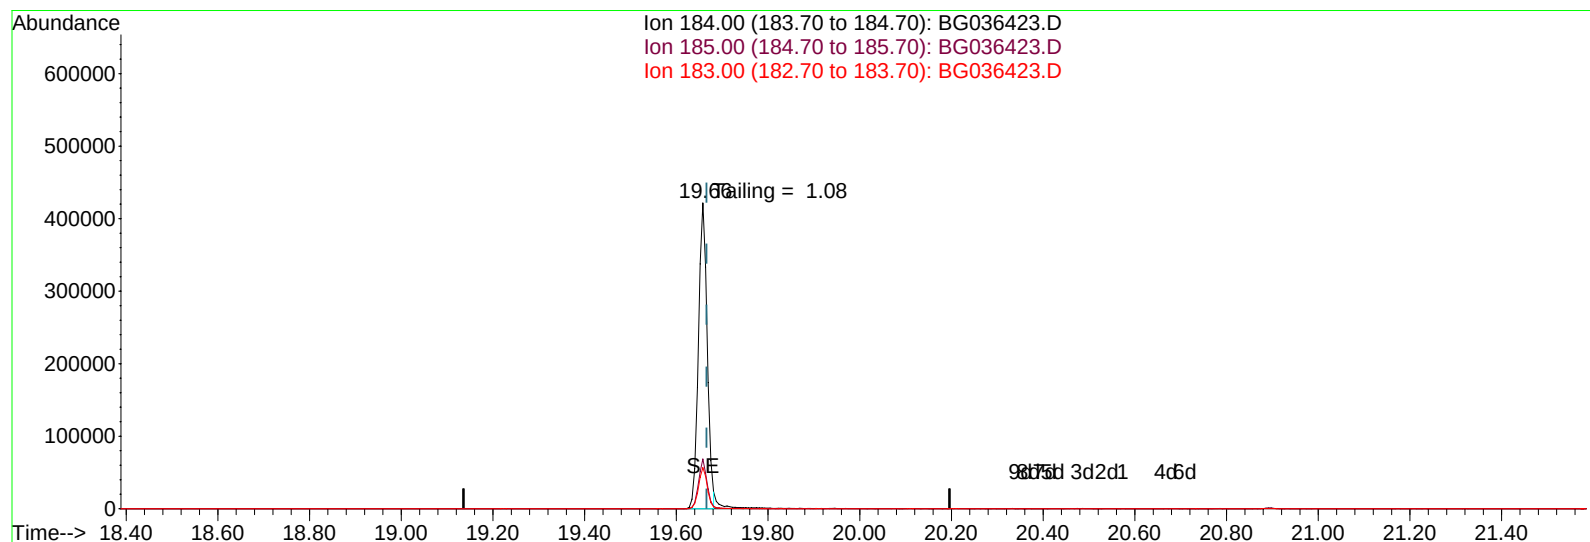

(76) Benzidine




20.574min (+0.908) 34.00ng

response 64

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	0.00#
183.00	13.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG082718\
Data File : BG036423.D
Acq On : 27 Aug 2018 9:35
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 27 15:05:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 23 12:07:02 2018
Response via : Initial Calibration

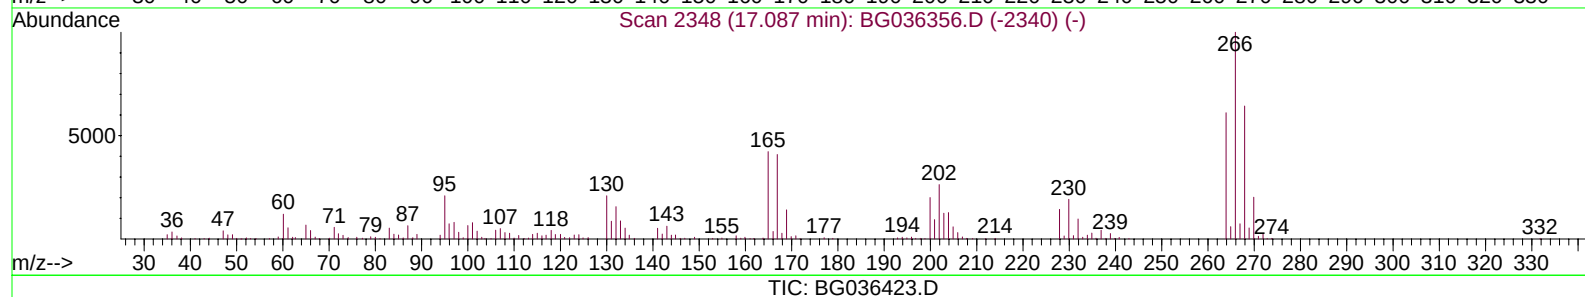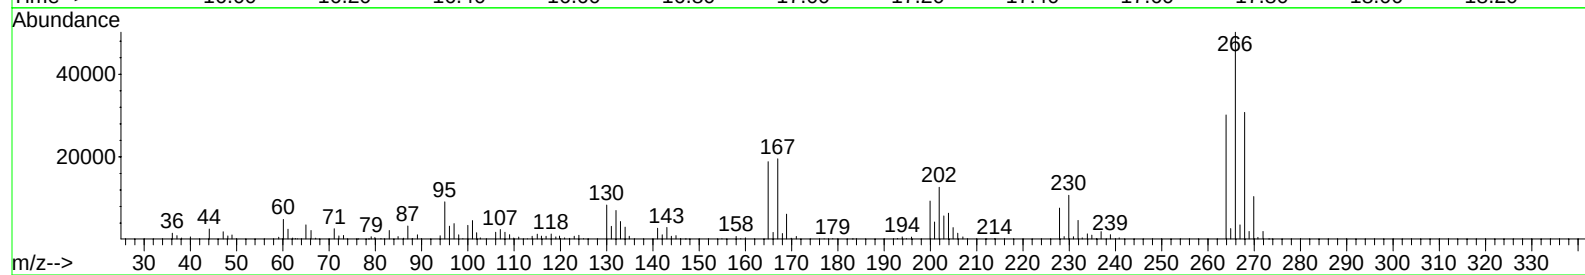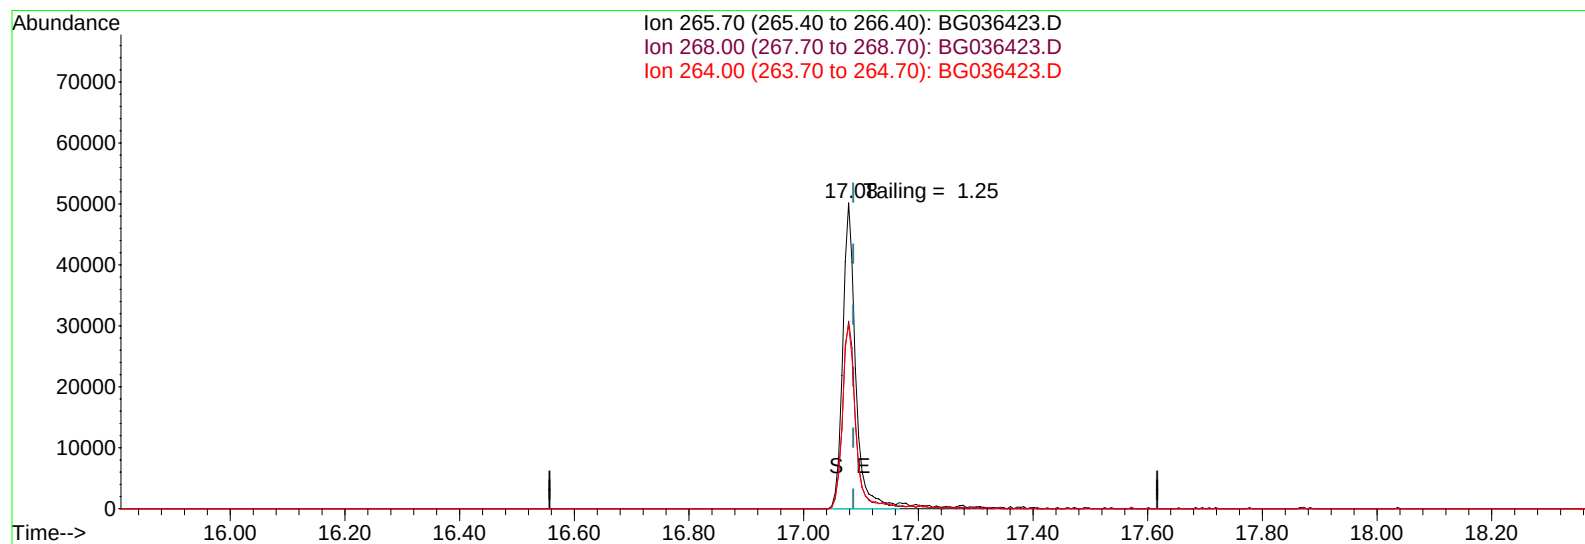

(69) Pentachlorophenol (C)

17.078min (-0.008) 15747.39ng

response 77902

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	61.34
264.00	61.10	60.14
0.00	0.00	0.00