
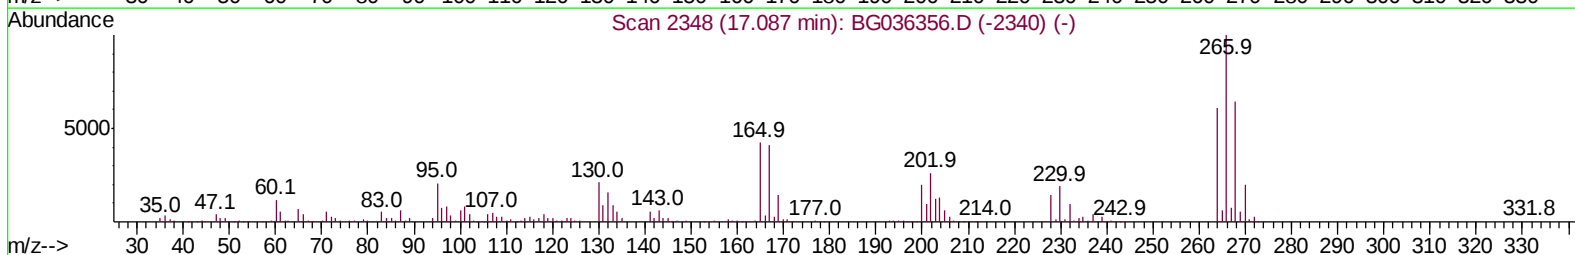
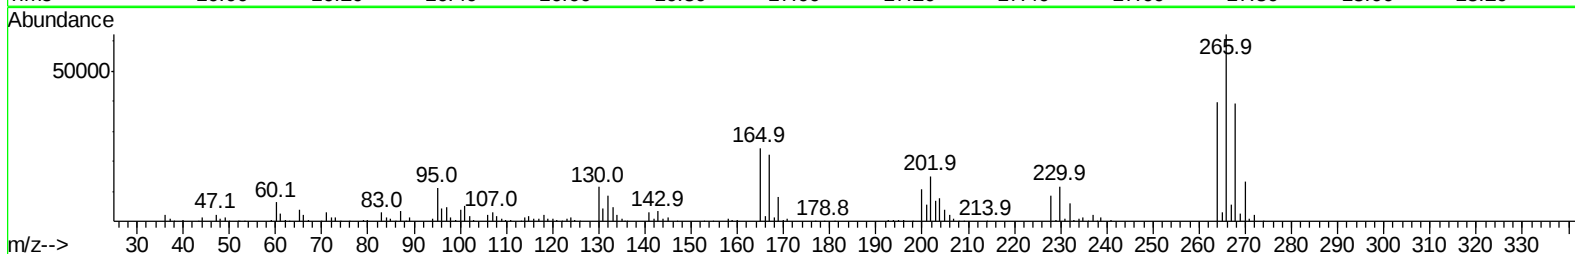


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082718\
Data File : BG036442.D
Acq On : 27 Aug 2018 23:14
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 05:55:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 23 12:07:02 2018
Response via : Initial Calibration

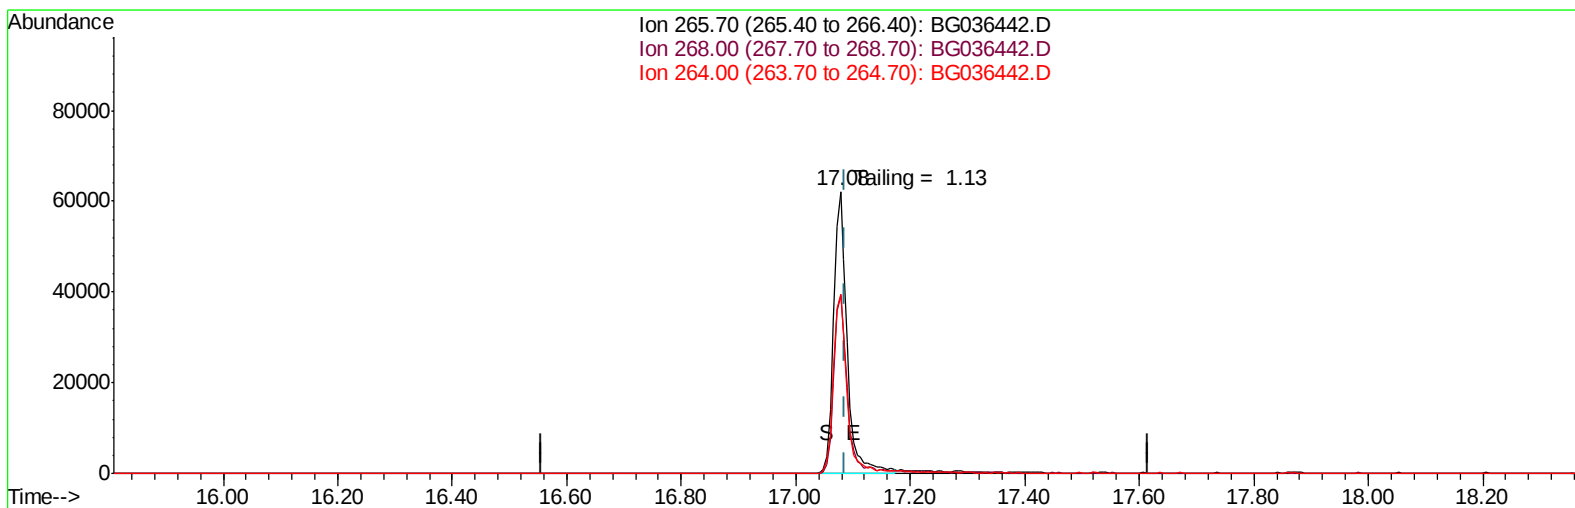

TIC: BG036442.D

(69) Pentachlorophenol (C)




17.078min (-0.009) 28412.32ng

response 101024

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	62.97
264.00	61.10	63.86
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082718\
Data File : BG036442.D
Acq On : 27 Aug 2018 23:14
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 05:55:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 23 12:07:02 2018
Response via : Initial Calibration

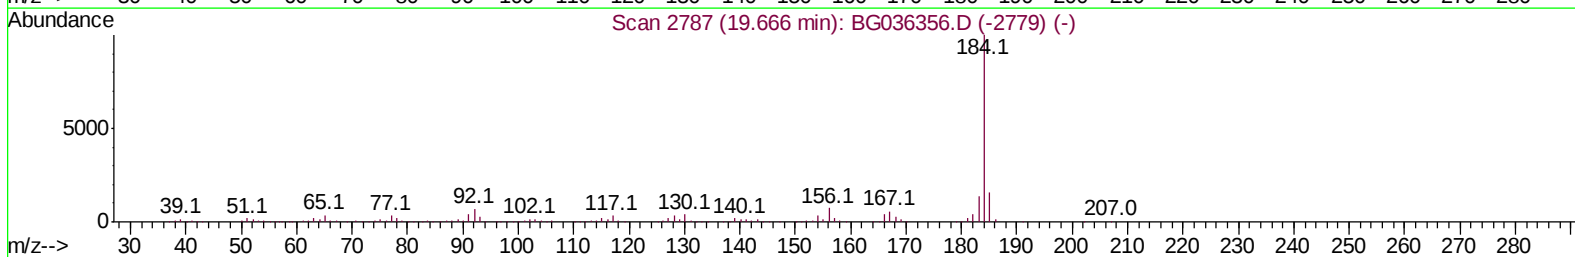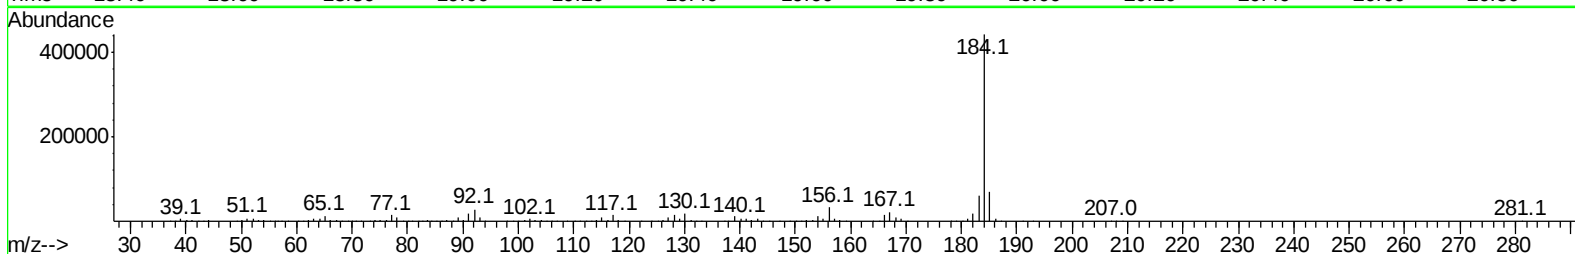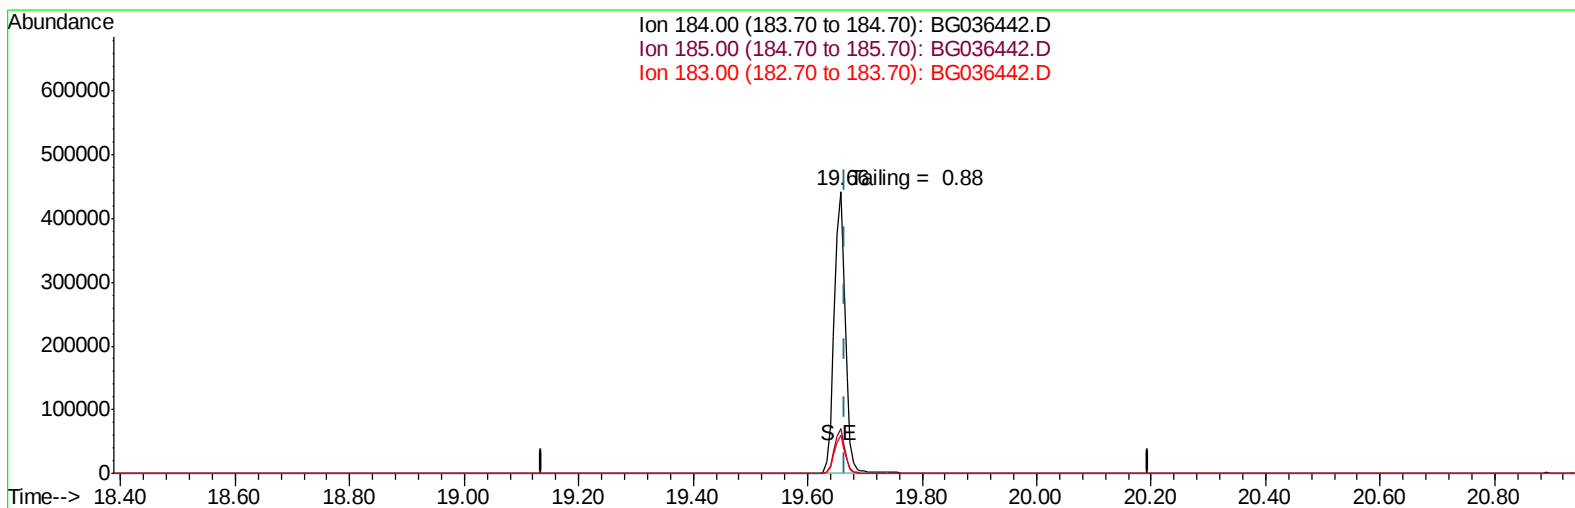

TIC: BG036442.D

(76) Benzidine

19.657min (-0.009) 0.00ng

response 601348

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.74
183.00	13.60	13.48
0.00	0.00	0.00