

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082718\
 Data File : BG036451.D
 Acq On : 28 Aug 2018 5:06
 Operator : JU/SJ
 Sample : J4621-09
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SP-2

Quant Time: Aug 28 07:24:22 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 23 12:07:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	69627	20.00	ng	0.00
21) Naphthalene-d8	10.87	136	283599	20.00	ng	-0.01
38) Acenaphthene-d10	14.69	164	173060	20.00	ng	-0.01
63) Phenanthrene-d10	17.43	188	435308	20.00	ng	0.00
75) Chrysene-d12	21.70	240	456267	20.00	ng	-0.01
86) Perylene-d12	24.91	264	429906	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	419154	95.49	ng	0.00
7) Phenol-d6	7.22	99	513857	81.77	ng	0.00
23) Nitrobenzene-d5	9.22	82	409077	78.26	ng	-0.01
41) 2,4,6-Tribromophenol	16.18	330	249860	121.00	ng	0.00
44) 2-Fluorobiphenyl	13.31	172	943996	77.88	ng	-0.01
78) Terphenyl-d14	20.04	244	1463672	74.98	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082718\
Data File : BG036451.D
Acq On : 28 Aug 2018 5:06
Operator : JU/SJ
Sample : J4621-09
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP-2

Quant Time: Aug 28 07:24:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 23 12:07:02 2018
Response via : Initial Calibration

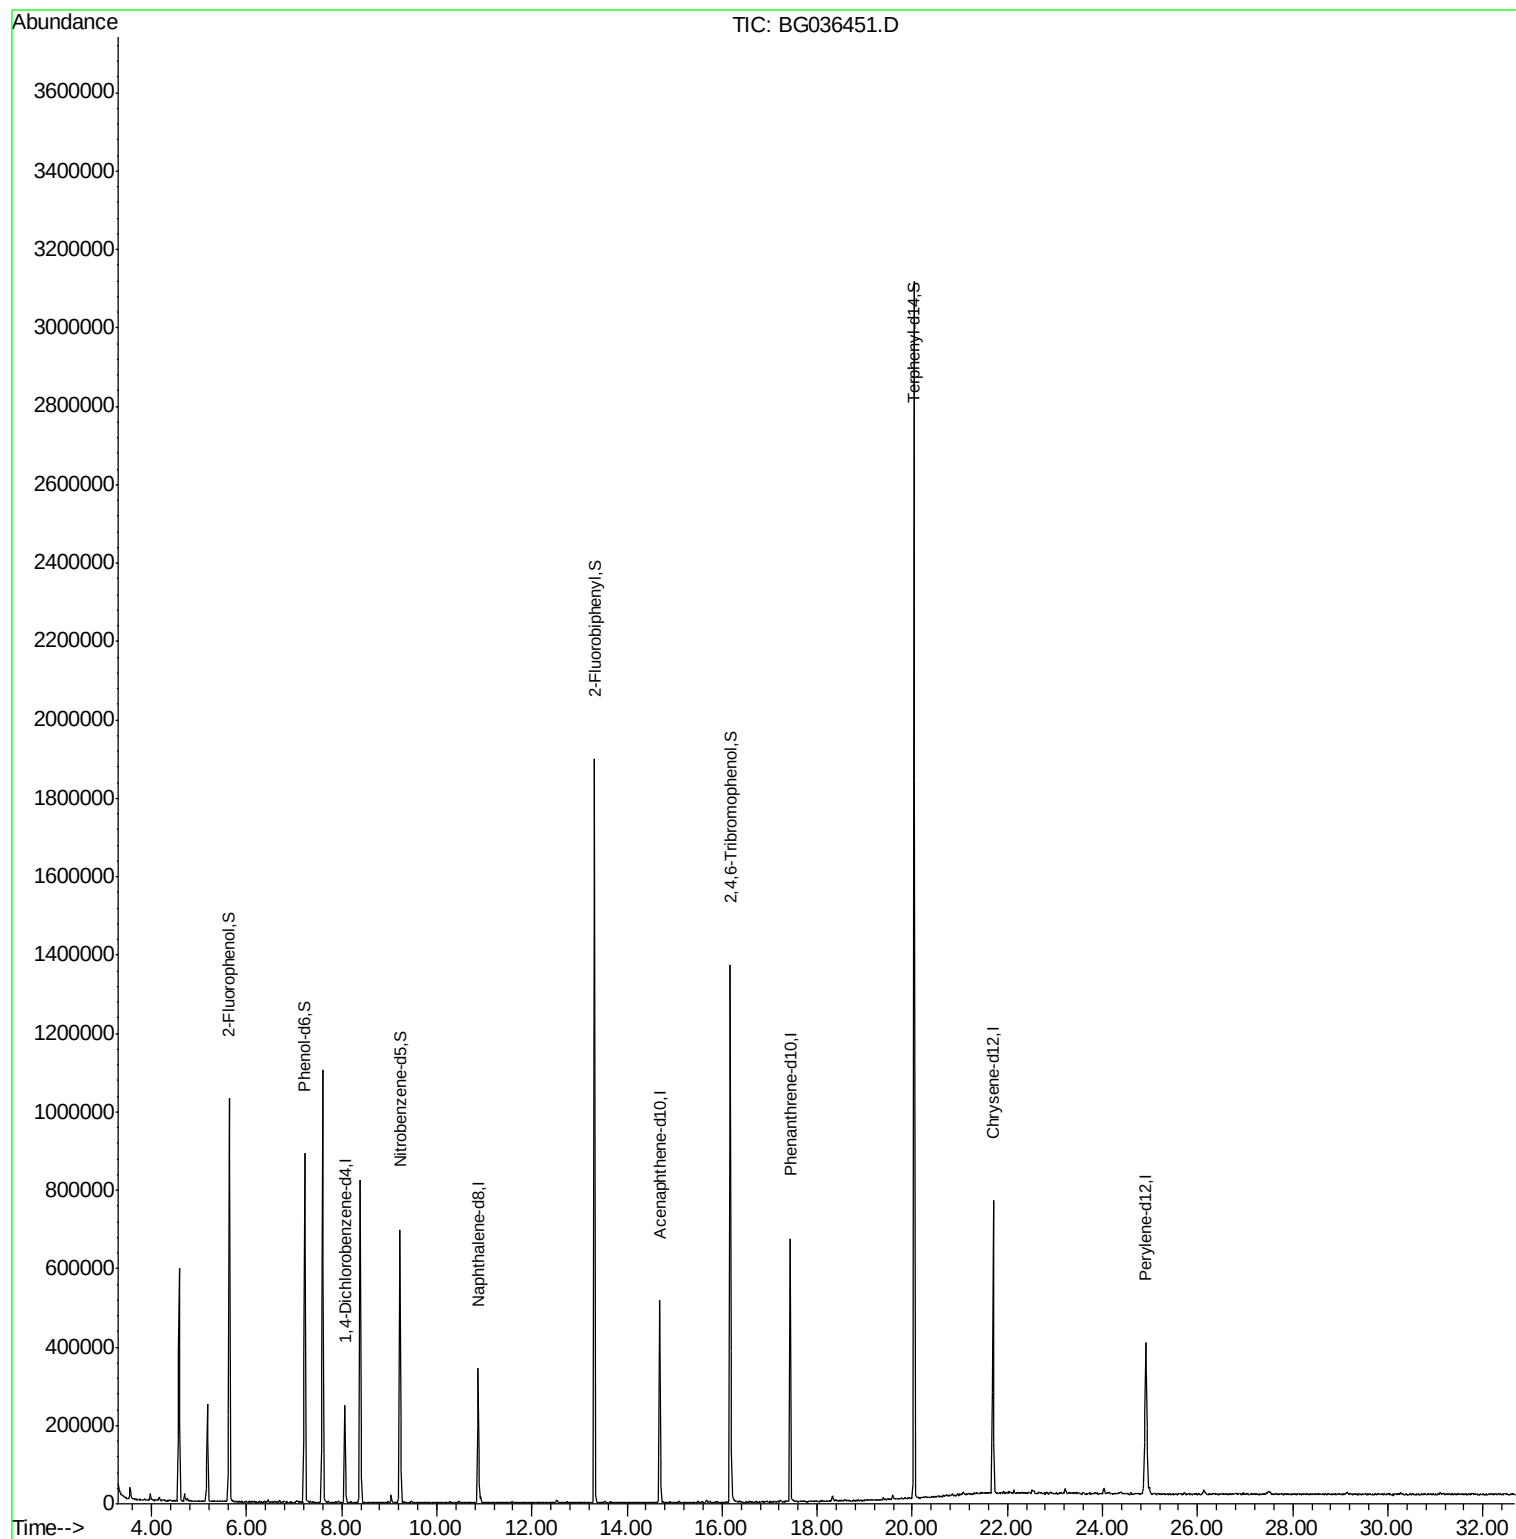

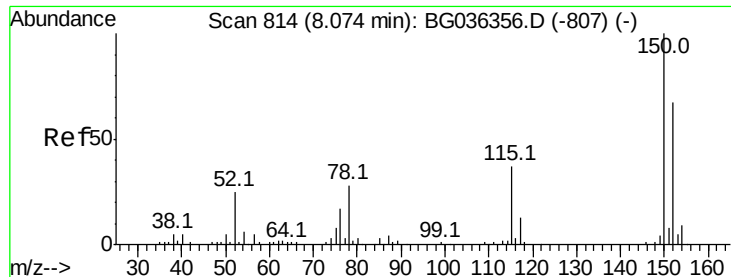


#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.07 min Scan# 813
 Delta R.T. -0.01 min
 Lab File: BG036451.D
 Acq: 28 Aug 2018 5:06

Instrument :
 BNA_G
 ClientSampled :
 SP-2

Tot Ion	Ratio	Lower	Upper
152	100		
150	156.9	119.5	179.3
115	58.4	44.5	66.7



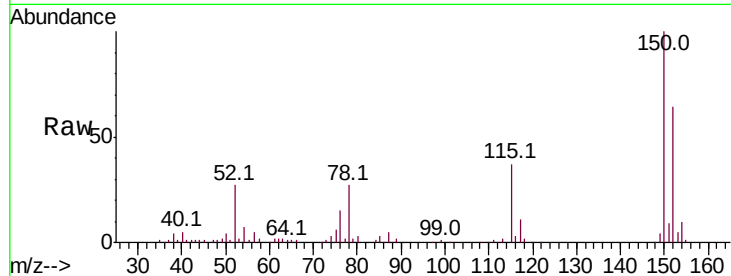


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

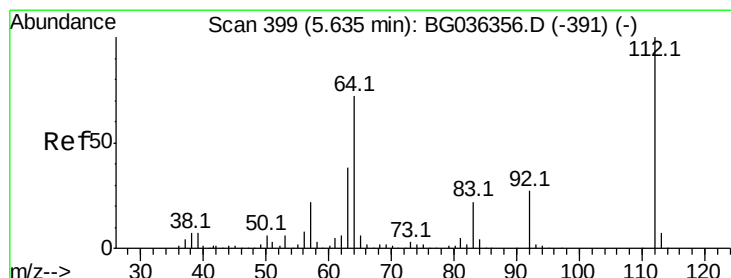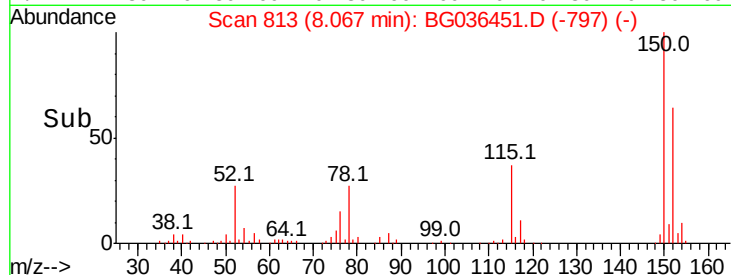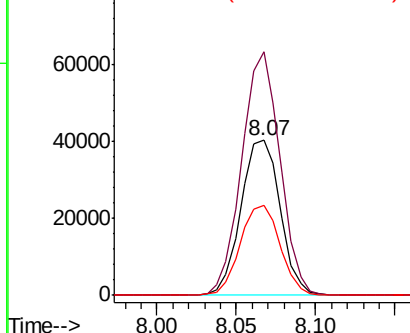

#5

2-Fluorophenol
 Concen: 95.495 ng
 RT: 5.63 min Scan# 399
 Delta R.T. -0.00 min
 Lab File: BG036451.D
 Acq: 28 Aug 2018 5:06

Tgt Ion	Ratio	Lower	Upper
112	100		
64	70.7	57.2	85.8
63	36.0	30.8	46.2


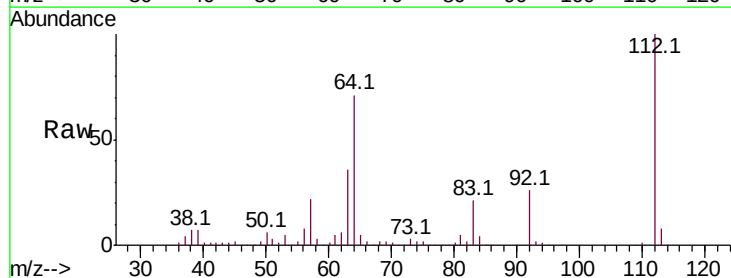



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

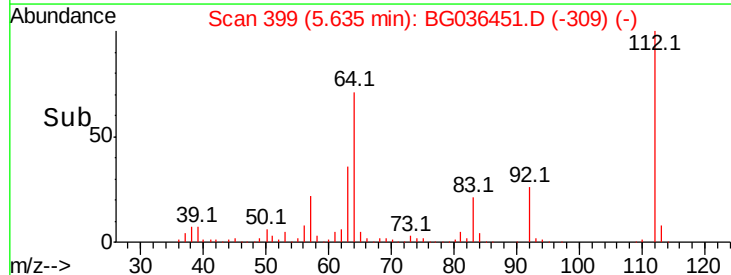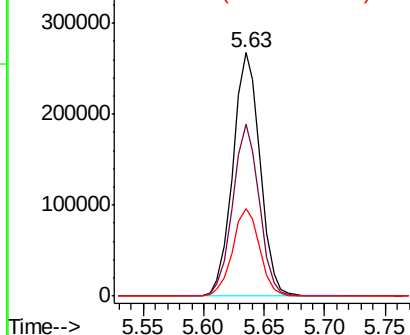

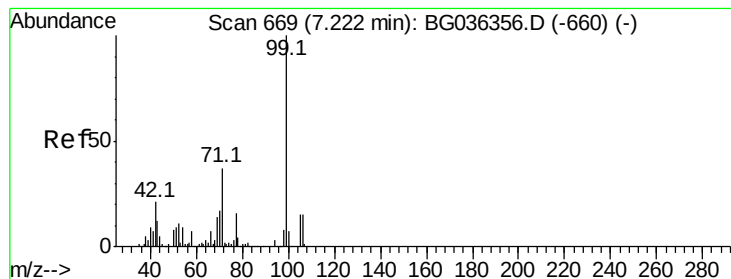

#7

Phenol-d6

Concen: 81.767 ng

RT: 7.22 min Scan# 669

Delta R.T. -0.00 min

Lab File: BG036451.D

Acq: 28 Aug 2018 5:06

Instrument :

BNA_G

ClientSampleId :

SP-2





Tot Ion: 99 Resp: 513857

Ion Ratio Lower Upper

99 100

42 19.5 16.5 24.7

71 35.4 29.4 44.2

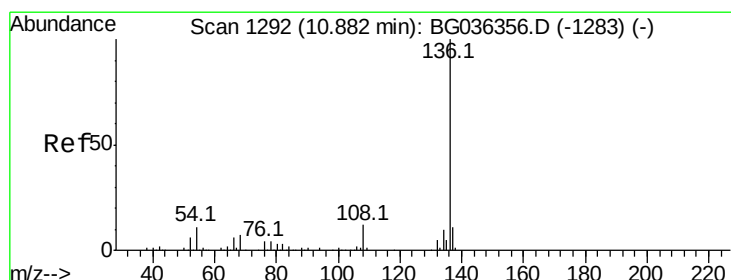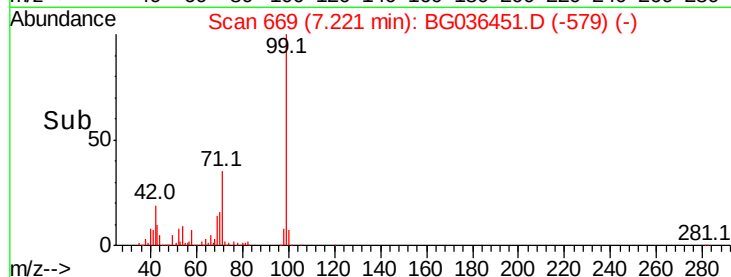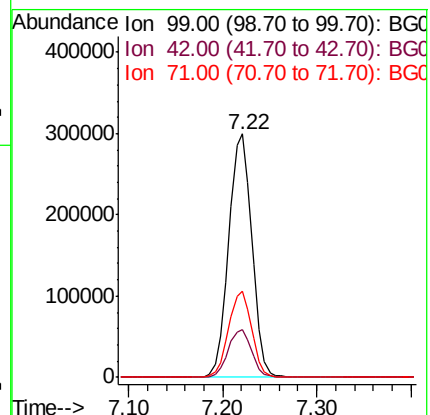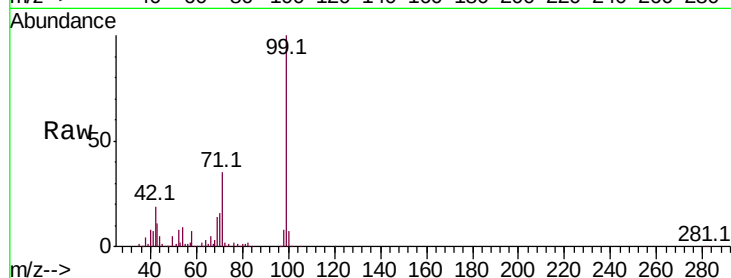

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.87 min Scan# 1290

Delta R.T. -0.01 min

Lab File: BG036451.D

Acq: 28 Aug 2018 5:06

Tgt Ion: 136 Resp: 283599




Ion Ratio Lower Upper


136 100

137 11.2 8.8 13.2

54 10.5 9.2 13.8

68 6.1 5.8 8.6

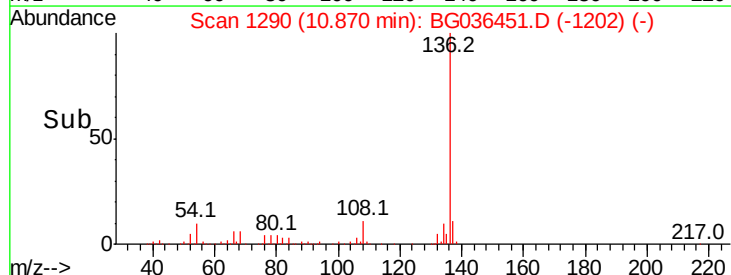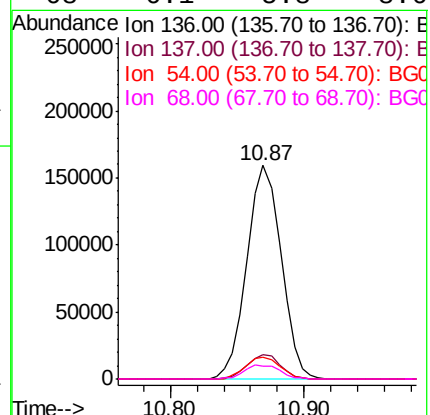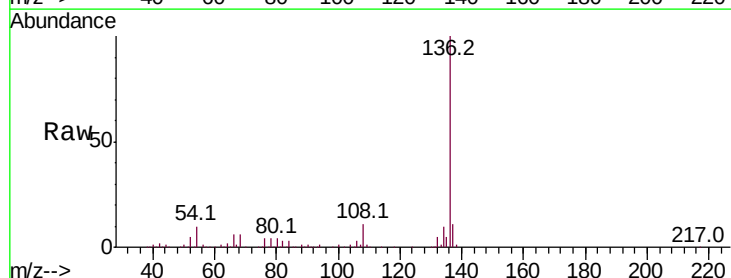

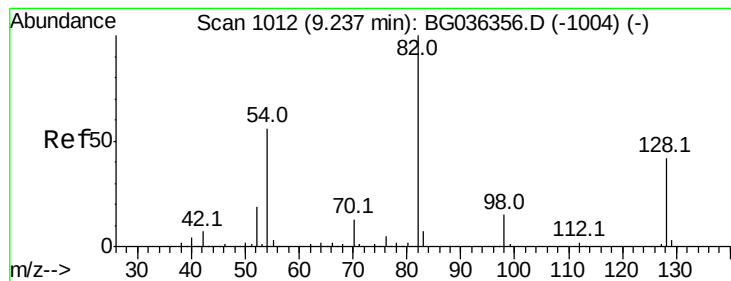

#23

Nitrobenzene-d5

Concen: 78.263 ng

RT: 9.22 min Scan# 1010

Delta R.T. -0.01 min

Lab File: BG036451.D

Acq: 28 Aug 2018 5:06

Instrument :

BNA_G

ClientSampleID :

SP-2





Tot Ion: 82 Resp: 409077

Ion Ratio Lower Upper

82 100

128 42.7 33.3 49.9

54 56.1 45.1 67.7

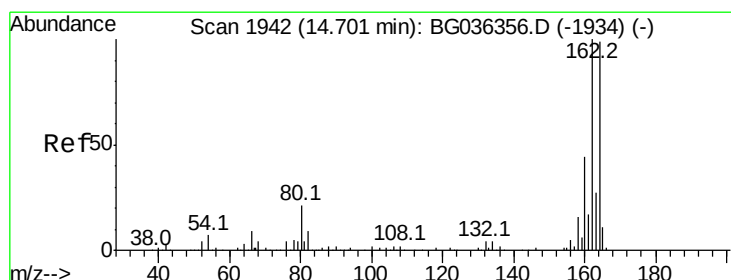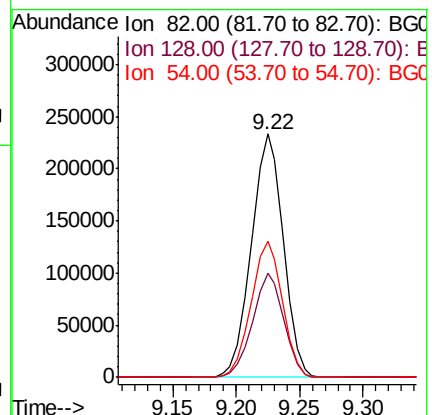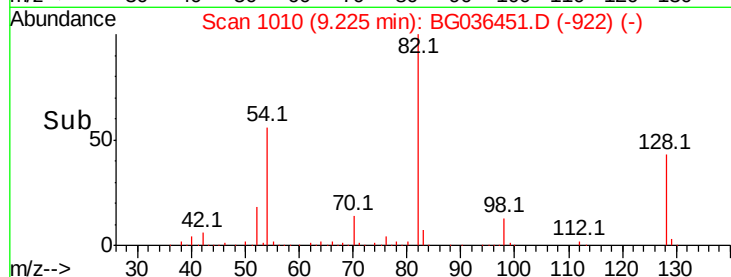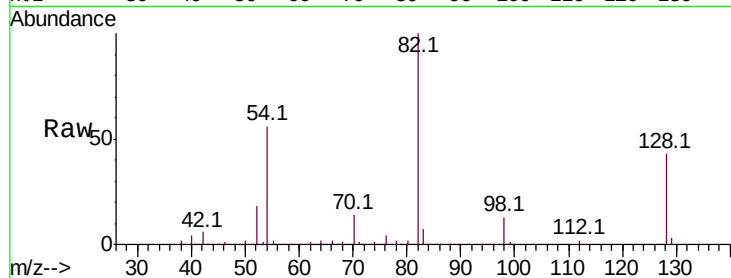

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.69 min Scan# 1940

Delta R.T. -0.01 min

Lab File: BG036451.D

Acq: 28 Aug 2018 5:06




Tgt Ion:164 Resp: 173060


Ion Ratio Lower Upper

164 100

162 108.7 80.7 121.1

160 45.6 35.3 52.9

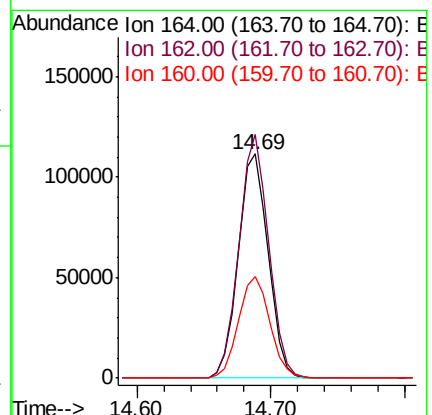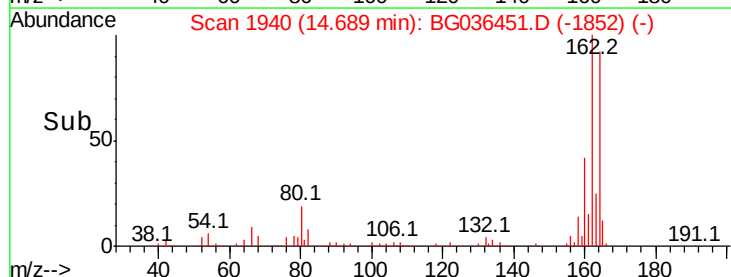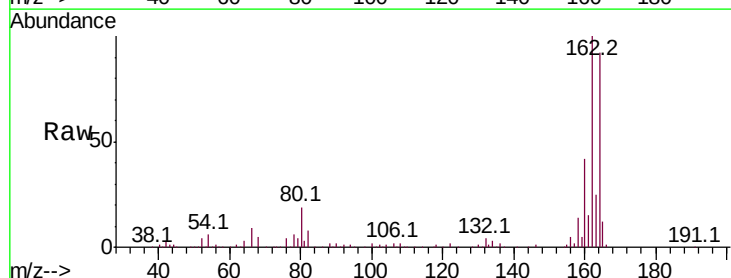


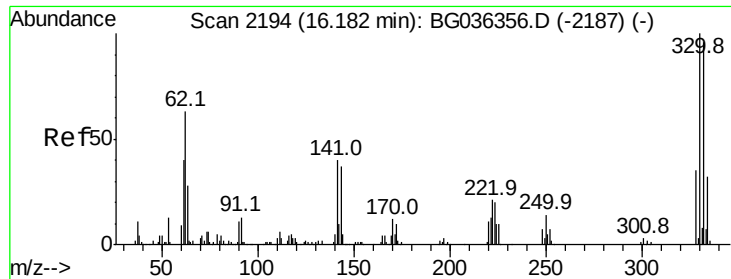




#41
 2,4,6-Tribromophenol
 Concen: 120.998 ng
 RT: 16.18 min Scan# 2193
 Delta R.T. -0.01 min
 Lab File: BG036451.D
 Acq: 28 Aug 2018 5:06

Instrument :
 BNA_G
 ClientSampleId :
 SP-2

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.8	75.4	113.2
141	37.6	30.7	46.1

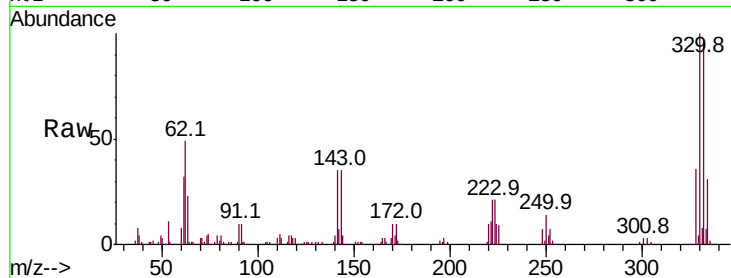


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

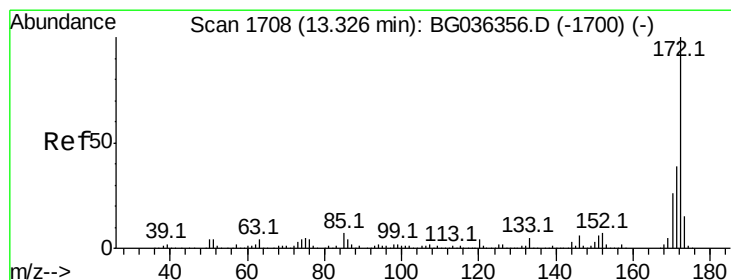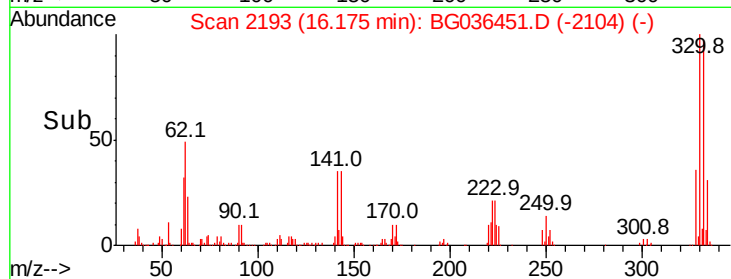
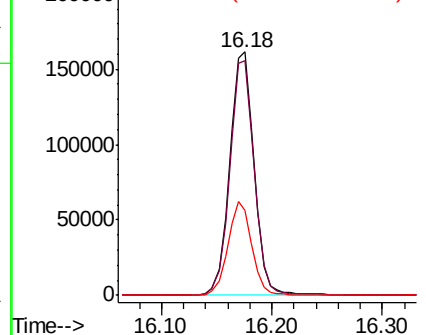



#44
 2-Fluorobiphenyl
 Concen: 77.884 ng
 RT: 13.31 min Scan# 1706
 Delta R.T. -0.01 min
 Lab File: BG036451.D
 Acq: 28 Aug 2018 5:06

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.9	31.3	46.9
170	25.9	21.0	31.6

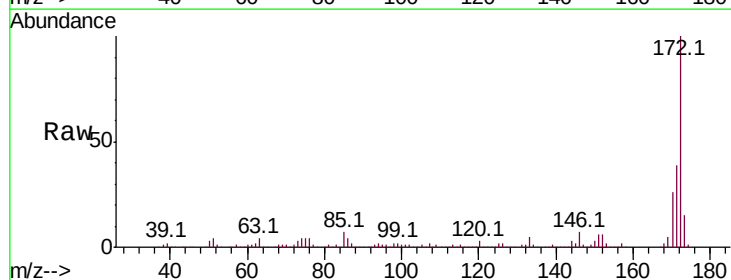

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

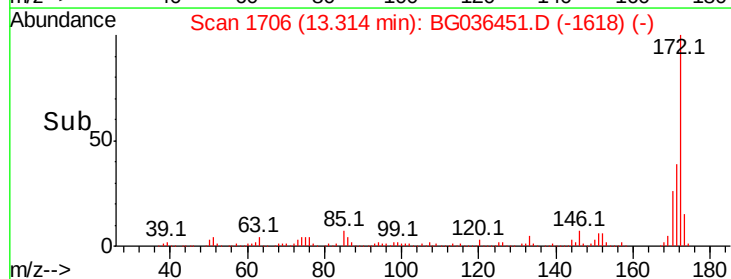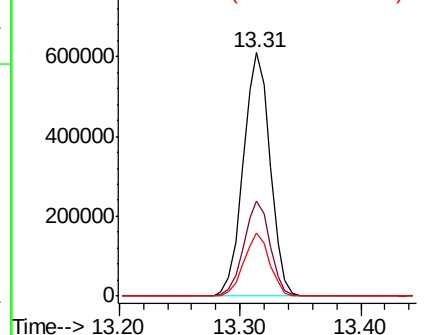


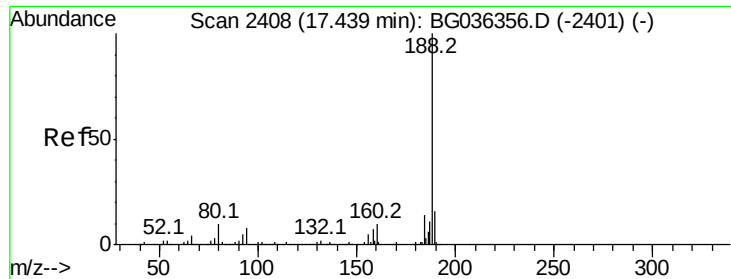




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.43 min Scan# 2407
Delta R.T. -0.01 min
Lab File: BG036451.D
Acq: 28 Aug 2018 5:06

Instrument :
BNA_G
ClientSampleId :
SP-2

Tot Ion:188 Resp: 435308
Ion Ratio Lower Upper
188 100
94 7.1 6.7 10.1
80 8.6 8.1 12.1

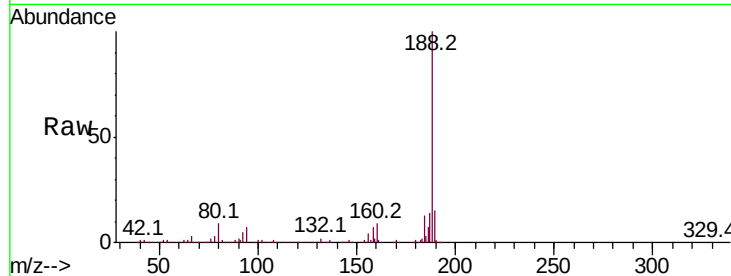


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

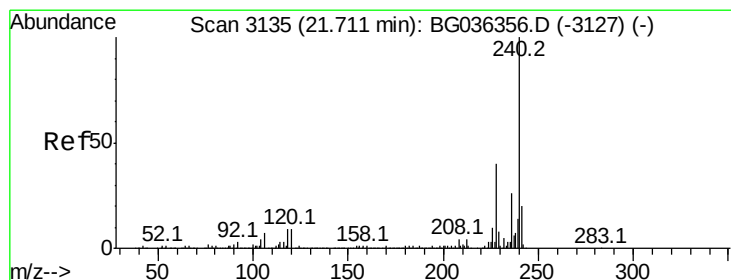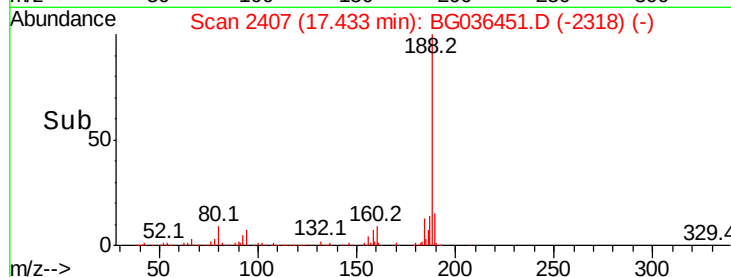
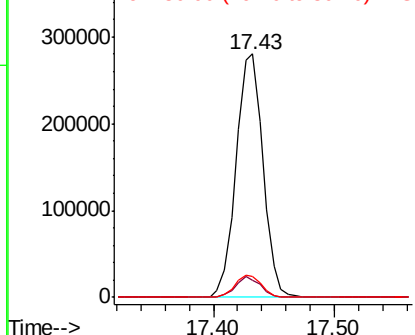



#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.70 min Scan# 3133
Delta R.T. -0.01 min
Lab File: BG036451.D
Acq: 28 Aug 2018 5:06

Tgt Ion:240 Resp: 456267
Ion Ratio Lower Upper
240 100
120 7.5 6.9 10.3
236 25.8 21.2 31.8

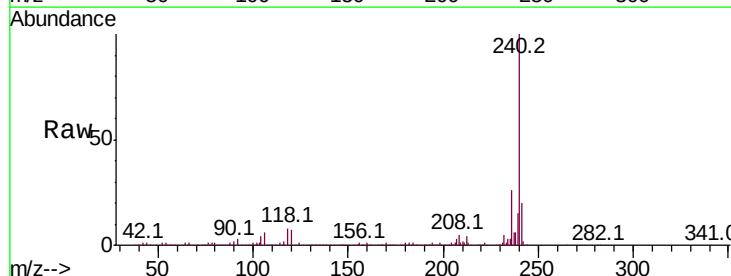

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

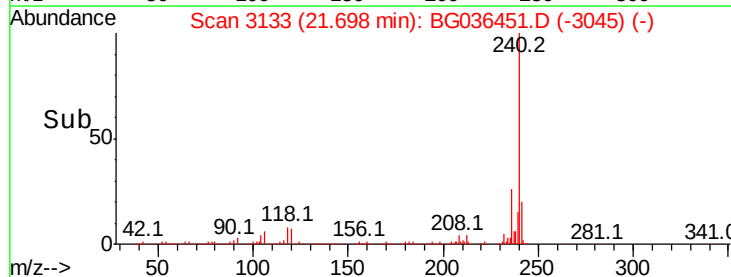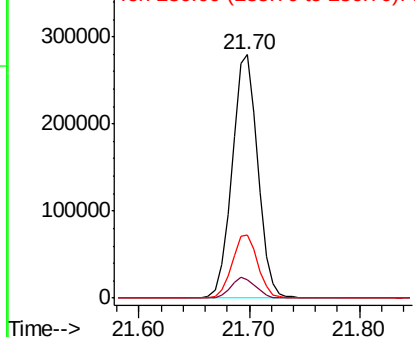

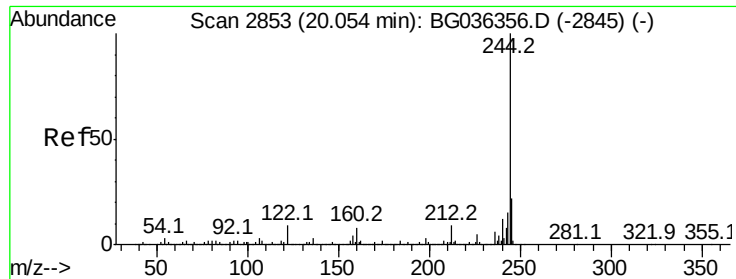

#78

Terphenyl-d14

Concen: 74.980 ng

RT: 20.04 min Scan# 2851

Delta R.T. -0.01 min

Lab File: BG036451.D

Acq: 28 Aug 2018 5:06

Instrument :

BNA_G

ClientSampled :

SP-2


Tot Ion:244 Resp: 1463672

Ion Ratio Lower Upper

244 100

212 8.8 7.0 10.6




122 8.7 7.1 10.7

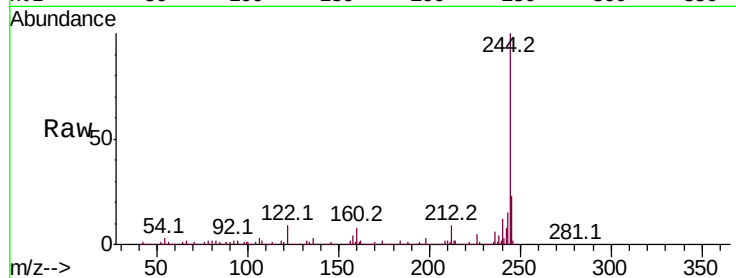

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

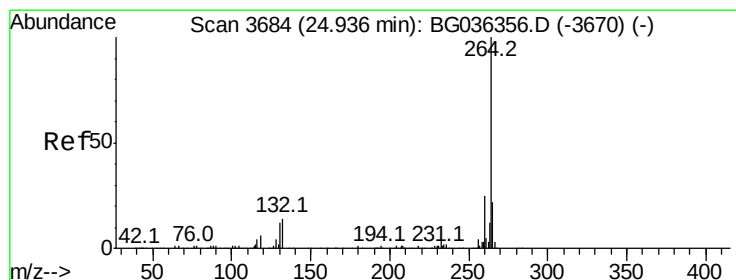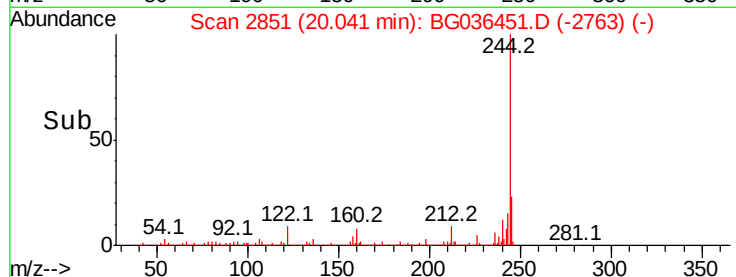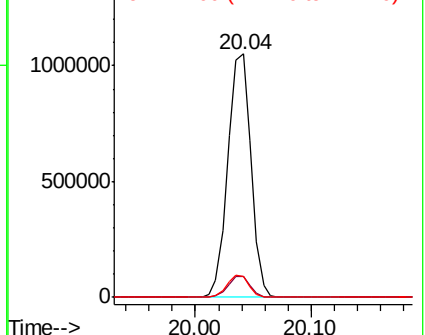

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.91 min Scan# 3680

Delta R.T. -0.02 min

Lab File: BG036451.D

Acq: 28 Aug 2018 5:06


Tgt Ion:264 Resp: 429906

Ion Ratio Lower Upper

264 100

260 24.3 19.6 29.4

265 21.6 17.4 26.0

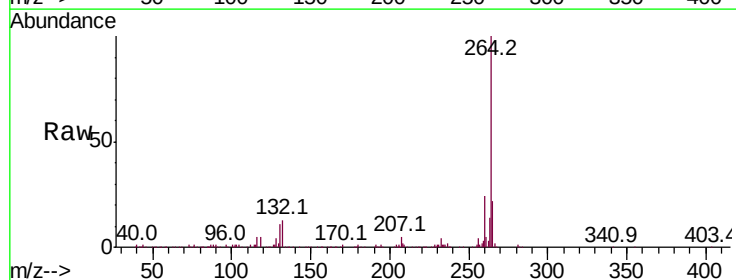

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

