

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG082718\
 Data File : BG036449.D
 Acq On : 28 Aug 2018 3:47
 Operator : JU/SJ
 Sample : J4614-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DSN-001A-082218

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.543	39	43	50	rVB	33542	51680	1.28%	0.218%
2	5.171	315	320	326	rVB2	30860	47602	1.18%	0.200%
3	5.576	381	389	394	rBV	232669	368527	9.15%	1.552%
4	5.635	394	399	405	rVV	485539	773064	19.19%	3.255%
5	5.706	405	411	423	rVB	663592	1432638	35.56%	6.033%
6	6.076	467	474	482	rBV	399473	650315	16.14%	2.738%
7	7.216	661	668	677	rVB	310488	538399	13.36%	2.267%
8	7.597	722	733	741	rBV	923185	1583301	39.30%	6.667%
9	8.067	804	813	819	rBV	232986	398550	9.89%	1.678%
10	8.391	860	868	874	rBV	827769	1434088	35.60%	6.039%
11	9.225	1002	1010	1020	rVB	723975	1265754	31.42%	5.330%
12	9.912	1119	1127	1138	rBV7	21702	55066	1.37%	0.232%
13	10.047	1144	1150	1160	rBV6	18889	53460	1.33%	0.225%
14	10.870	1281	1290	1295	rBV	317064	578499	14.36%	2.436%
15	10.923	1295	1299	1306	rVB	159926	262598	6.52%	1.106%
16	11.516	1389	1400	1406	rBV2	26493	54487	1.35%	0.229%
17	12.521	1563	1571	1578	rBV	31049	53865	1.34%	0.227%
18	12.738	1600	1608	1615	rVB2	25948	47360	1.18%	0.199%
19	13.314	1699	1706	1713	rBV	1910799	2891353	71.77%	12.175%
20	14.137	1841	1846	1851	rVB	115081	166033	4.12%	0.699%
21	14.689	1933	1940	1946	rBV2	481197	783808	19.46%	3.301%
22	14.754	1946	1951	1956	rVB	63402	97157	2.41%	0.409%
23	15.083	2001	2007	2013	rBV	26030	41981	1.04%	0.177%
24	15.664	2101	2106	2113	rVV	50311	79901	1.98%	0.336%
25	15.729	2113	2117	2124	rVB	29838	44949	1.12%	0.189%
26	16.170	2185	2192	2210	rVB	1383856	2216949	55.03%	9.335%
27	16.393	2226	2230	2240	rVB4	22439	44053	1.09%	0.186%
28	17.433	2400	2407	2412	rBV	628542	977266	24.26%	4.115%
29	17.827	2466	2474	2480	rBV2	30946	60737	1.51%	0.256%
30	18.320	2554	2558	2565	rBV2	60277	94807	2.35%	0.399%
31	18.837	2641	2646	2655	rVB4	26277	49403	1.23%	0.208%
32	19.854	2814	2819	2827	rBV2	39299	76646	1.90%	0.323%
33	20.036	2844	2850	2858	rBV	3026815	4028782	100.00%	16.965%
34	20.823	2980	2984	2987	rBV2	34924	47388	1.18%	0.200%

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG082718\
Data File : BG036449.D
Acq On : 28 Aug 2018 3:47
Operator : JU/SJ
Sample : J4614-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DSN-001A-082218

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	21.352	3071	3074	3083	rBV6	28423	61666	1.53%	0.260%
36	21.693	3126	3132	3140	rVB	714575	1146656	28.46%	4.828%
37	24.031	3525	3530	3536	rVB4	25335	52353	1.30%	0.220%
38	24.912	3667	3680	3689	rBV2	393947	1136823	28.22%	4.787%


Sum of corrected areas: 23747964

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG082718\
Data File : BG036449.D
Acq On : 28 Aug 2018 3:47
Operator : JU/SJ
Sample : J4614-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DSN-001A-082218

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

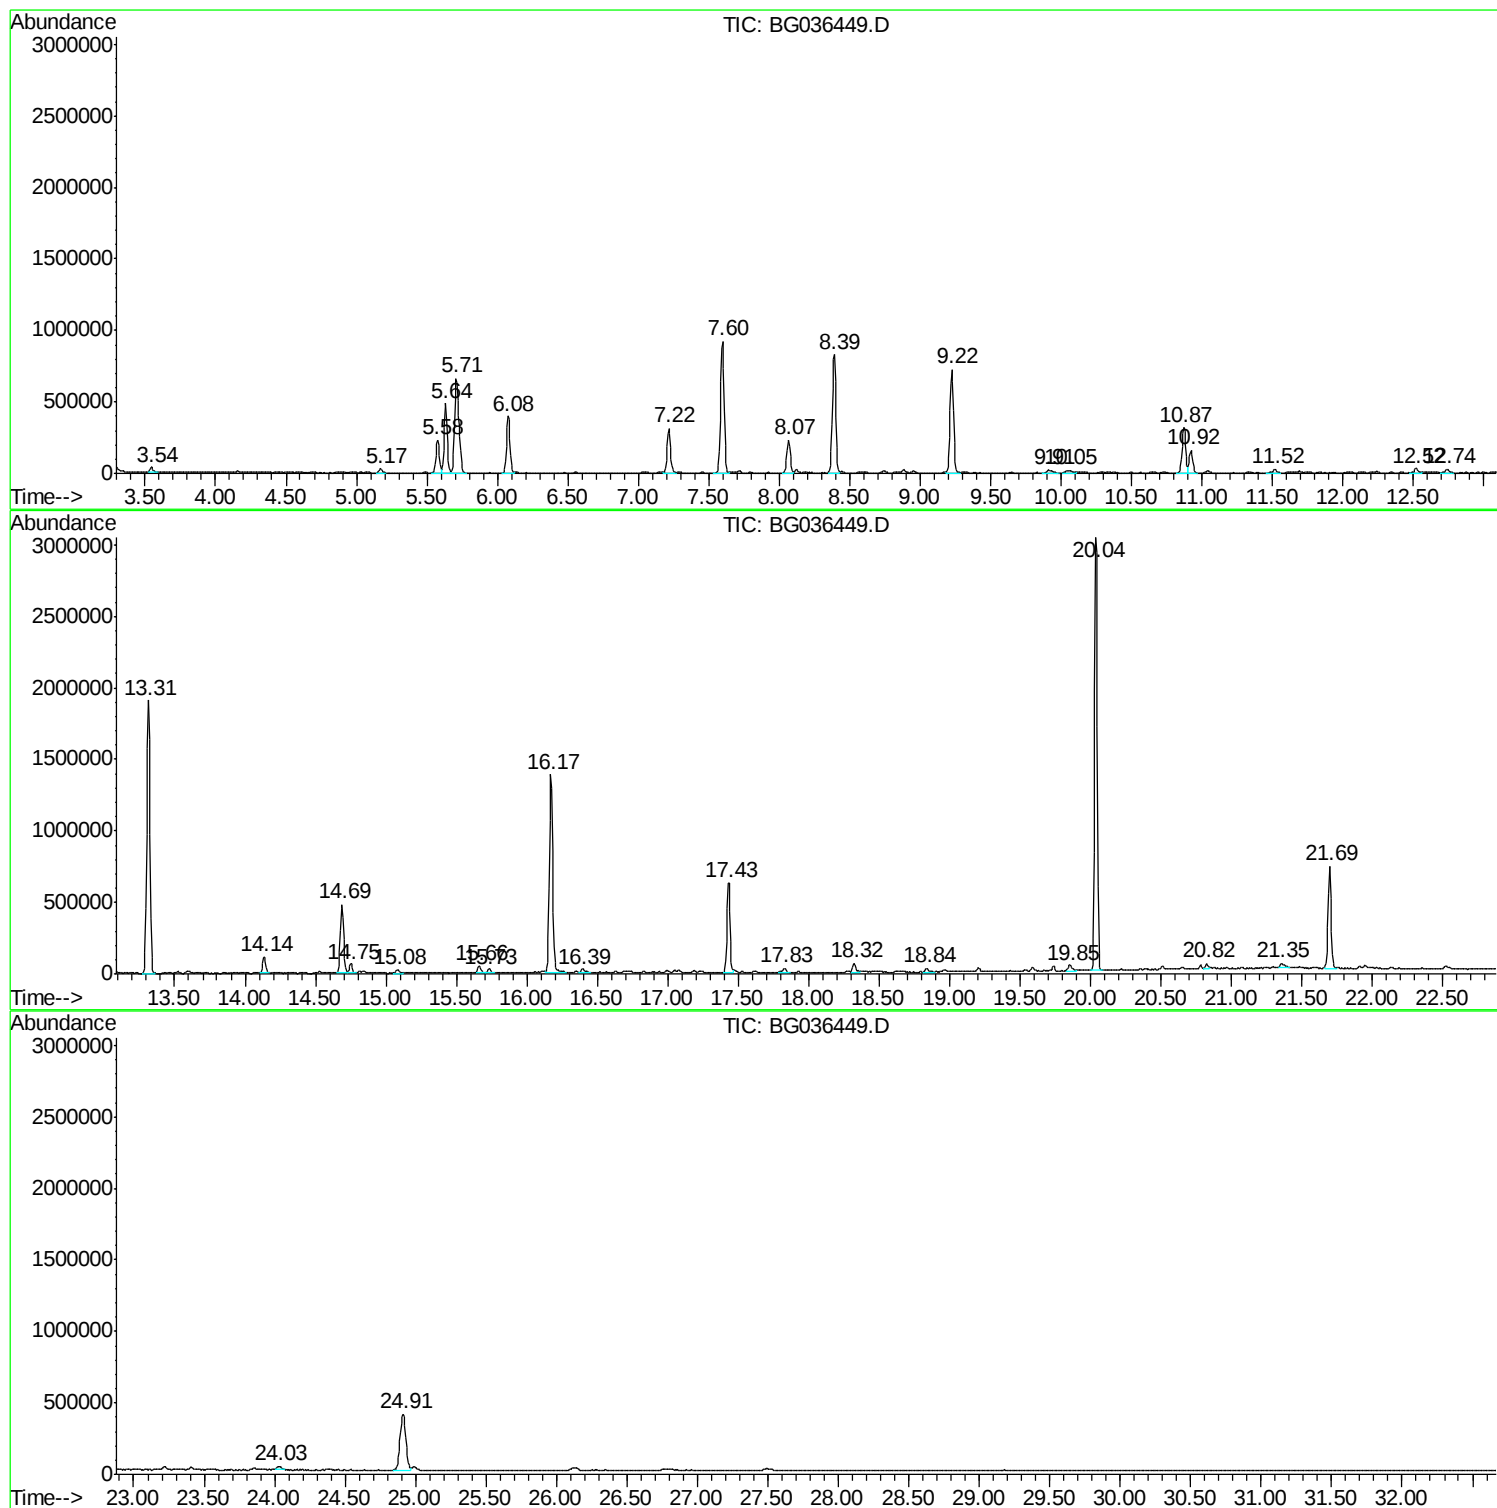

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082718\
Data File : BG036449.D
Acq On : 28 Aug 2018 3:47
Operator : JU/SJ
Sample : J4614-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DSN-001A-082218

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082718\
Data File : BG036449.D
Acq On : 28 Aug 2018 3:47
Operator : JU/SJ
Sample : J4614-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DSN-001A-082218

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc