


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082718\
 Data File : BG036423.D
 Acq On : 27 Aug 2018 9:35
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 23 12:07:02 2018

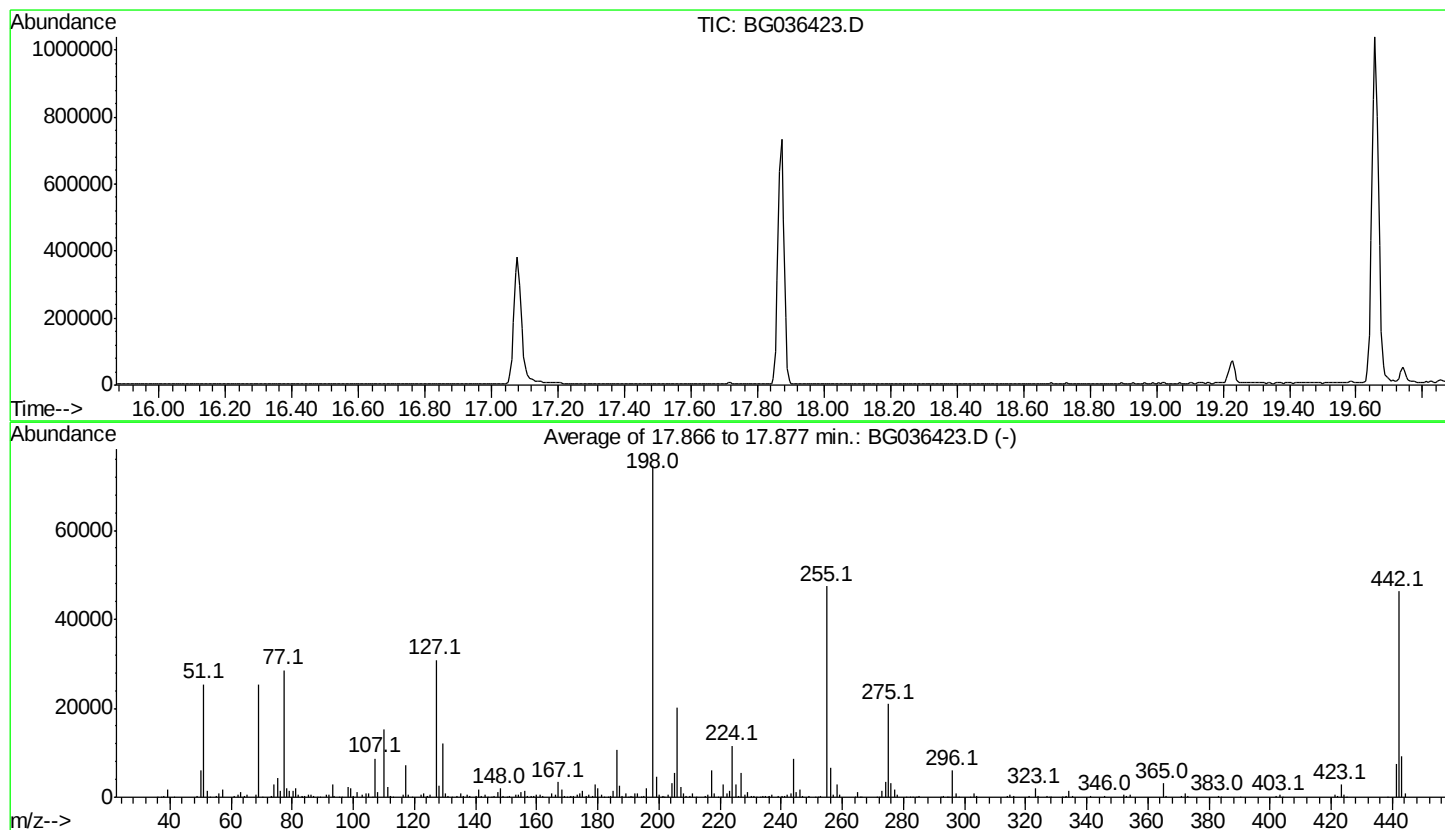

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	25426	PASS
68	69	0.00	2	2.0	514	PASS
69	198	0.00	100	34.1	25402	PASS
70	69	0.00	2	0.4	110	PASS
127	198	10	80	41.5	30946	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	74554	PASS
199	198	5	9	6.3	4697	PASS
275	198	10	60	28.1	20928	PASS
365	198	1	100	4.1	3040	PASS
441	198	0.01	100	10.1	7512	PASS
442	198	50	100	62.1	46314	PASS
443	442	15	24	20.1	9329	PASS