


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG082718\
 Data File : BG036442.D
 Acq On : 27 Aug 2018 23:14
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 23 12:07:02 2018

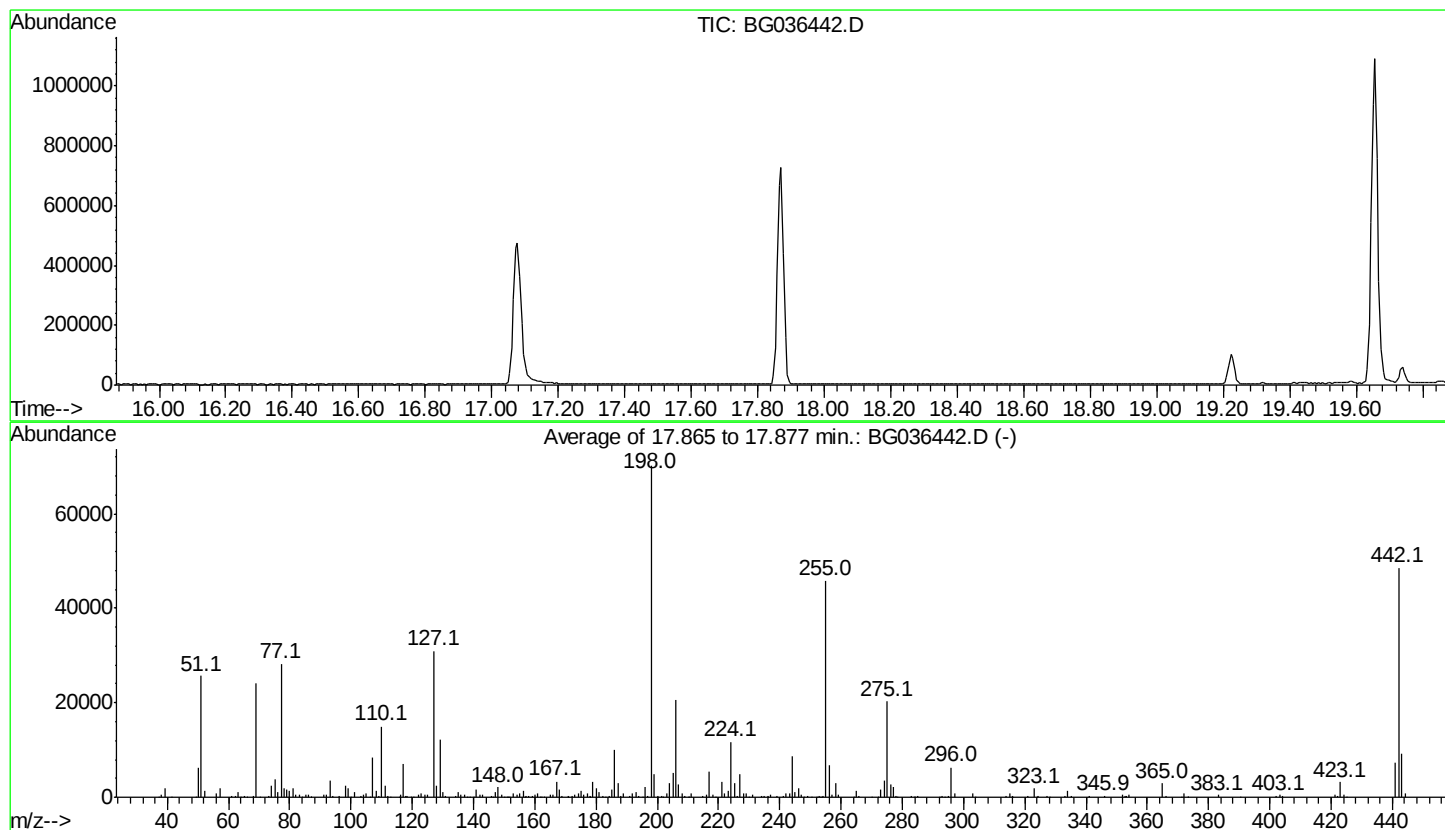

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	25625	PASS
68	69	0.00	2	0.7	178	PASS
69	198	0.00	100	34.3	24105	PASS
70	69	0.00	2	0.5	110	PASS
127	198	10	80	44.1	30928	PASS
197	198	0.00	2	0.2	154	PASS
198	198	100	100	100.0	70192	PASS
199	198	5	9	6.8	4778	PASS
275	198	10	60	28.8	20205	PASS
365	198	1	100	4.2	2980	PASS
441	198	0.01	100	10.4	7302	PASS
442	198	50	100	69.2	48600	PASS
443	442	15	24	18.9	9187	PASS