

Data Path : Z:\HPCHEM1\BNA G\DATA\BG082815\
 Data File : BG018515.D
 Acq On : 28 Aug 2015 16:32
 Operator : UM/MA
 Sample : PB85238BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Aug 31 01:55:36 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 31 01:58:19 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	56395	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	257141	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	171564	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.38	188	439182	20.00	ng/ul	0.00
78) Chrysene-d12	21.64	240	459796	20.00	ng/ul	-0.01
86) Perylene-d12	24.83	264	450510	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.44	96	9480	7.43	ng/uL	0.00
5) Phenol-d5	7.17	99	190884	37.29	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.34	67	126645	39.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	145215	37.04	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	162824	37.86	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	83308	41.56	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	79455	38.92	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	159353	36.78	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	238079	48.62	ng/ul	0.00
44) Dimethylphthalate-d6	14.04	166	572458	39.66	ng/ul	0.00
47) Acenaphthylene-d8	14.33	160	698033	38.40	ng/ul	0.00
52) 4-Nitrophenol-d4	14.82	143	100127	38.56	ng/ul	0.00
58) Fluorene-d10	15.63	176	501545	39.89	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.74	200	55886	25.87	ng/ul	0.00
71) Anthracene-d10	17.48	188	838637	39.93	ng/ul	0.00
79) Pyrene-d10	19.76	212	934849	39.19	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.62	264	979540	40.96	ng/ul	0.00

Target Compounds


					Ovalue
15) N-Nitroso-di-n-propylamine	8.71	70	3706	1.04	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG082815\
Data File : BG018515.D
Acq On : 28 Aug 2015 16:32
Operator : UM/MA
Sample : PB85238BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Aug 31 01:55:36 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 31 01:58:19 2015
Response via : Initial Calibration

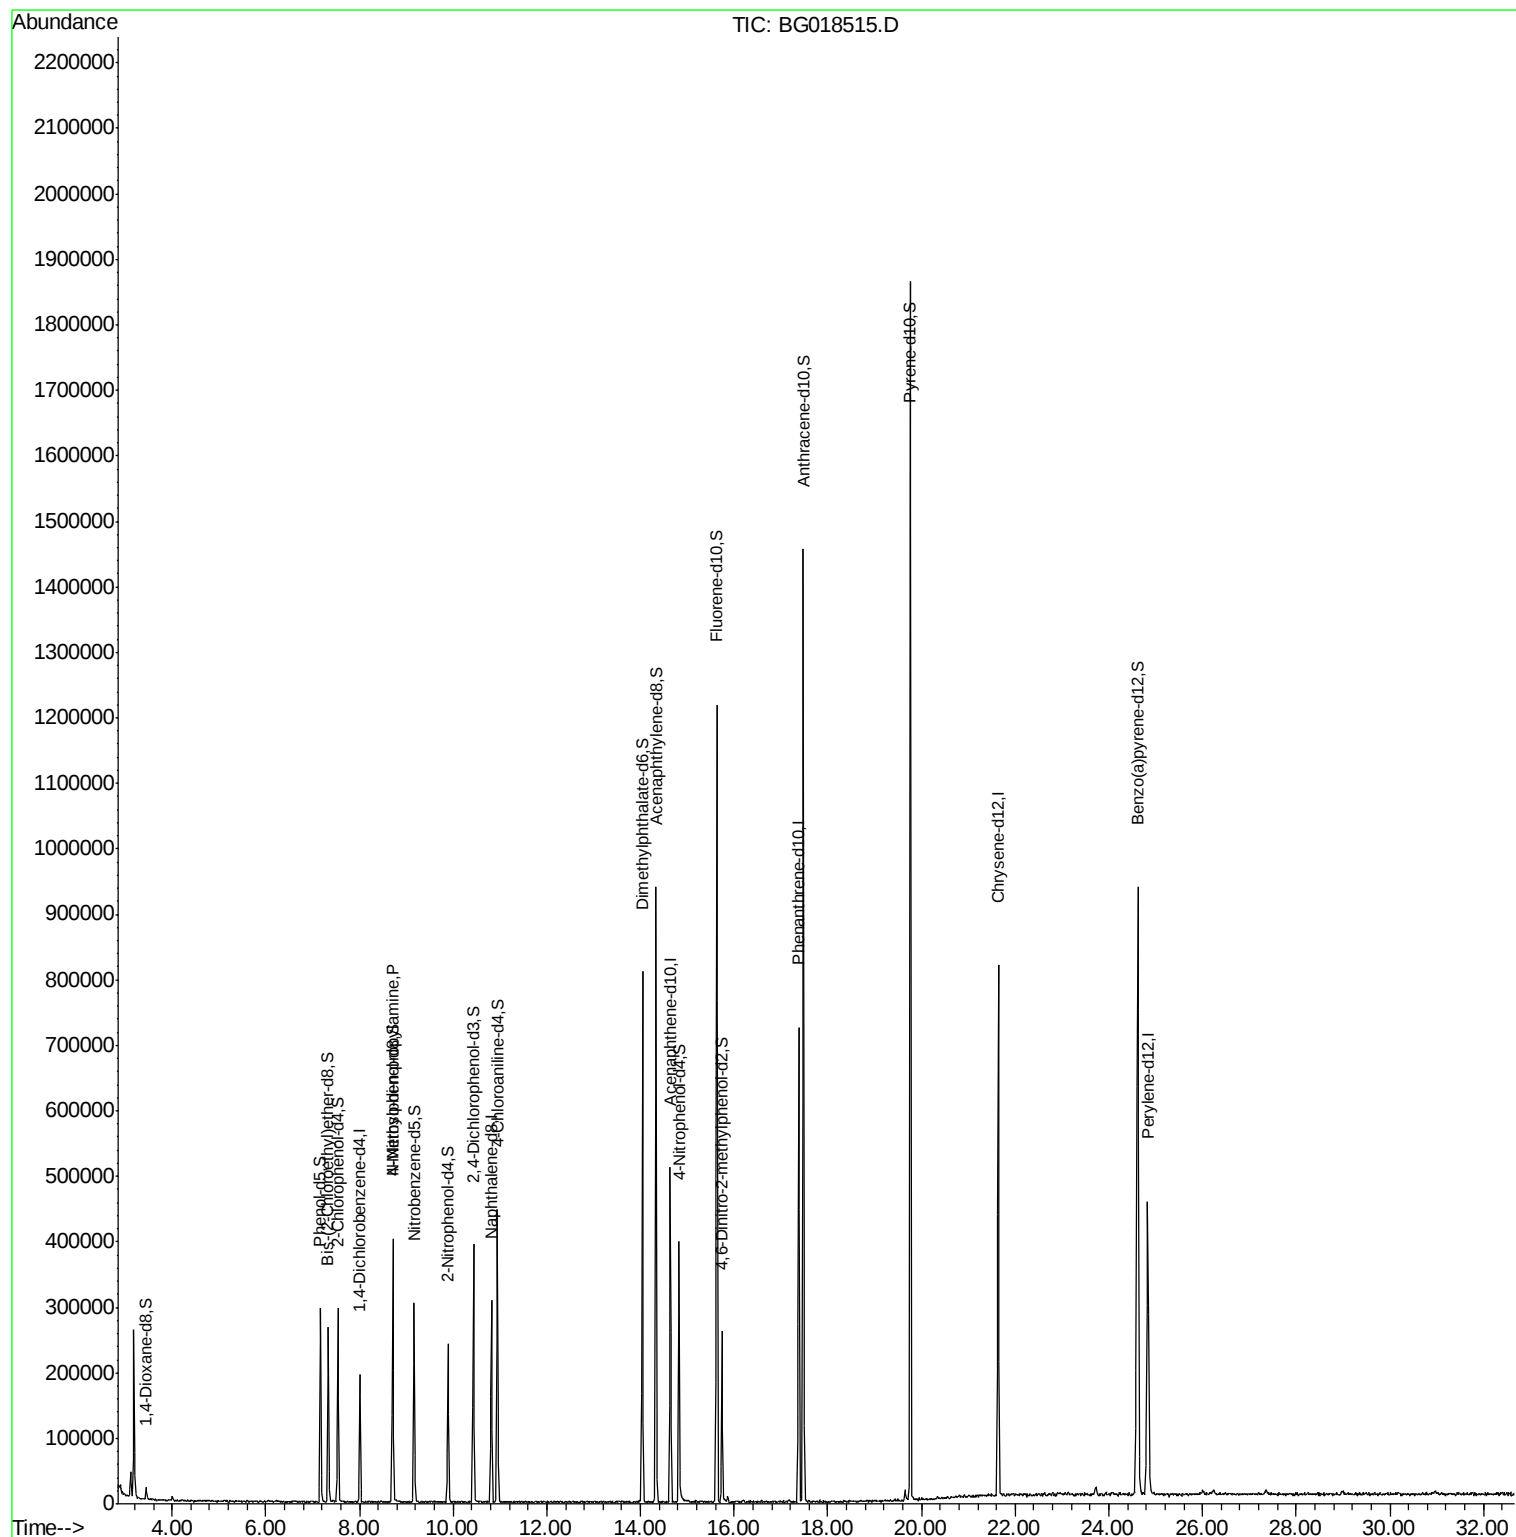

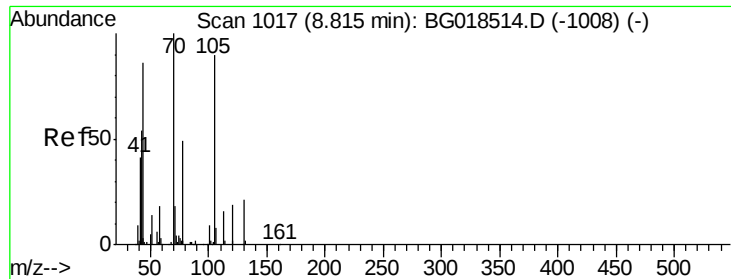

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.04 ng/ul
 RT: 8.71 min Scan# 999
 Delta R.T. -0.10 min
 Lab File: BG018515.D
 Acq: 28 Aug 2015 16:32

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion: 70 Resp: 3706
 Ion Ratio Lower Upper
 70 100
 42 403.0 50.7 76.1#
 101 0.0 7.4 11.2#
 130 0.0 15.8 23.6#

