

Data Path : Z:\HPCHEM1\BNA G\DATA\BG082815\
 Data File : BG018523.D
 Acq On : 28 Aug 2015 21:37
 Operator : UM/MA
 Sample : G3448-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Aug 31 03:27:33 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 31 03:29:45 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	61965	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	283947	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	193600	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.38	188	509839	20.00	ng/ul	0.00
78) Chrysene-d12	21.64	240	535195	20.00	ng/ul	0.00
86) Perylene-d12	24.83	264	519723	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.45	96	3762	2.68	ng/uL	0.00
5) Phenol-d5	7.16	99	155870	27.71	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.34	67	101369	29.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	115946	26.92	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	113619	24.04	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	68338	30.87	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	66941	29.69	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	135193	28.26	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	122486	22.65	ng/ul	0.00
44) Dimethylphthalate-d6	14.04	166	511278	31.39	ng/ul	0.00
47) Acenaphthylene-d8	14.33	160	624891	30.47	ng/ul	0.00
52) 4-Nitrophenol-d4	14.82	143	95569	32.62	ng/ul	0.00
58) Fluorene-d10	15.63	176	464455	32.74	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.74	200	59717	23.81	ng/ul	0.00
71) Anthracene-d10	17.48	188	769321	31.55	ng/ul	0.00
79) Pyrene-d10	19.76	212	863470	31.10	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.61	264	859444	31.15	ng/ul	0.00


Target Compounds						Ovalue
32) Caprolactam	11.69	113	1828	1.01	ng/ul	84
45) Dimethylphthalate	14.09	163	247326	15.39	ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG082815\
Data File : BG018523.D
Acq On : 28 Aug 2015 21:37
Operator : UM/MA
Sample : G3448-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Aug 31 03:27:33 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 31 03:29:45 2015
Response via : Initial Calibration




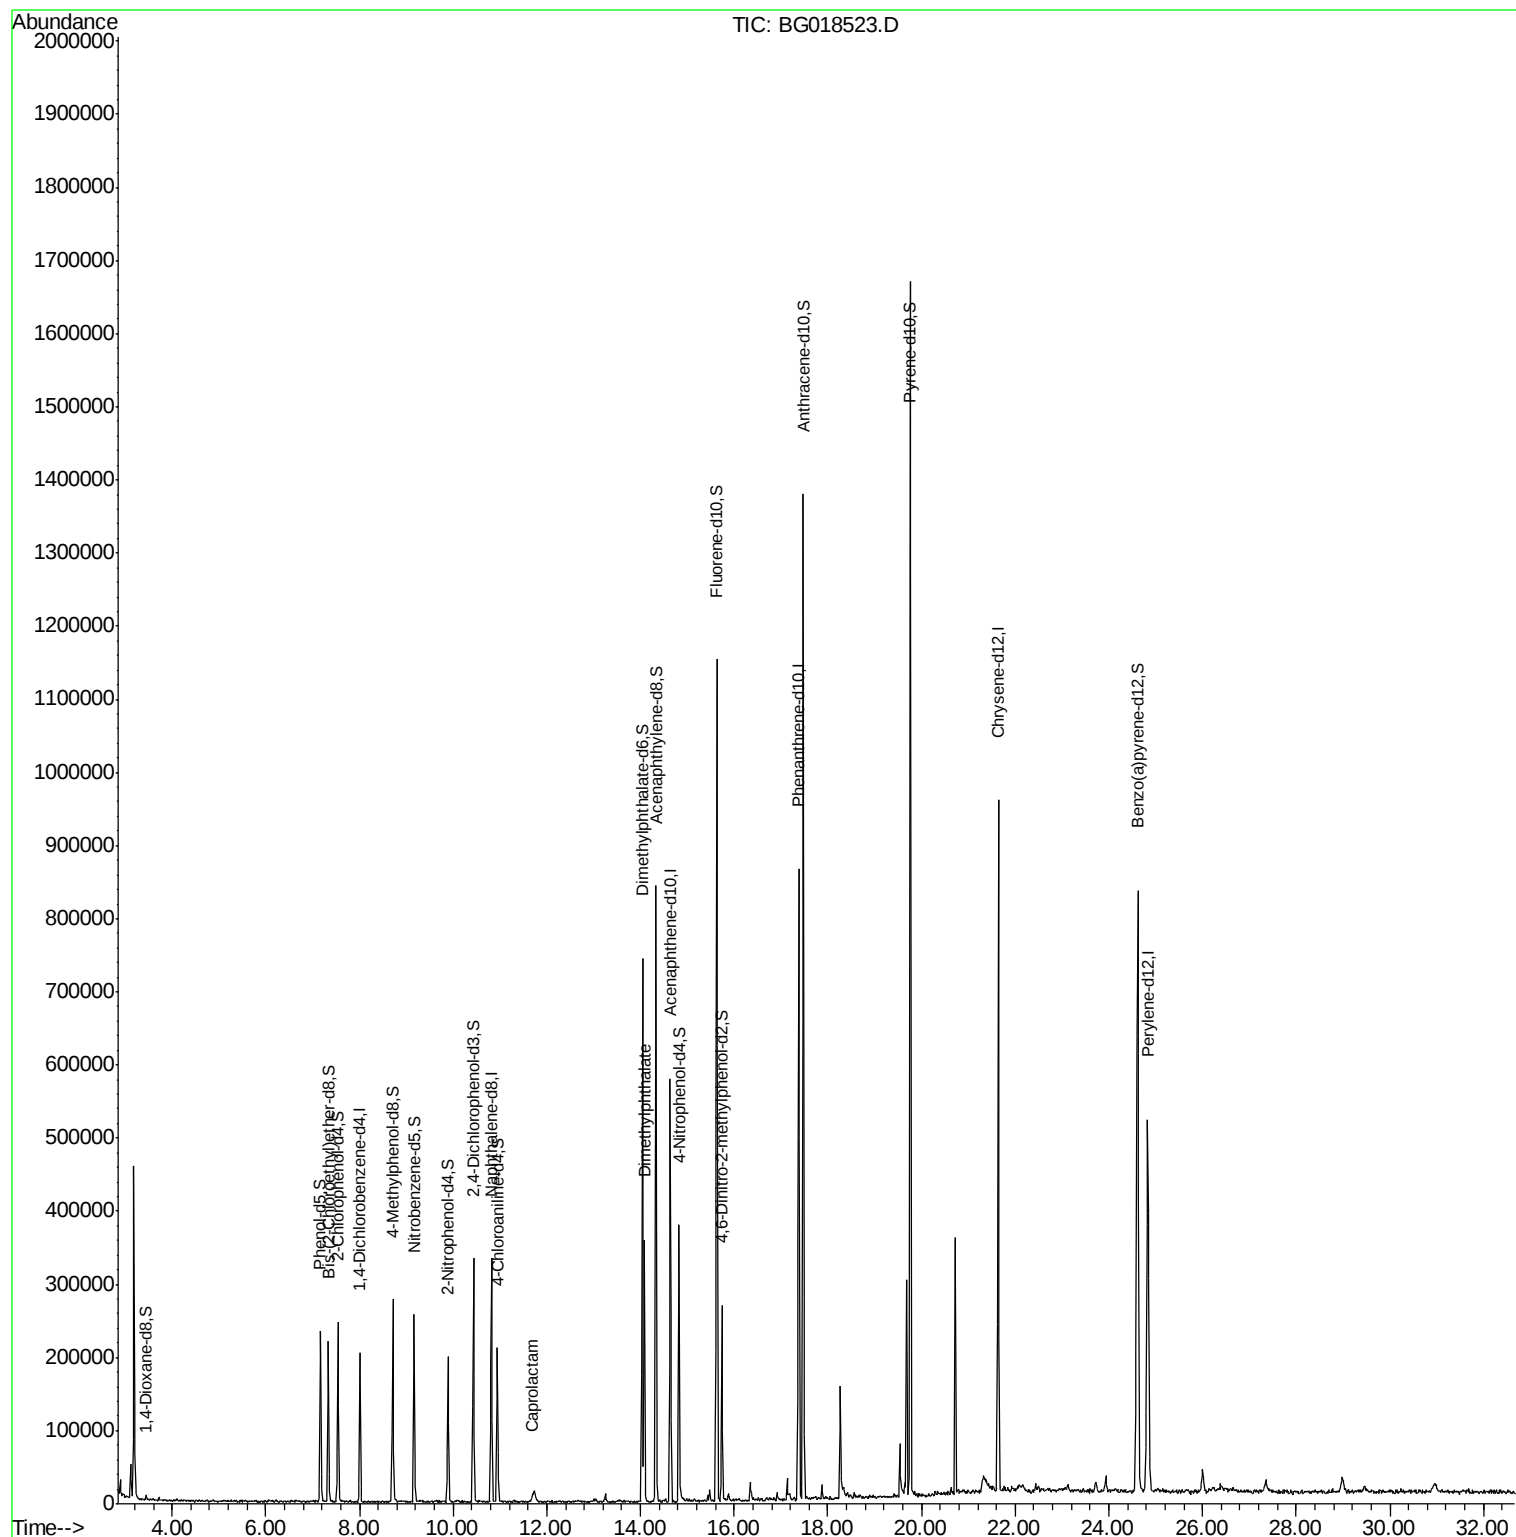


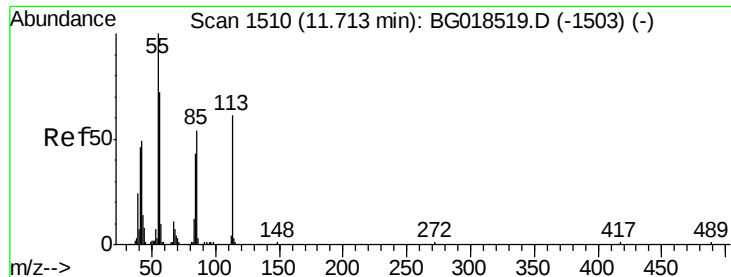

#32
 Caprolactam
 Concen: 1.01 ng/ul
 RT: 11.69 min Scan# 1507
 Delta R.T. -0.02 min
 Lab File: BG018523.D
 Acq: 28 Aug 2015 21:37

Instrument :
 BNA_G
 ClientSampled :

Tot Ion:113 Resp: 1828
 Ion Ratio Lower Upper
 113 100
 55 132.4 124.2 186.4
 56 106.7 98.2 147.4

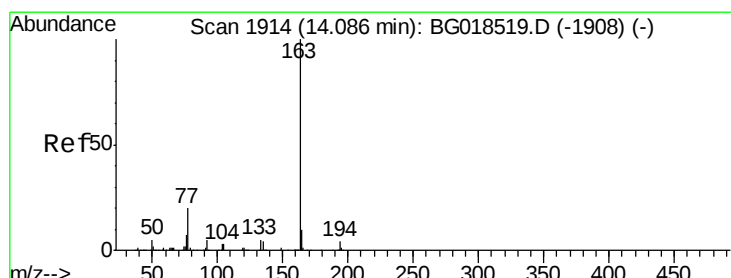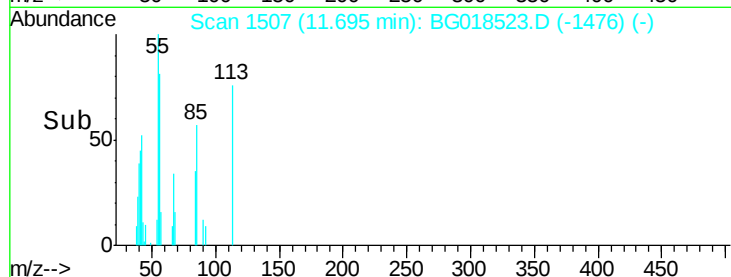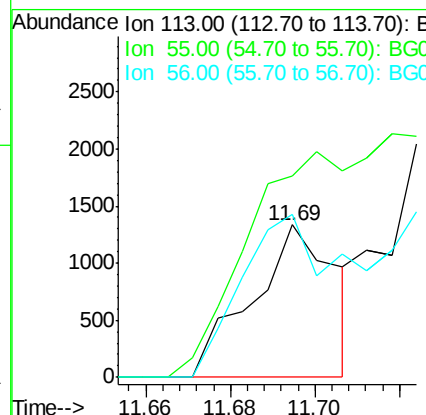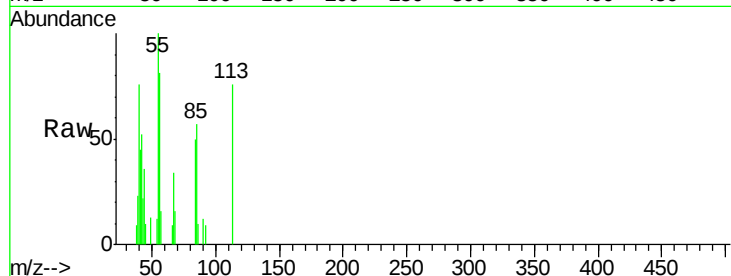

#45
 Dimethylphthalate
 Concen: 15.39 ng/ul
 RT: 14.09 min Scan# 1914
 Delta R.T. -0.00 min
 Lab File: BG018523.D
 Acq: 28 Aug 2015 21:37

Tgt Ion:163 Resp: 247326
 Ion Ratio Lower Upper
 163 100
 194 4.3 2.9 4.3#
 164 9.5 7.7 11.5

