

Data Path : Z:\HPCHEM1\BNA G\DATA\BG082815\
 Data File : BG018526.D
 Acq On : 28 Aug 2015 23:31
 Operator : UM/MA
 Sample : G3448-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Aug 31 03:28:04 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 31 03:29:45 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	78617	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	365145	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	237526	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.38	188	572351	20.00	ng/ul	0.00
78) Chrysene-d12	21.64	240	563451	20.00	ng/ul	0.00
86) Perylene-d12	24.84	264	556934	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.45	96	2977	1.67	ng/uL	0.00
5) Phenol-d5	7.16	99	139490	19.55	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	83323	18.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	102303	18.72	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	113695	18.96	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	56890	19.99	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	55986	19.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	119472	19.42	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	120161	17.28	ng/ul	0.00
44) Dimethylphthalate-d6	14.04	166	378119	18.92	ng/ul	0.00
47) Acenaphthylene-d8	14.33	160	498697	19.82	ng/ul	0.00
52) 4-Nitrophenol-d4	14.82	143	56161	15.62	ng/ul	0.00
58) Fluorene-d10	15.62	176	347915	19.99	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.74	200	35538	12.62	ng/ul	0.00
71) Anthracene-d10	17.48	188	551218	20.14	ng/ul	0.00
79) Pyrene-d10	19.76	212	562359	19.24	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.61	264	567546	19.20	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.09	163	153922	7.81	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG082815\
Data File : BG018526.D
Acq On : 28 Aug 2015 23:31
Operator : UM/MA
Sample : G3448-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Aug 31 03:28:04 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 31 03:29:45 2015
Response via : Initial Calibration

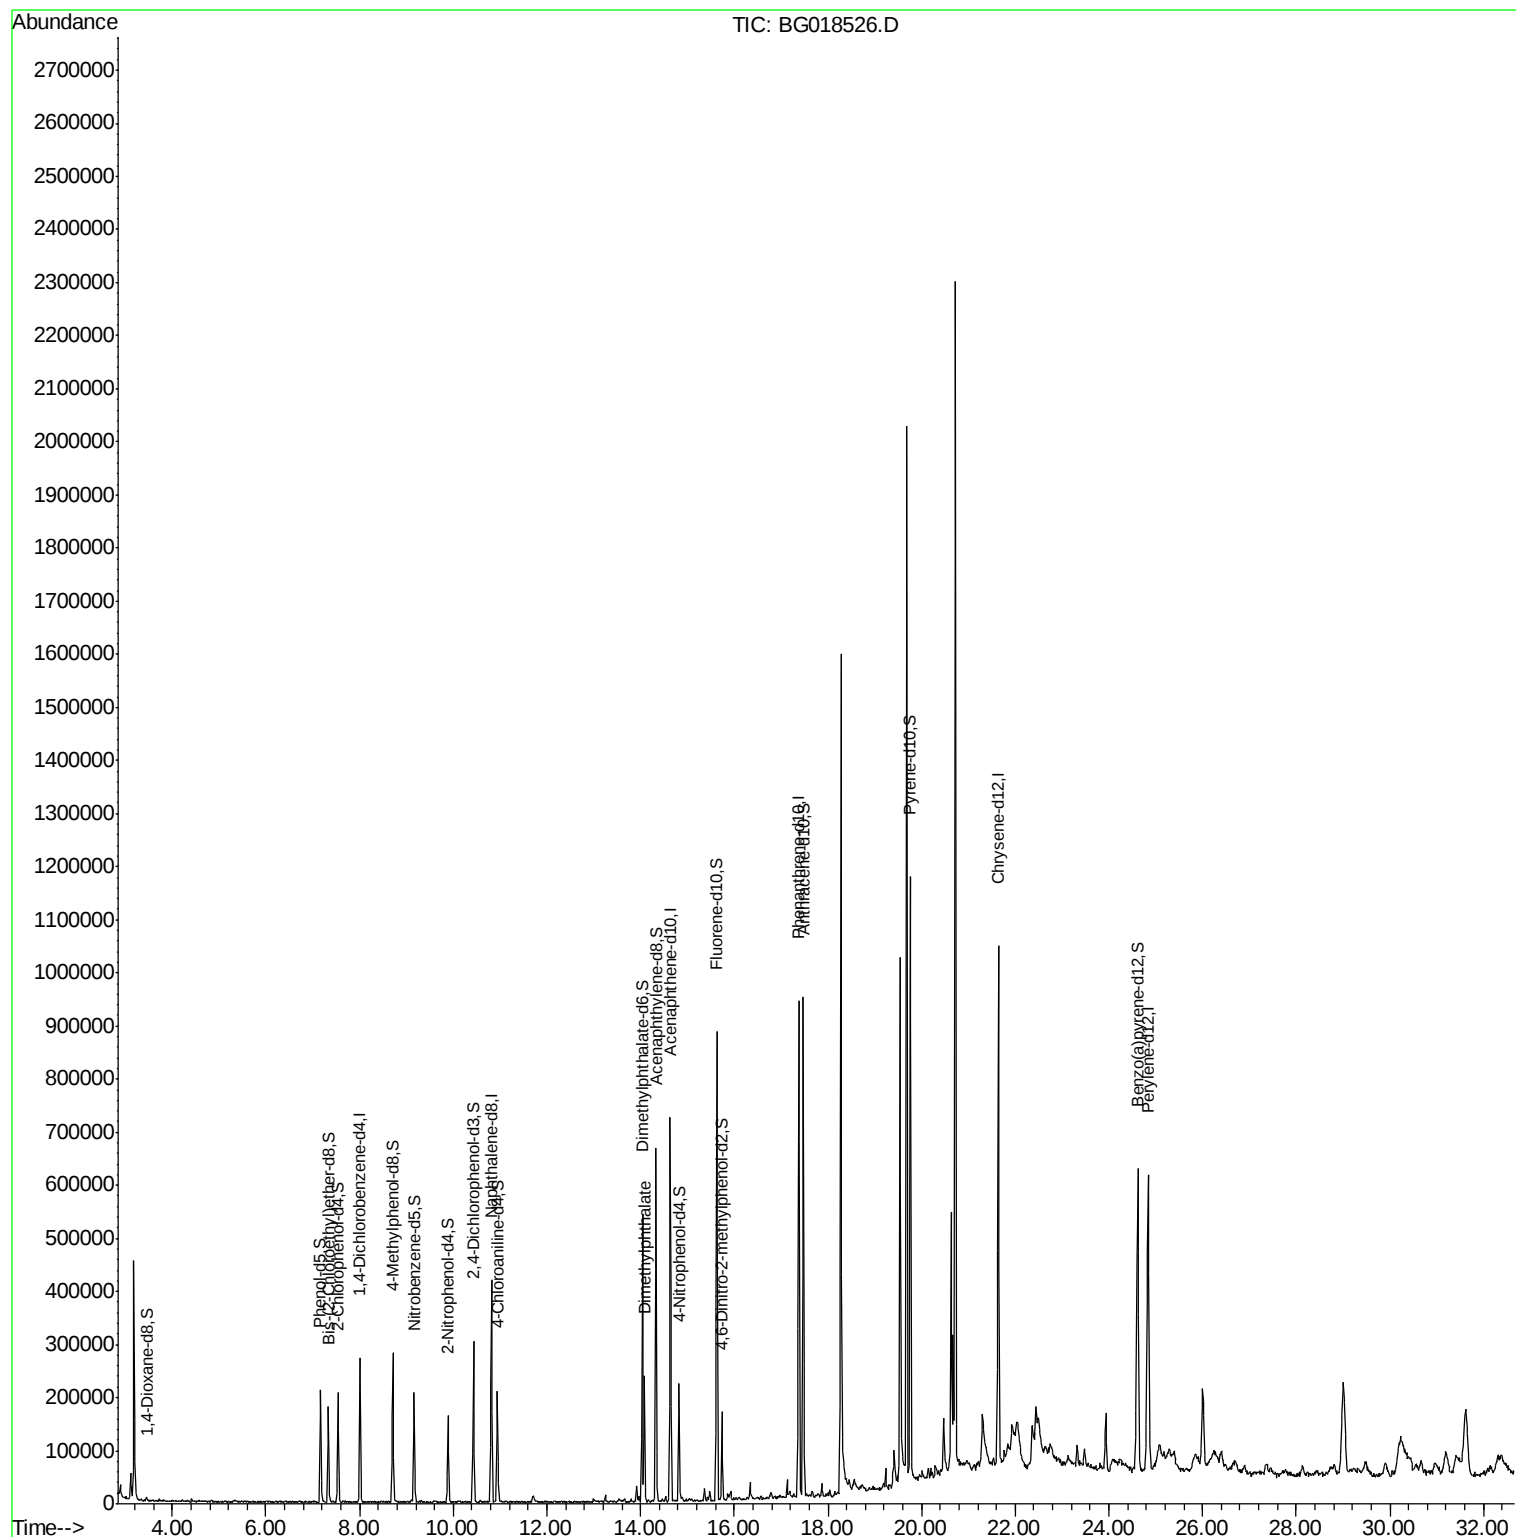


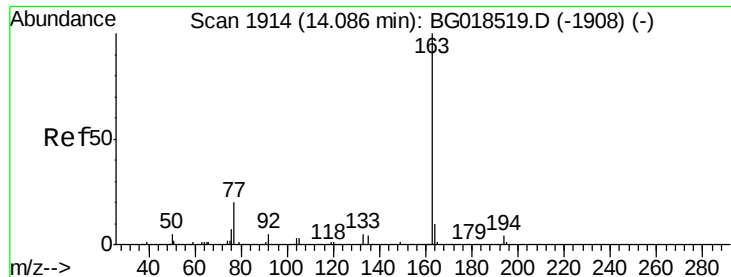

#45
 Dimethylphthalate
 Concen: 7.81 ng/ul
 RT: 14.09 min Scan# 1914
 Delta R.T. -0.00 min
 Lab File: BG018526.D
 Acq: 28 Aug 2015 23:31

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.7	2.9	4.3#
164	10.3	7.7	11.5

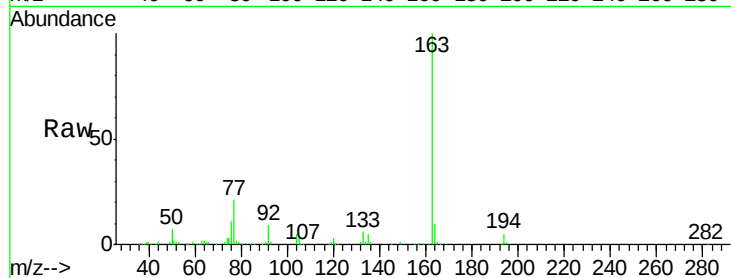

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

