

Data Path : Z:\HPCHEM1\BNA G\DATA\BG082815\
 Data File : BG018530.D
 Acq On : 29 Aug 2015 2:03
 Operator : UM/MA
 Sample : G3448-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Aug 31 03:28:43 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 31 03:29:45 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	80690	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	378622	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	246253	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.38	188	601315	20.00	ng/ul	0.00
78) Chrysene-d12	21.64	240	591646	20.00	ng/ul	0.00
86) Perylene-d12	24.84	264	592546	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.44	96	2959	1.62	ng/uL	0.00
5) Phenol-d5	7.17	99	160290	21.89	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	95226	20.98	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	118820	21.18	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	136567	22.19	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	61901	20.97	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	62243	20.71	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	140325	22.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	177163	24.57	ng/ul	0.00
44) Dimethylphthalate-d6	14.04	166	434062	20.95	ng/ul	0.00
47) Acenaphthylene-d8	14.33	160	501178	19.21	ng/ul	0.00
52) 4-Nitrophenol-d4	14.82	143	68720	18.44	ng/ul	0.00
58) Fluorene-d10	15.63	176	335467	18.59	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.74	200	29580	10.00	ng/ul	0.00
71) Anthracene-d10	17.47	188	506996	17.63	ng/ul	0.00
79) Pyrene-d10	19.76	212	477936	15.57	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.61	264	432903	13.76	ng/ul	0.00


Target Compounds						Ovalue
32) Caprolactam	11.70	113	5140	2.13	ng/ul	88
45) Dimethylphthalate	14.08	163	170708	8.35	ng/ul#	98
77) Fluoranthene	19.43	202	35118	1.01	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG082815\
Data File : BG018530.D
Acq On : 29 Aug 2015 2:03
Operator : UM/MA
Sample : G3448-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Aug 31 03:28:43 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 31 03:29:45 2015
Response via : Initial Calibration

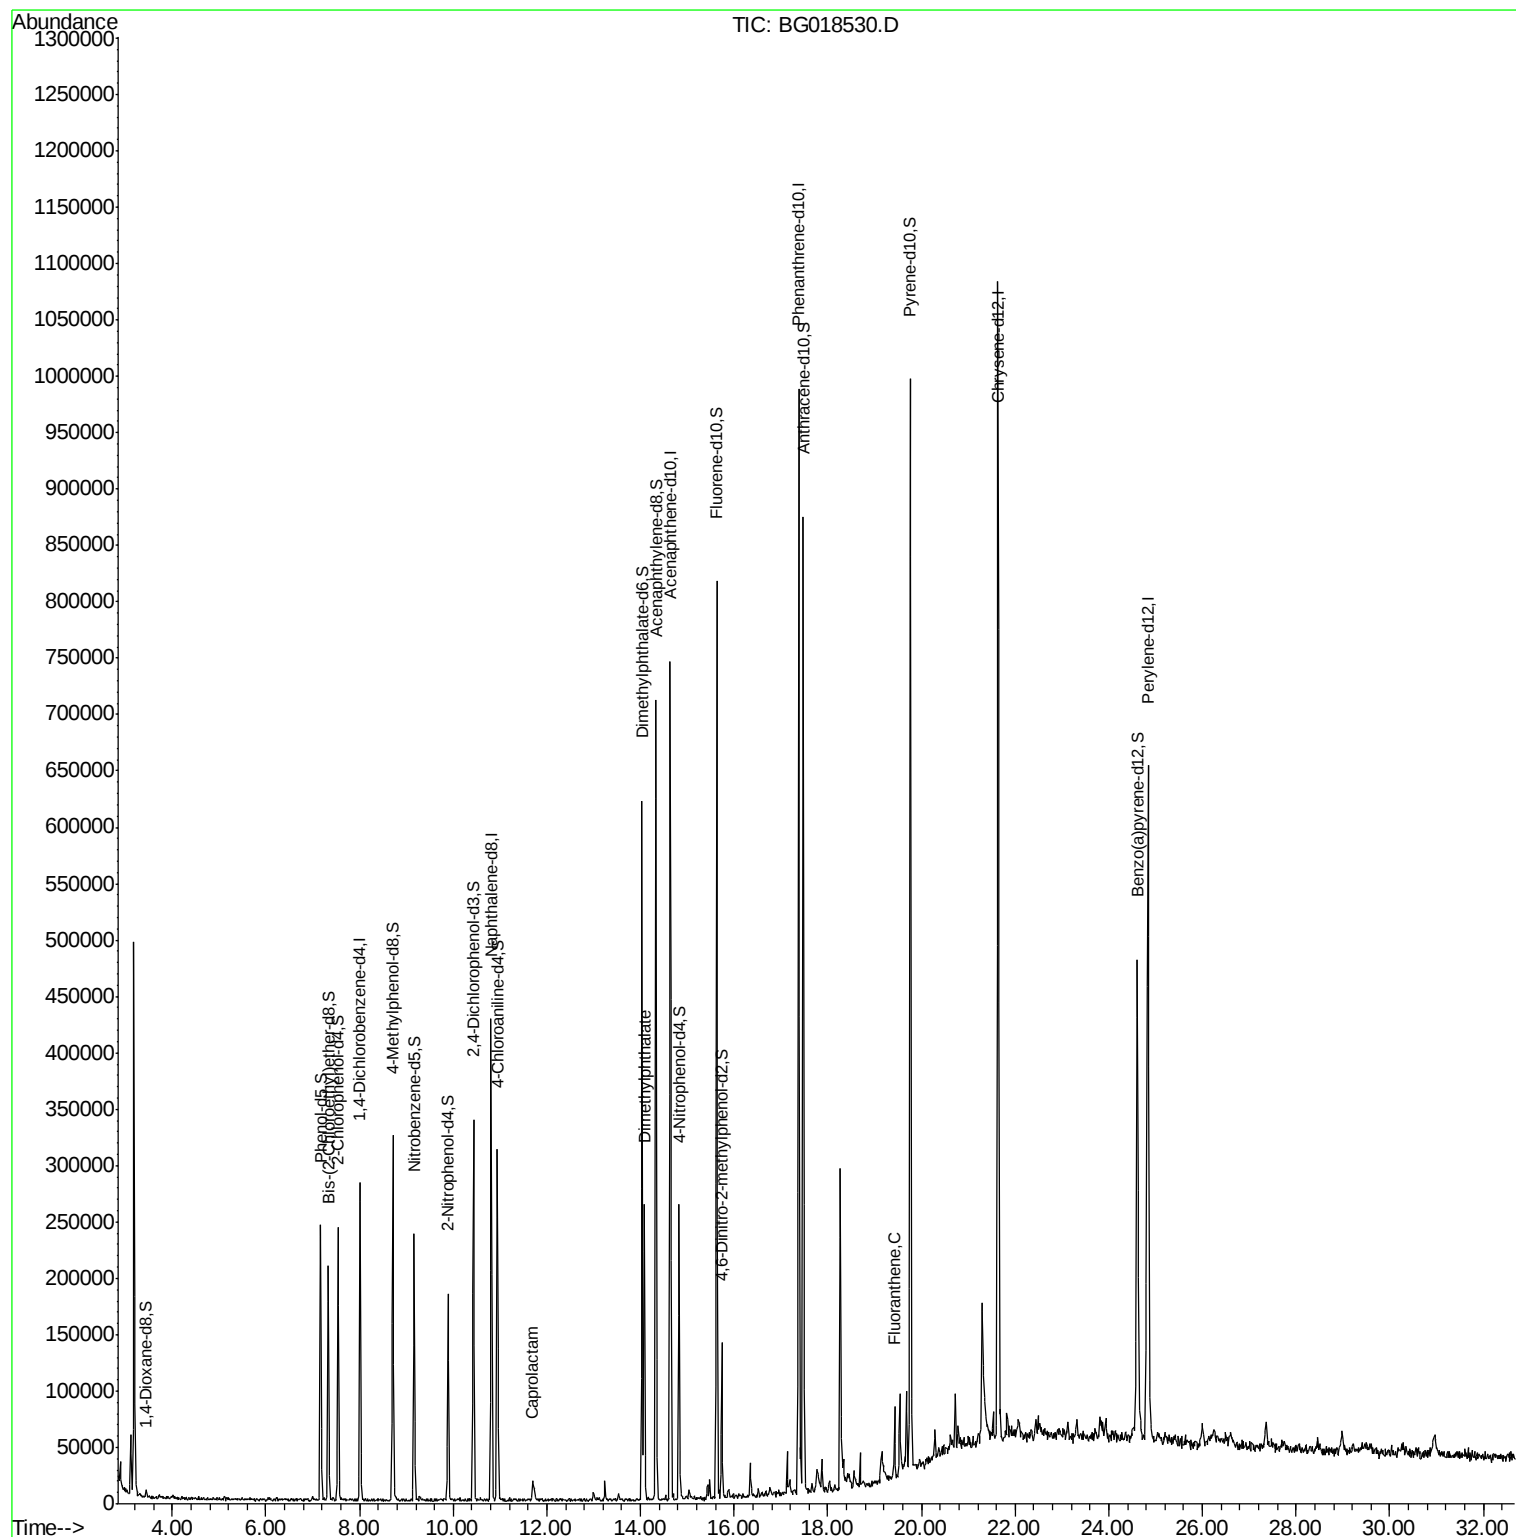

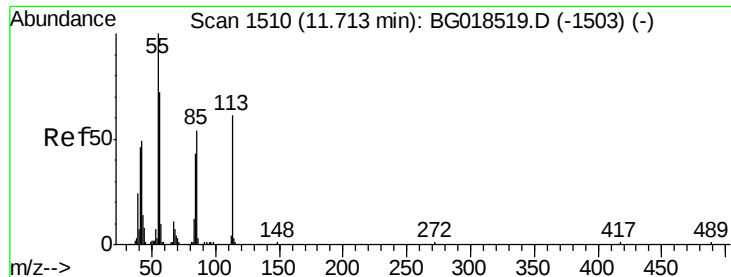

#32

Caprolactam

Concen: 2.13 ng/ul

RT: 11.70 min Scan# 1508

Delta R.T. -0.01 min

Lab File: BG018530.D

Acq: 29 Aug 2015 2:03

Instrument :

BNA_G

ClientSampled :


Tot Ion:113 Resp: 5140

Ion Ratio Lower Upper

113 100

55 133.2 124.2 186.4




56 130.0 98.2 147.4

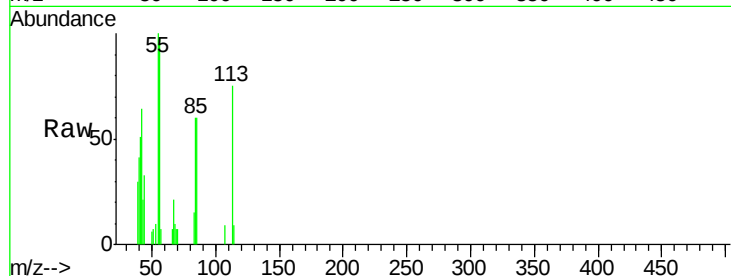

Abundance Ion 113.00 (112.70 to 113.70): E

Ion 55.00 (54.70 to 55.70): BGC

Ion 56.00 (55.70 to 56.70): BGC

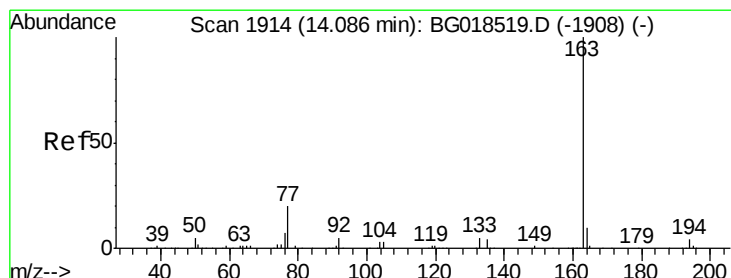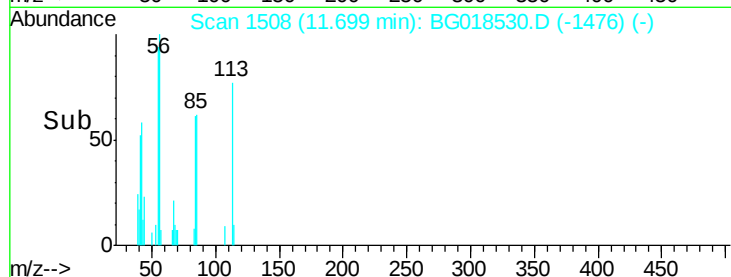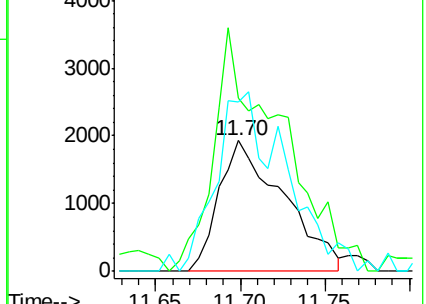

#45

Dimethylphthalate

Concen: 8.35 ng/ul

RT: 14.08 min Scan# 1914

Delta R.T. -0.00 min

Lab File: BG018530.D

Acq: 29 Aug 2015 2:03


Tgt Ion:163 Resp: 170708

Ion Ratio Lower Upper

163 100

194 4.6 2.9 4.3#



164 10.2 7.7 11.5

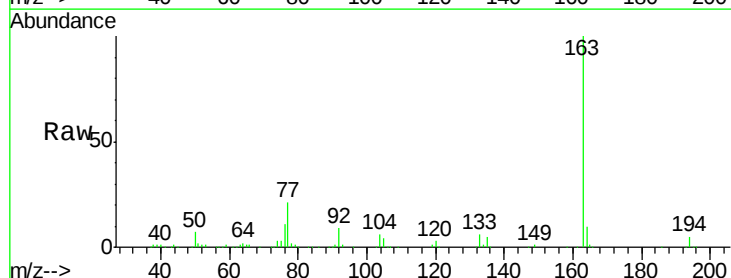


Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

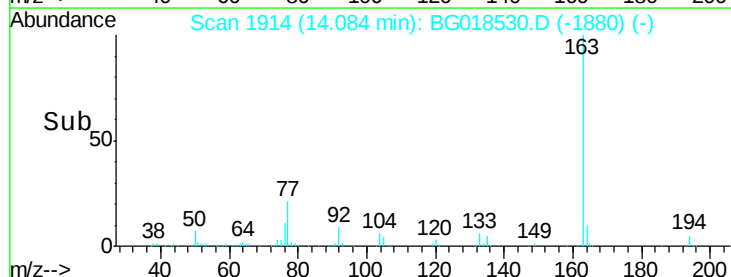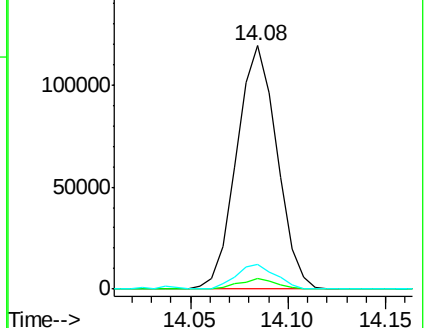


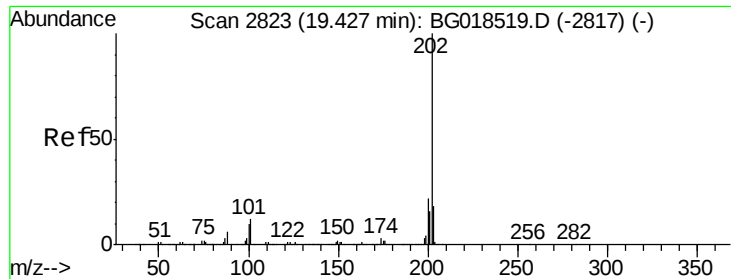

#77
 Fluoranthene
 Concen: 1.01 ng/ul
 RT: 19.43 min Scan# 2823
 Delta R.T. -0.00 min
 Lab File: BG018530.D
 Acq: 29 Aug 2015 2:03

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
202	100		
101	11.3	9.7	14.5
100	8.4	7.8	11.8

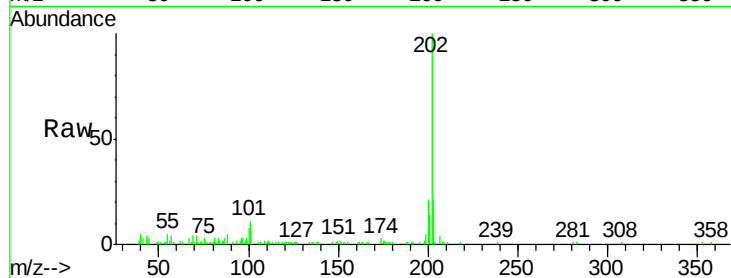

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

