


Data Path : Z:\HPCHEM1\BNA G\DATA\BG082815\
Data File : BG018513.D
Acq On : 28 Aug 2015 13:57
Operator : UM/MA
Sample : G3436-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BC3B3

Quant Time: Aug 31 01:49:32 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 31 01:23:00 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
8/31/2015 1:47:19 PM

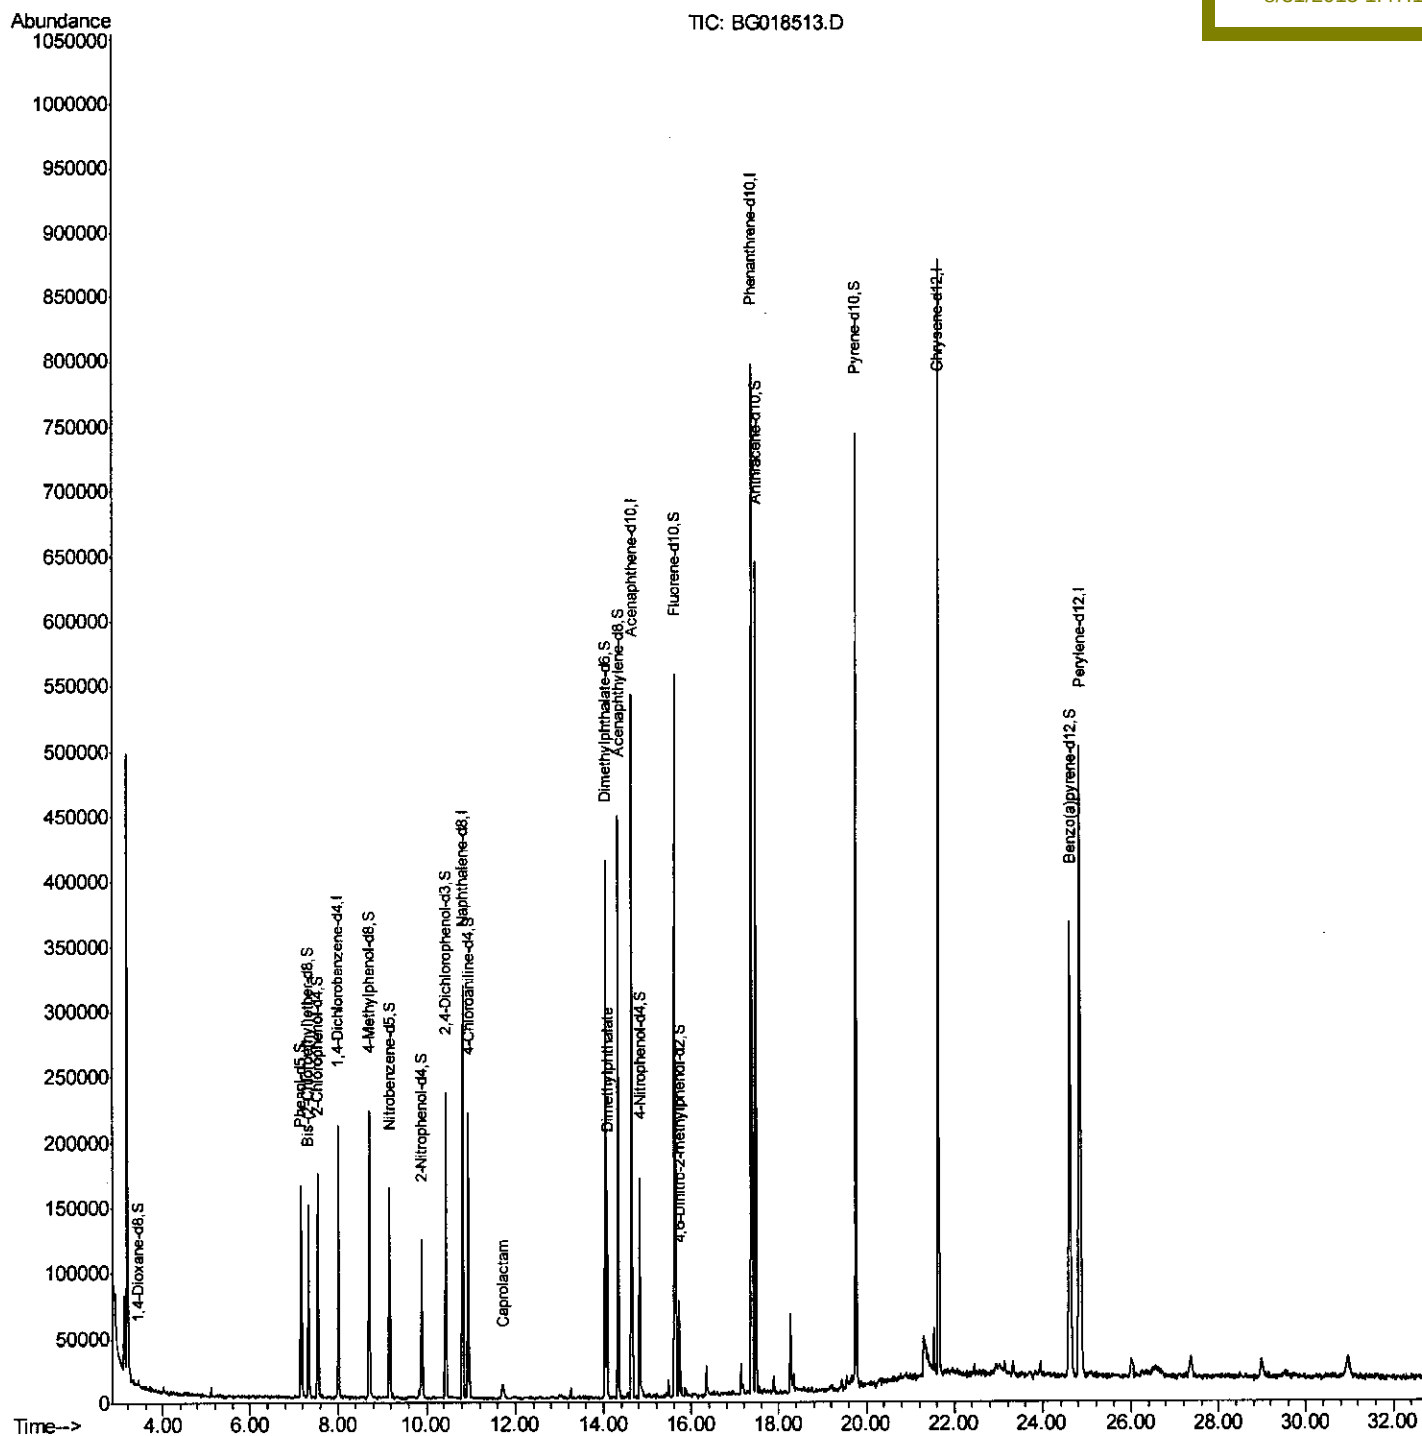

Quantitation Report (Qedit)



Data Path : Z:\HPCHEM1\BNA G\DATA\BG082815\
 Data File : BG018513.D
 Acq On : 28 Aug 2015 13:57
 Operator : UM/MA
 Sample : G3436-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BC3B3

Quant Time: Aug 31 01:20:46 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 31 01:23:00 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 8/31/2015 1:47:19 PM

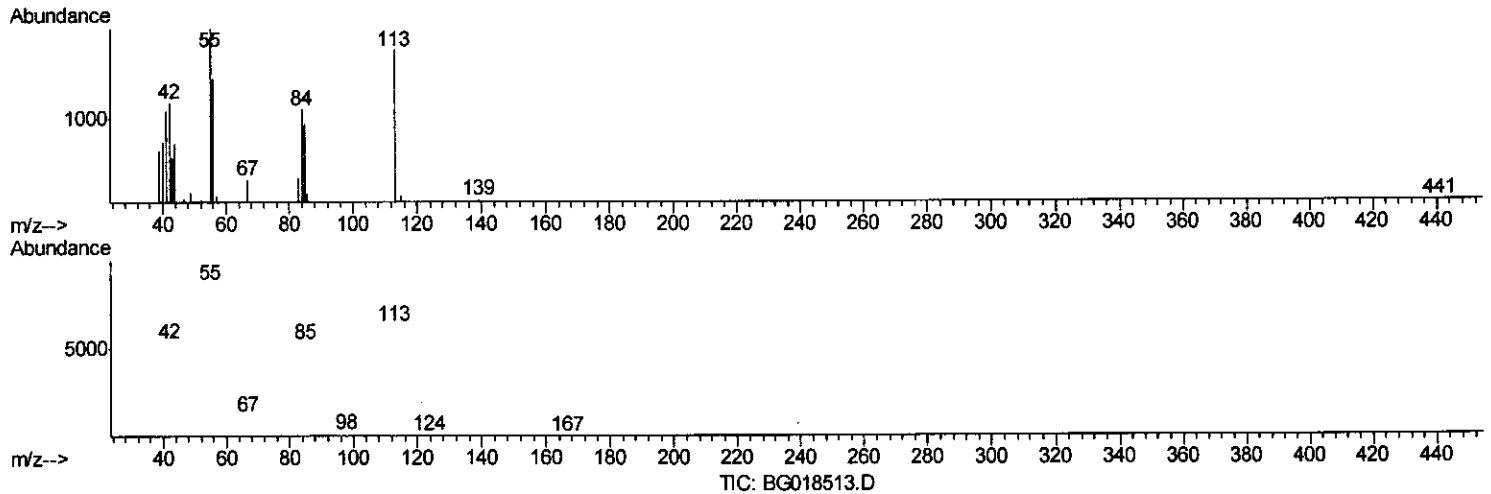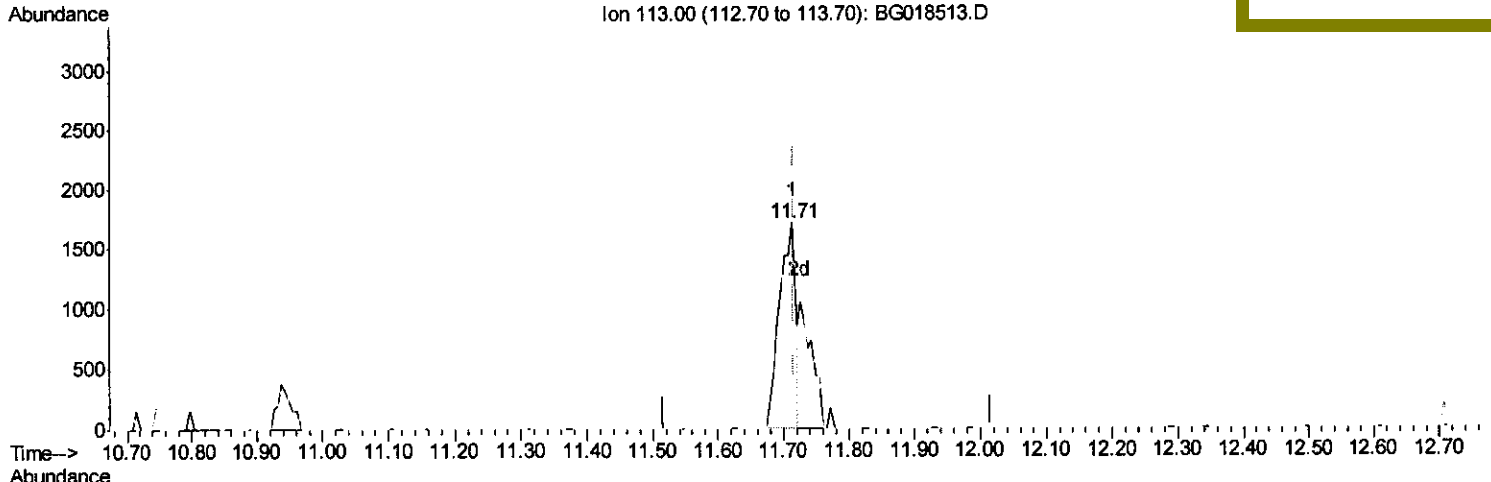

(32) Caprolactam

11.713min (-0.002) 1.64ng/ul

response 2850

Ion	Exp%	Act%
113.00	100	100
55.00	155.30	112.95#
56.00	122.80	82.24#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA G\DATA\BG082815\
 Data File : BG018513.D
 Acq On : 28 Aug 2015 13:57
 Operator : UM/MA
 Sample : G3436-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BC3B3

Quant Time: Aug 31 01:20:46 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 31 01:23:00 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 8/31/2015 1:47:19 PM

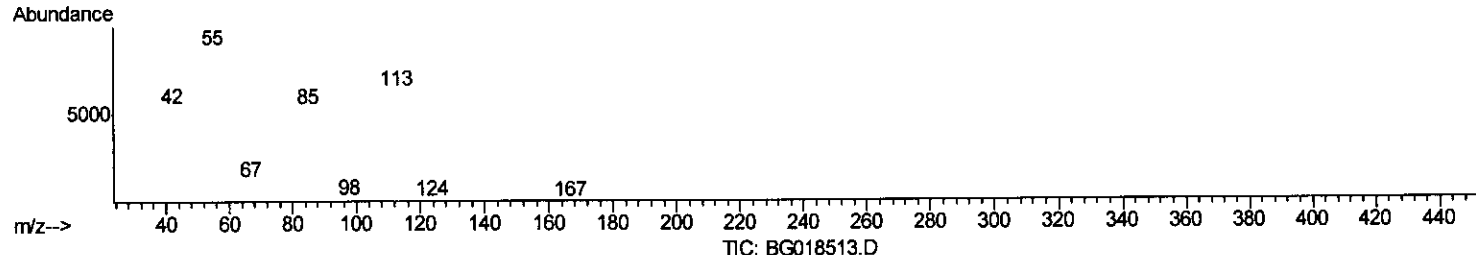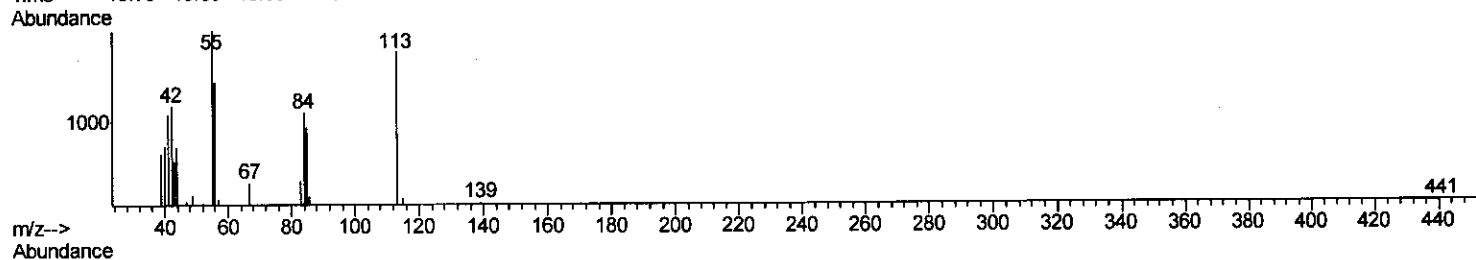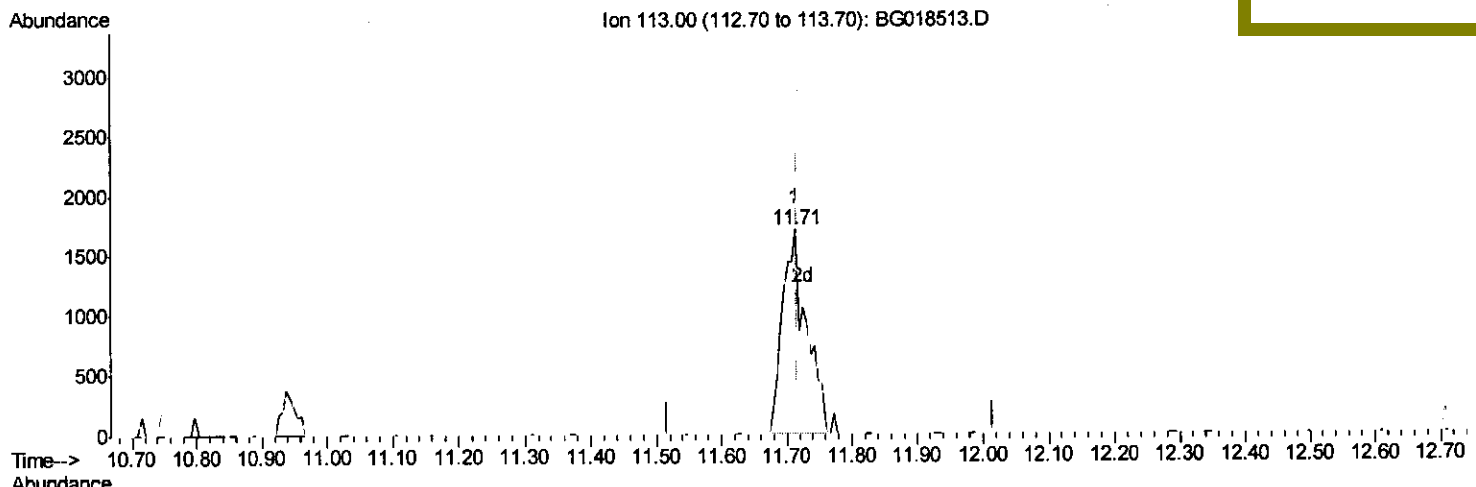

(32) Caprolactam

11.713min (-0.002) 2.49ng/ul m

response 4330

Ion	Exp%	Act%
113.00	100	100
55.00	155.30	112.95#
56.00	122.80	82.24#
0.00	0.00	0.00

U.M
 09/01/15

Data Path : Z:\HPCHEM1\BNA G\DATA\BG082815\
 Data File : BG018513.D
 Acq On : 28 Aug 2015 13:57
 Operator : UM/MA
 Sample : G3436-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampled :
 BC3B3

Quant Time: Aug 31 01:49:32 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 31 01:23:00 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 8/31/2015 1:47:19 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	61515	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	273952	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	180605	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.38	188	471436	20.00	ng/ul	0.00
78) Chrysene-d12	21.64	240	493651	20.00	ng/ul	0.00
86) Perylene-d12	24.83	264	482994	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.44	96	3335	2.40	ng/uL	0.00
5) Phenol-d5	7.17	99	108757	19.48	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	71179	20.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	84940	19.86	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	93364	19.90	ng/ul	0.00
19) Nitrobenzene-d5	9.16	128	43956	20.58	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	43656	20.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	90588	19.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	127251	24.39	ng/ul	0.00
44) Dimethylphthalate-d6	14.04	166	303048	19.94	ng/ul	0.00
47) Acenaphthylene-d8	14.33	160	331107	17.30	ng/ul	0.00
52) 4-Nitrophenol-d4	14.82	143	45621	16.69	ng/ul	0.00
58) Fluorene-d10	15.63	176	226066	17.08	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.74	200	17302	7.46	ng/ul	0.00
71) Anthracene-d10	17.48	188	367540	16.30	ng/ul	0.00
79) Pyrene-d10	19.76	212	376170	14.69	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.61	264	344718	13.44	ng/ul	-0.01

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
32) Caprolactam	11.71	113	4330m	2.49	ng/ul	
45) Dimethylphthalate	14.08	163	104440	6.97	ng/ul#	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

U.M
 09/01/15