

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082815\
 Data File : BG018524.D
 Acq On : 28 Aug 2015 22:15
 Operator : UM/MA
 Sample : G3448-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AC4

Quant Time: Aug 31 03:27:42 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 31 03:29:45 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	67462	20.00	ng/ul	0.00
18) Naphthalene-d8	10.82	136	323396	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	215692	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.38	188	541820	20.00	ng/ul	0.00
78) Chrysene-d12	21.64	240	547288	20.00	ng/ul	0.00
86) Perylene-d12	24.83	264	533074	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.45	96	2317	1.52	ng/uL	0.00
5) Phenol-d5	7.17	99	98027	16.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	62664	16.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	74422	15.87	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	79458	15.45	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	40650	16.13	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	39598	15.42	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	88486	16.24	ng/ul	0.00
29) 4-Chloroaniline-d4	10.95	131	105032	17.06	ng/ul	0.00
44) Dimethylphthalate-d6	14.04	166	296484	16.34	ng/ul	0.00
47) Acenaphthylene-d8	14.33	160	326002	14.27	ng/ul	0.00
52) 4-Nitrophenol-d4	14.82	143	41889	12.83	ng/ul	0.00
58) Fluorene-d10	15.63	176	207385	13.12	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	27625	10.37	ng/ul	0.00
71) Anthracene-d10	17.47	188	301354	11.63	ng/ul	0.00
79) Pyrene-d10	19.76	212	270559	9.53	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.61	264	217167	7.67	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.08	163	113302	6.33	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082815\
Data File : BG018524.D
Acq On : 28 Aug 2015 22:15
Operator : UM/MA
Sample : G3448-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AC4

Quant Time: Aug 31 03:27:42 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 31 03:29:45 2015
Response via : Initial Calibration

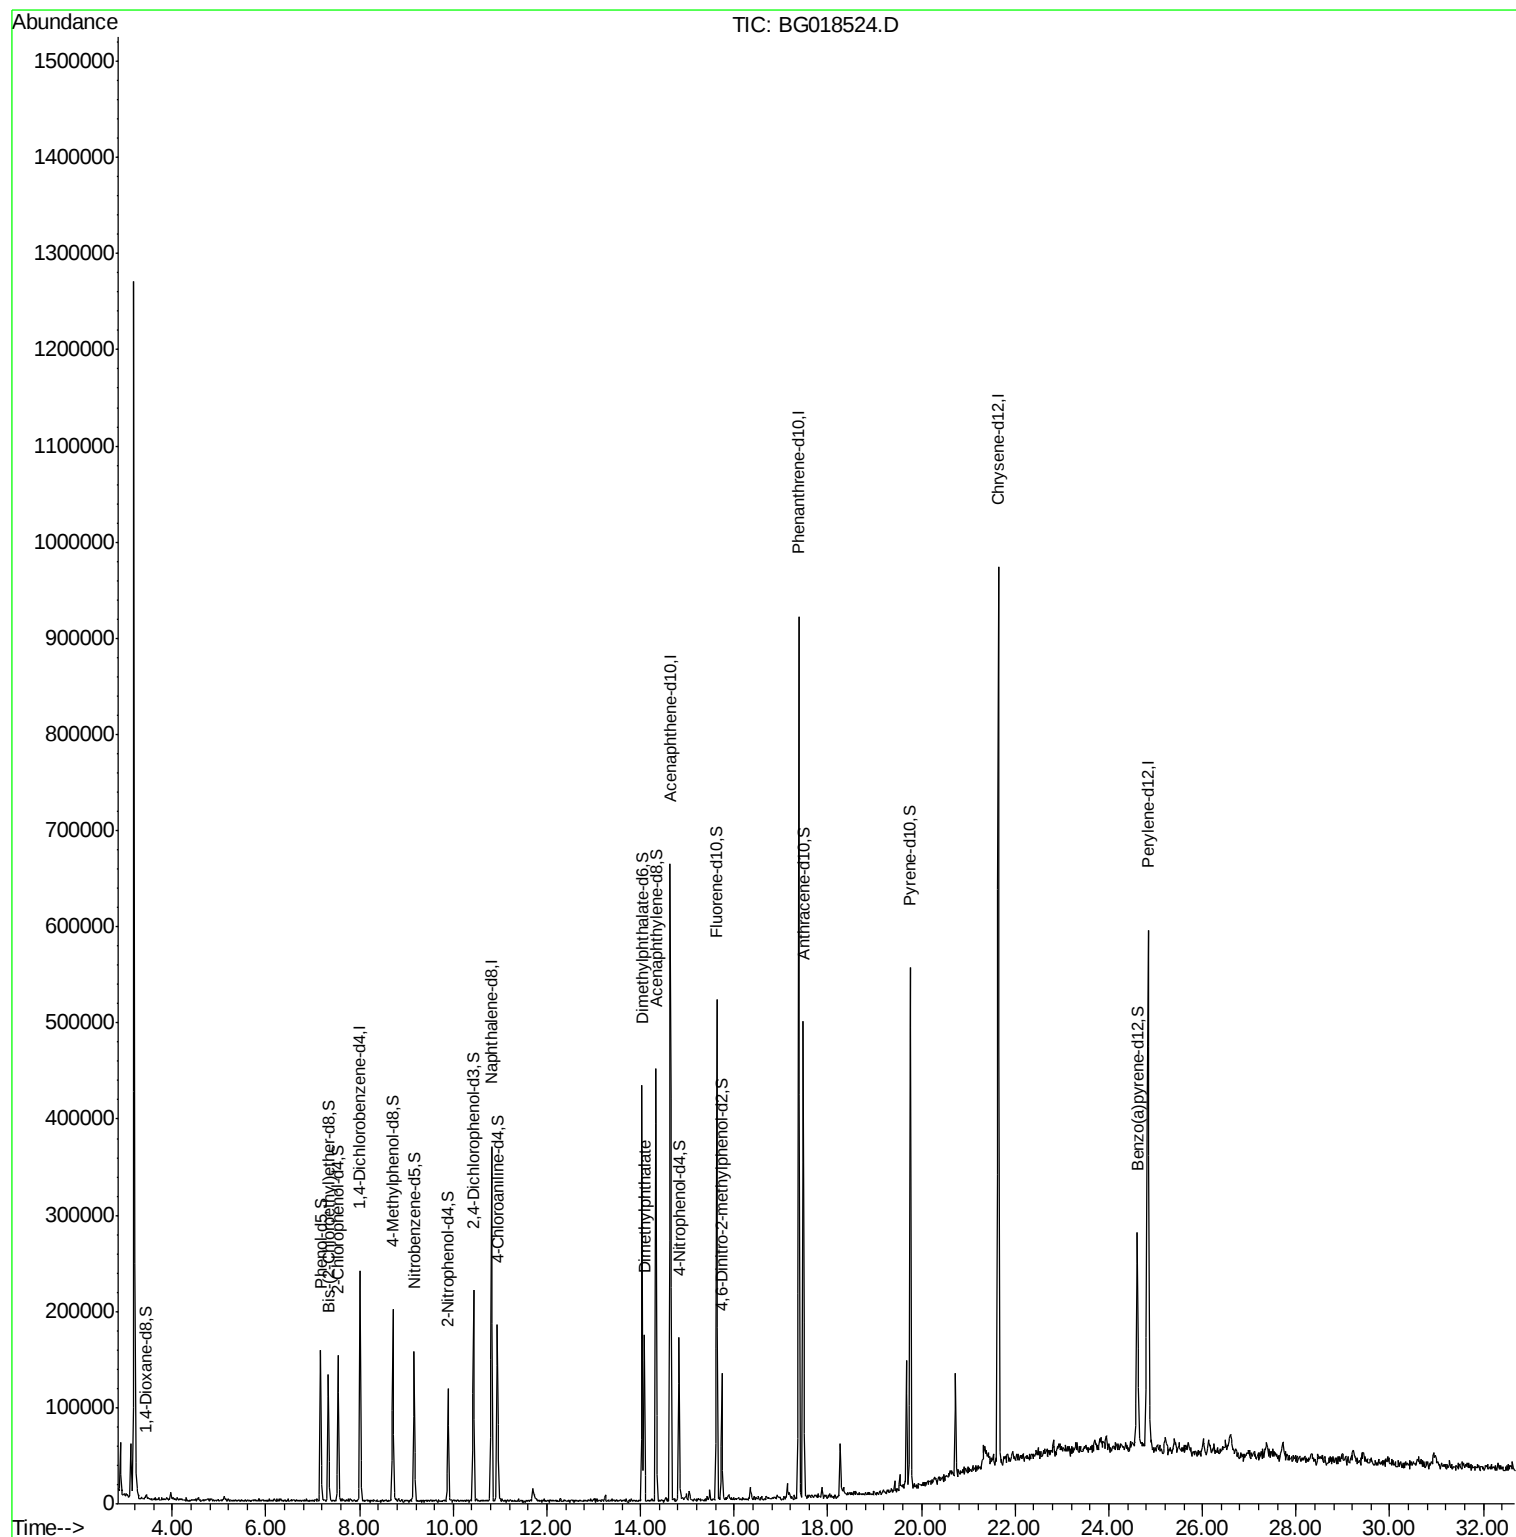

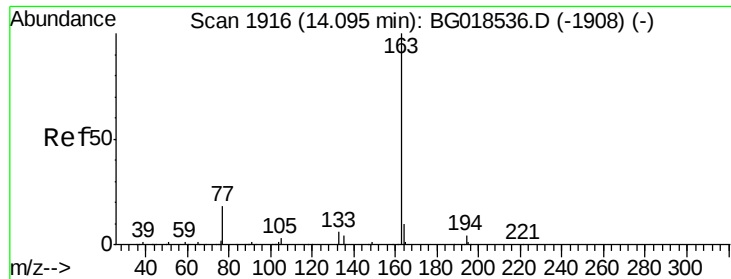

#45
 Dimethylphthalate
 Concen: 6.33 ng/ul
 RT: 14.08 min Scan# 1914
 Delta R.T. -0.00 min
 Lab File: BG018524.D
 Acq: 28 Aug 2015 22:15

Instrument :
 BNA_G
 ClientSampleId :
 C0AC4

Tgt Ion:	163	Resp:	113302
Ion	Ratio	Lower	Upper
163	100		
194	4.0	2.9	4.3
164	8.8	7.7	11.5

