
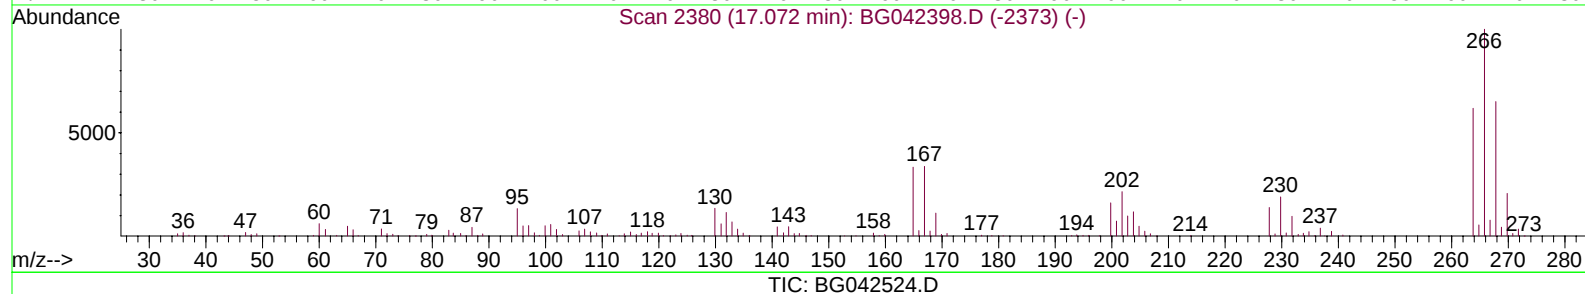
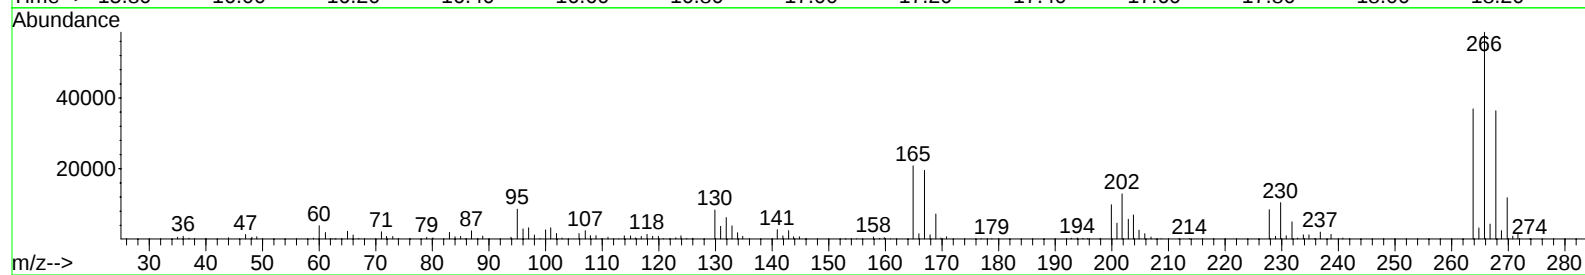


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG082819\
Data File : BG042524.D
Acq On : 28 Aug 2019 8:06
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 18:38:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 14:29:15 2019
Response via : Initial Calibration

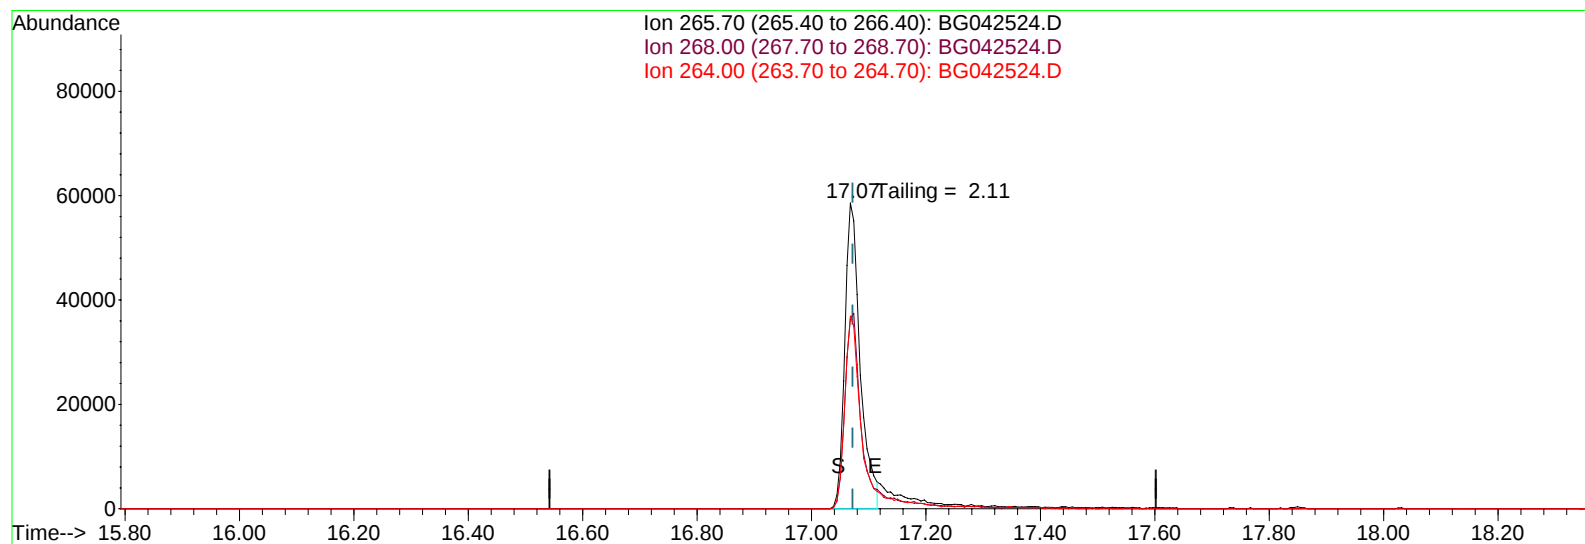

(70) Pentachlorophenol (C)




17.068min (-0.004) 162502.44ng

response 125738

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	62.11
264.00	61.80	63.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG082819\
Data File : BG042524.D
Acq On : 28 Aug 2019 8:06
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 18:38:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 14:29:15 2019
Response via : Initial Calibration

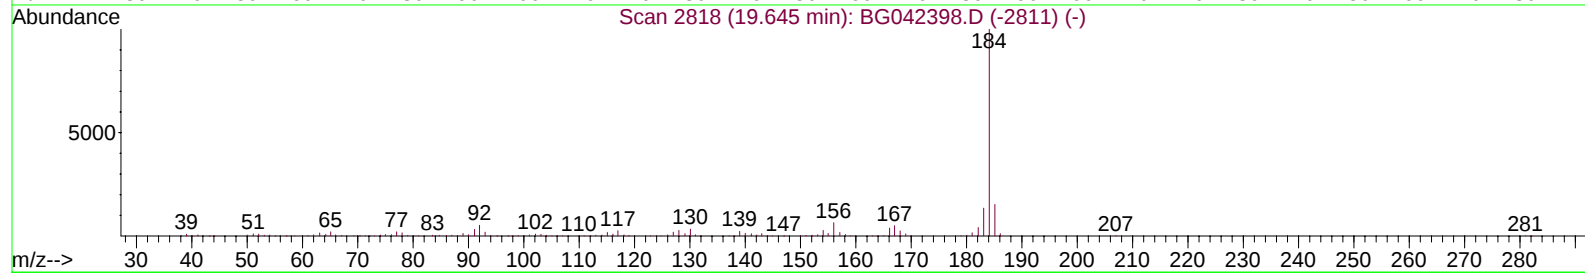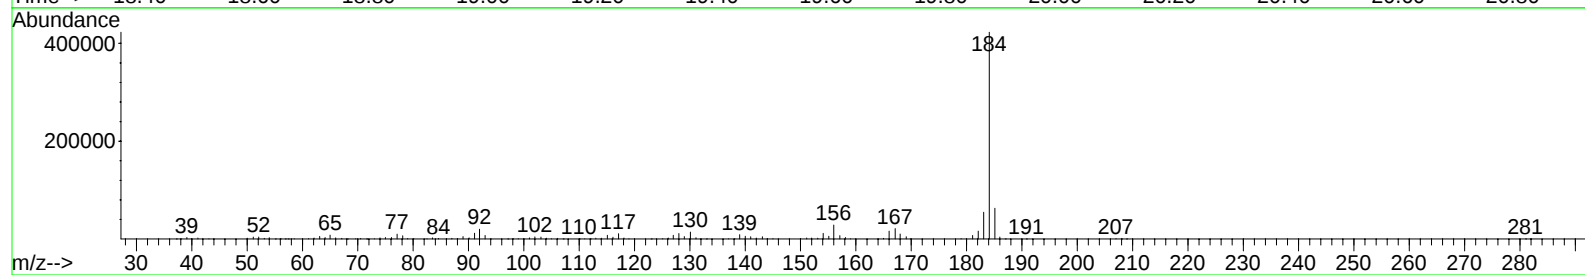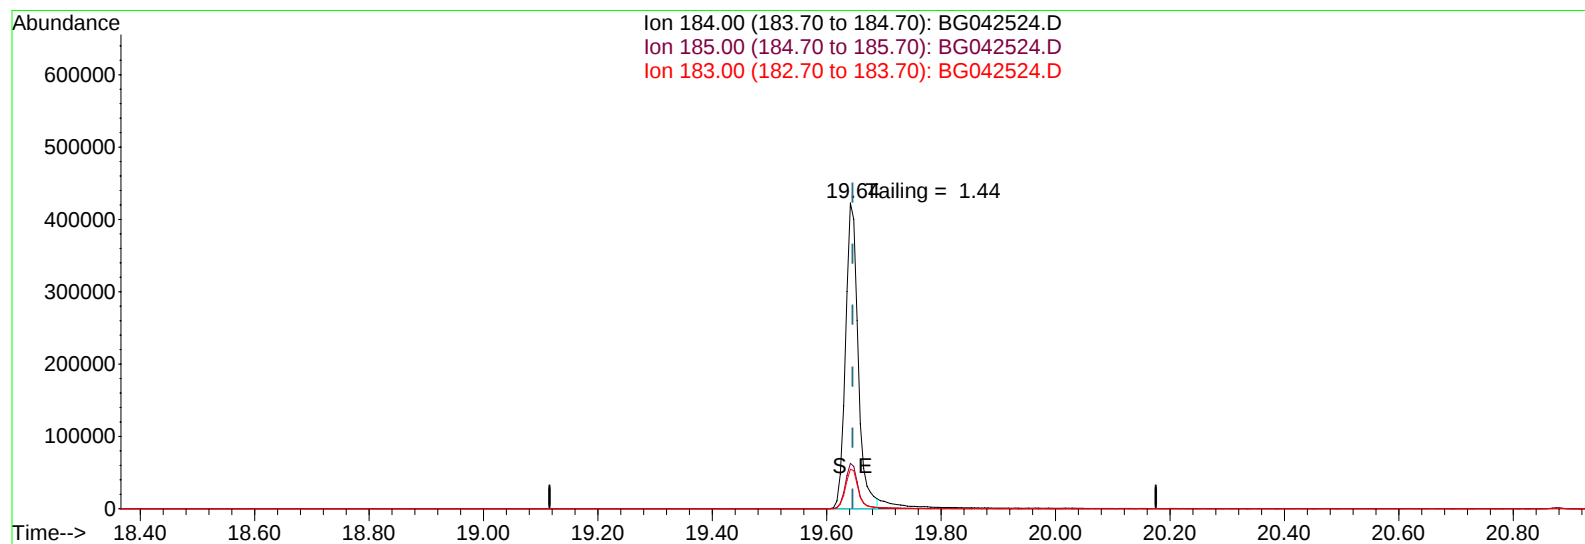

(77) Benzidine

19.641min (-0.004) 347662.21ng

response 687766

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.89
183.00	13.50	12.96
0.00	0.00	0.00