


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082819\  
 Data File : BG042524.D  
 Acq On : 28 Aug 2019 8:06  
 Operator : HP/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG082219.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Aug 22 14:29:15 2019

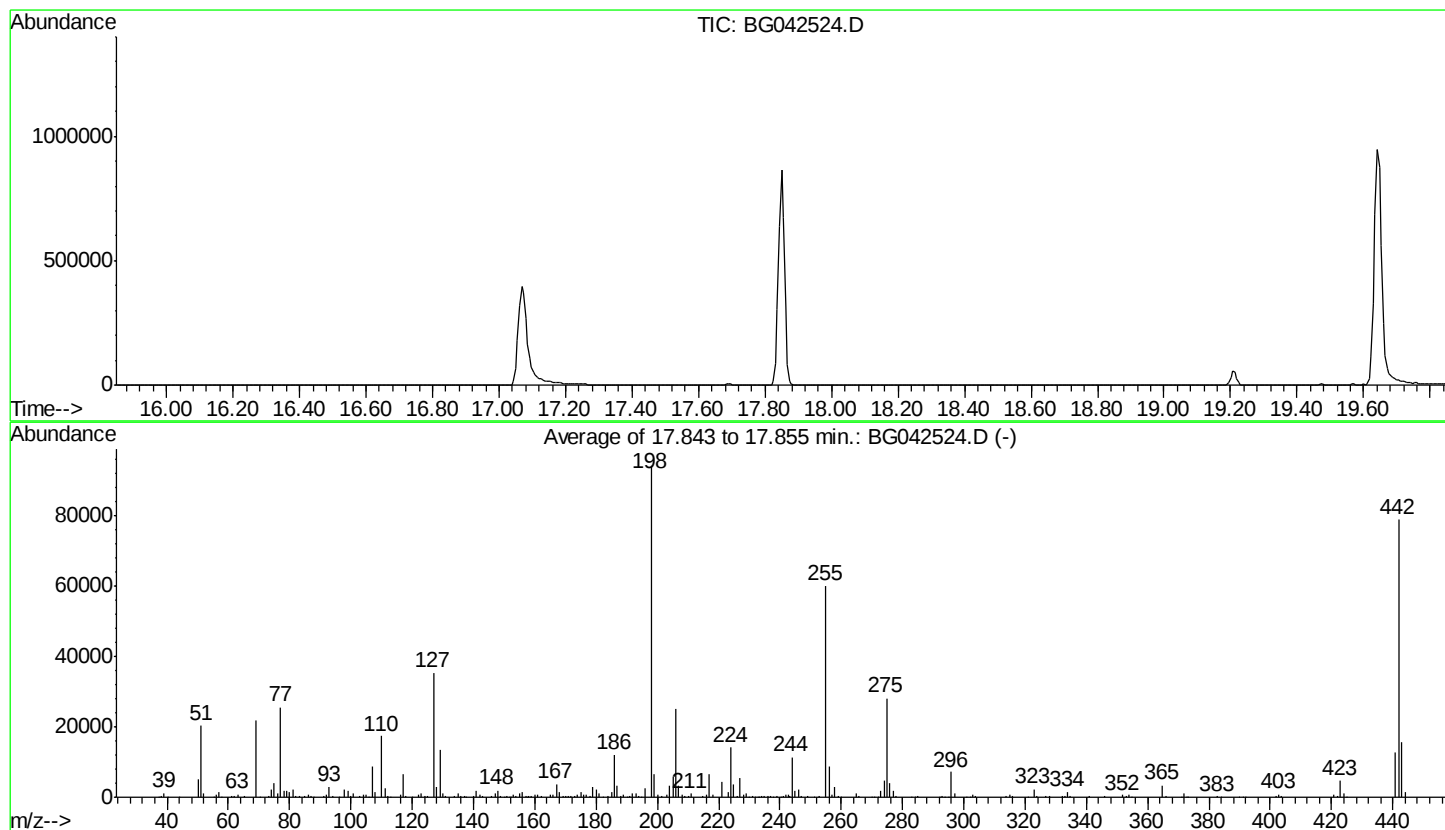

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 21.6      | 20279   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 23.4      | 21978   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.3       | 57      | PASS             |
| 127         | 198          | 10           | 80           | 37.6      | 35338   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 94064   | PASS             |
| 199         | 198          | 5            | 9            | 6.9       | 6504    | PASS             |
| 275         | 198          | 10           | 60           | 29.8      | 28026   | PASS             |
| 365         | 198          | 1            | 100          | 3.6       | 3379    | PASS             |
| 441         | 198          | 0.01         | 100          | 13.5      | 12722   | PASS             |
| 442         | 198          | 50           | 100          | 83.7      | 78765   | PASS             |
| 443         | 442          | 15           | 24           | 19.8      | 15610   | PASS             |