


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082922\
 Data File : BG054765.D
 Acq On : 29 Aug 2022 9:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 25 17:50:55 2022

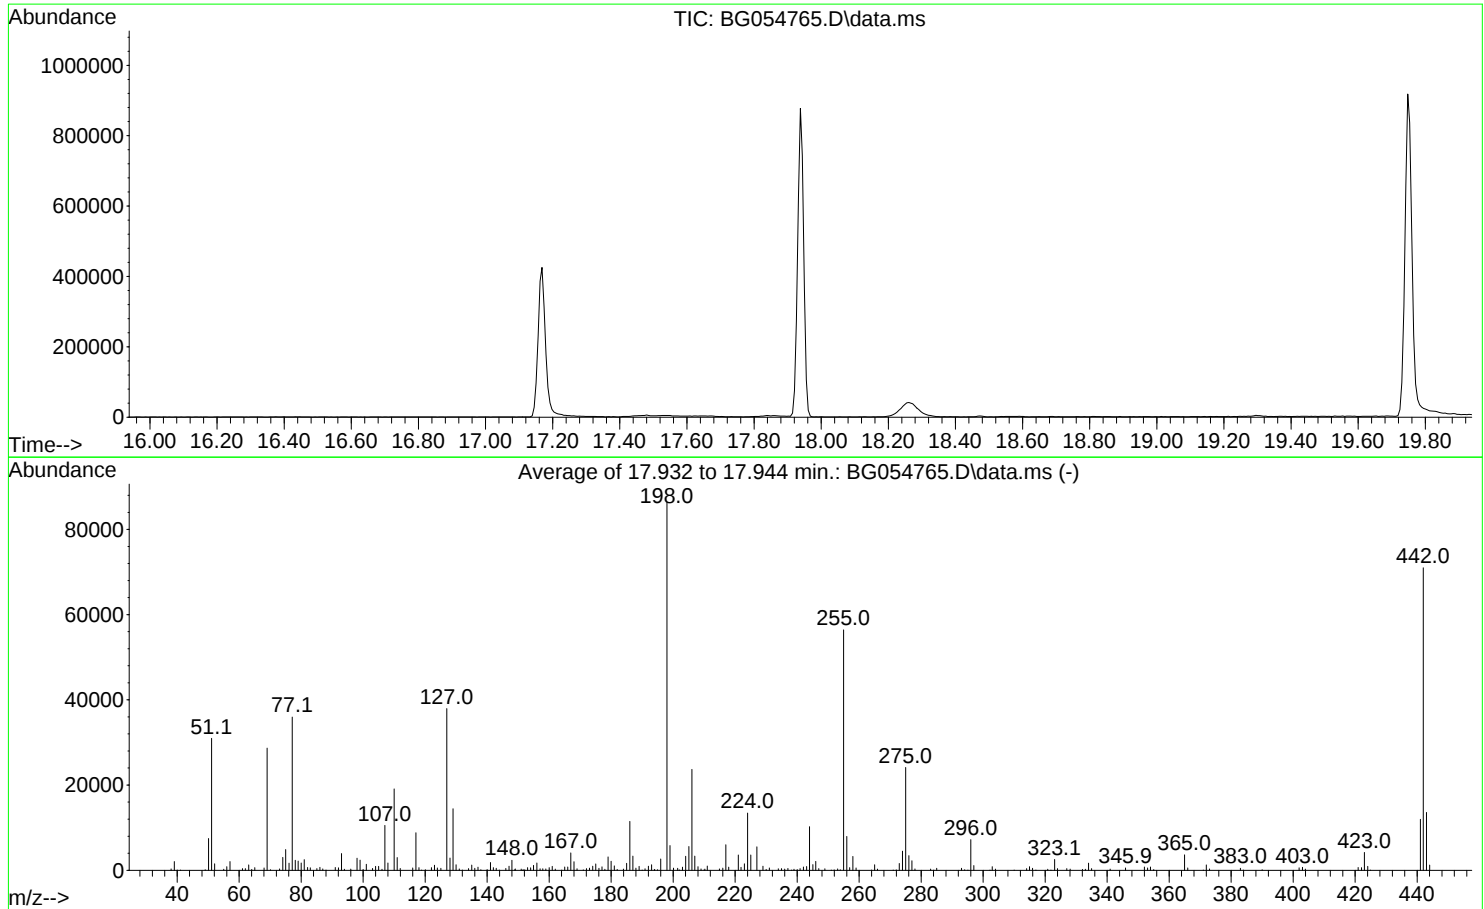




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	30968	PASS
68	69	0.00	2	2.0	560	PASS
69	198	0.00	100	33.2	28685	PASS
70	69	0.00	2	0.4	128	PASS
127	198	10	80	43.9	37936	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	86344	PASS
199	198	5	9	6.7	5818	PASS
275	198	10	60	27.9	24120	PASS
365	198	1	100	4.2	3610	PASS
441	198	0.01	100	13.8	11957	PASS
442	442	50	100	100.0	71008	PASS
443	442	15	24	19.1	13590	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082922\
Data File : BG054765.D
Acq On : 29 Aug 2022 9:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 30 05:18:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

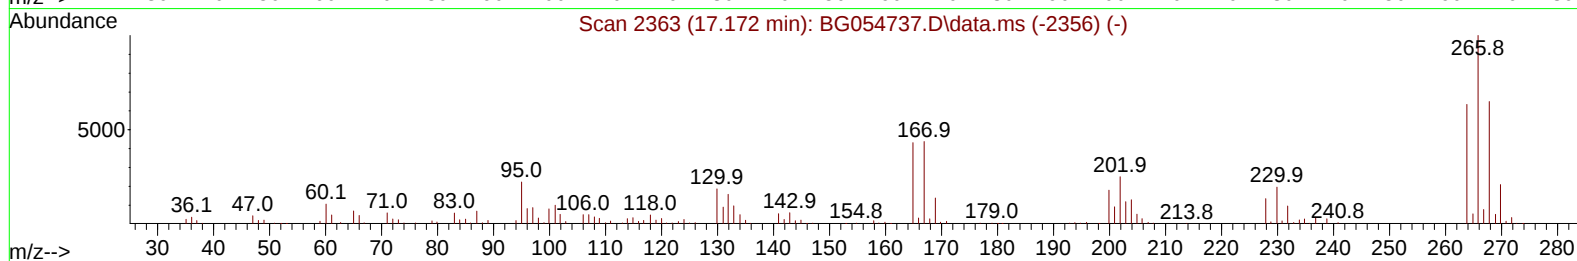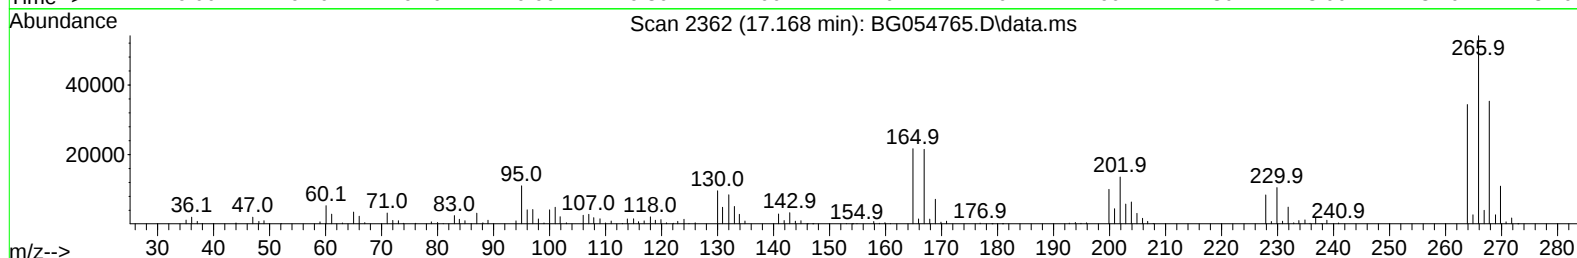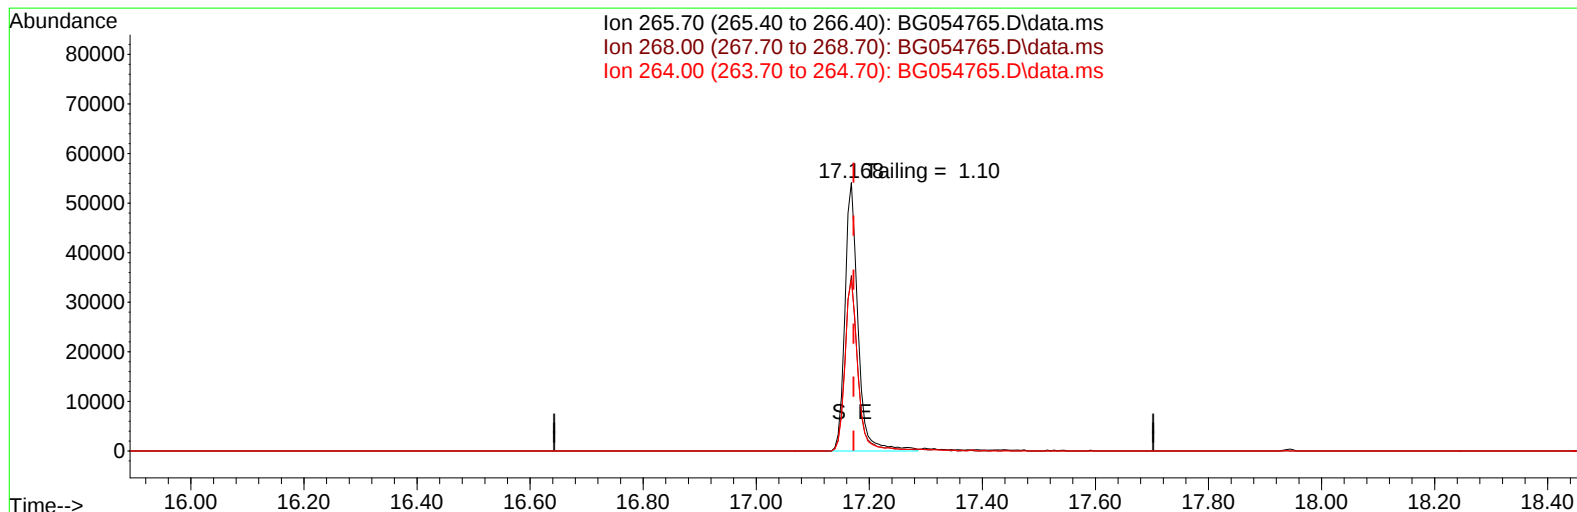

TIC: BG054765.D\data.ms

(70) Pentachlorophenol (C)

17.168min (-0.004) 21519.00 ng




response 85719

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	65.33
264.00	61.70	63.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082922\
Data File : BG054765.D
Acq On : 29 Aug 2022 9:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 30 05:18:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

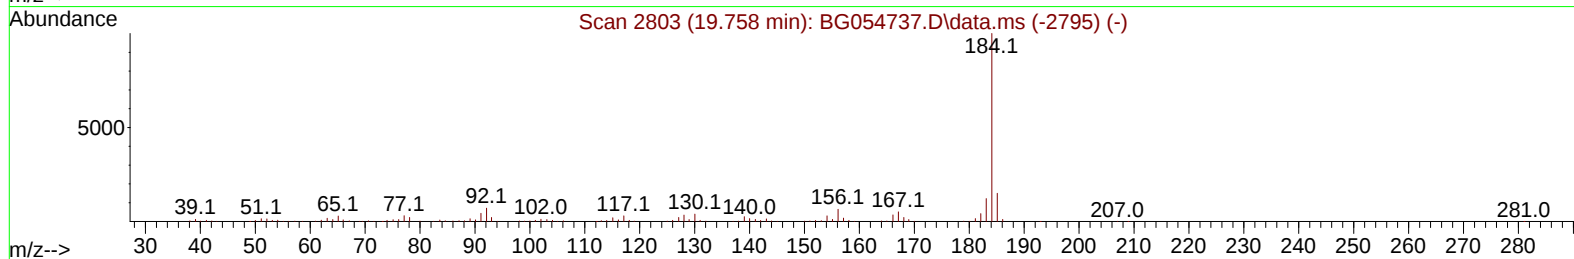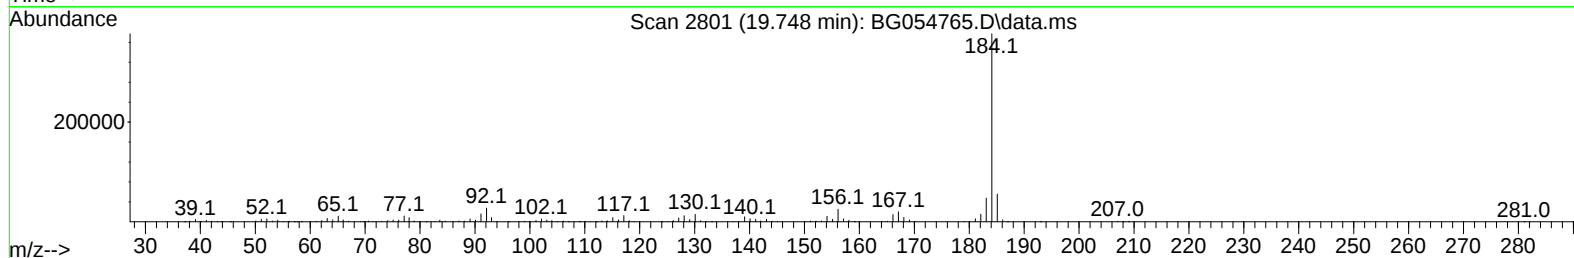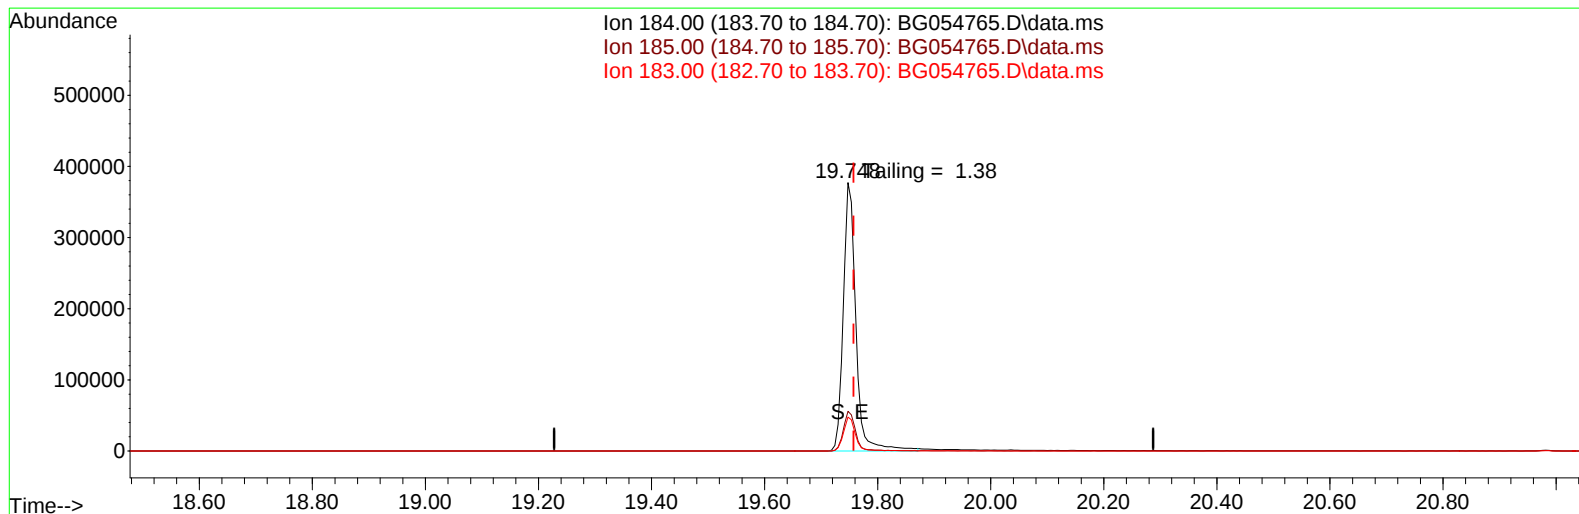

TIC: BG054765.D\data.ms

(77) Benzidine

19.748min (-0.010) 0.00 ng

response 589731

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.77
183.00	12.30	12.66
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/29/2022	BNA_G	BG054765.D
Compound Name	Response	Retention Time
DDT	275781	20.982
DDD	5241	20.535
DDE	469	20.03
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5710	281491	2.03

Instrument :
BNA_G
ClientSampleId :
DFTPP