
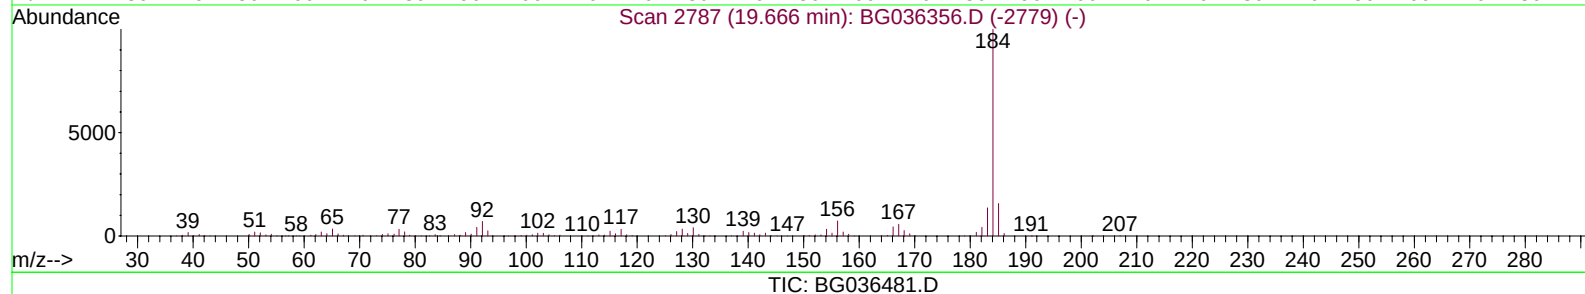
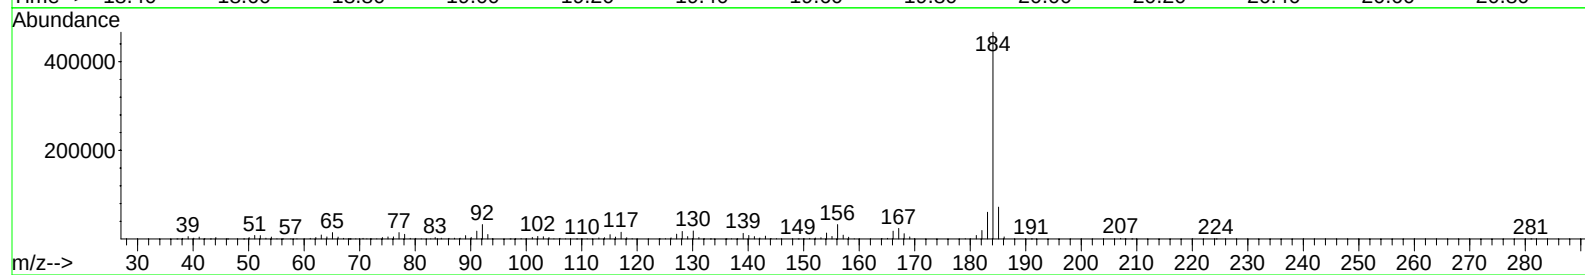


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG083018\
Data File : BG036481.D
Acq On : 30 Aug 2018 16:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 30 18:23:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 23 12:07:02 2018
Response via : Initial Calibration

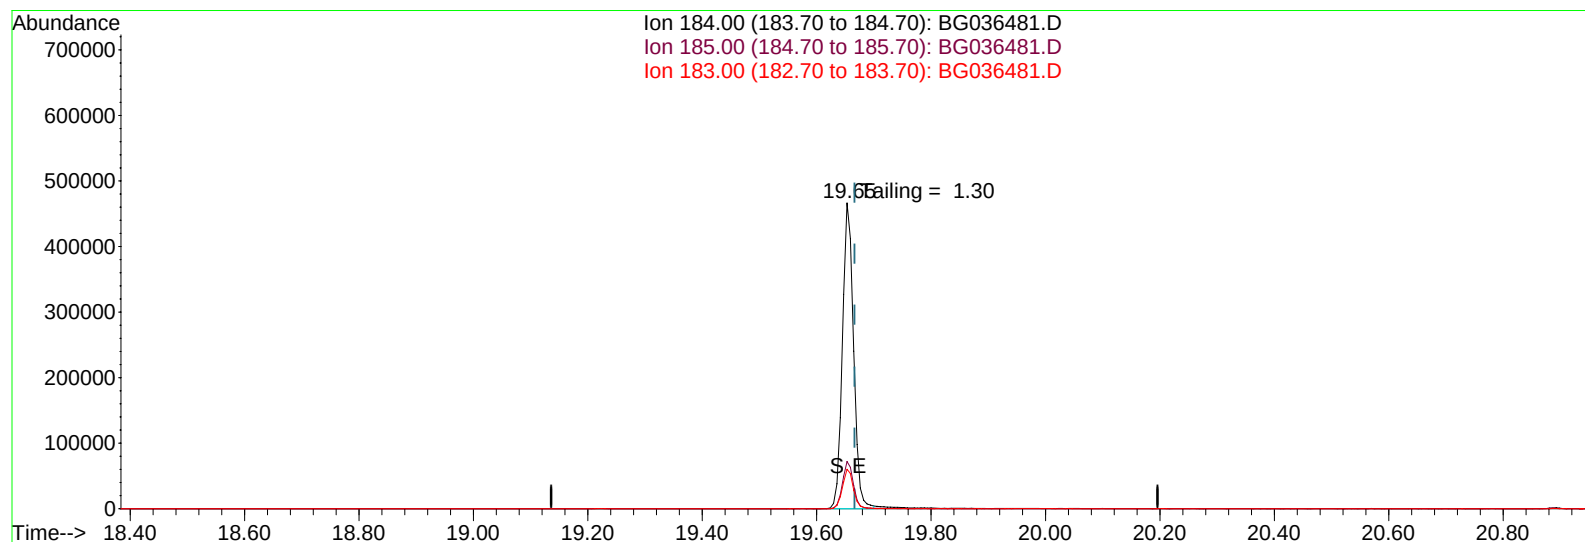

(76) Benzidine




19.653min (-0.013) 0.00ng

response 640879

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.43
183.00	13.60	12.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG083018\
Data File : BG036481.D
Acq On : 30 Aug 2018 16:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 30 18:23:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 23 12:07:02 2018
Response via : Initial Calibration

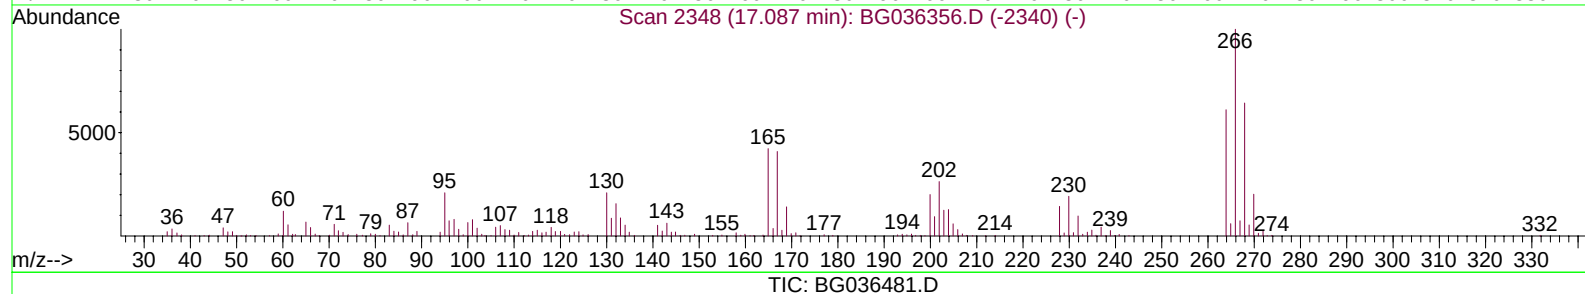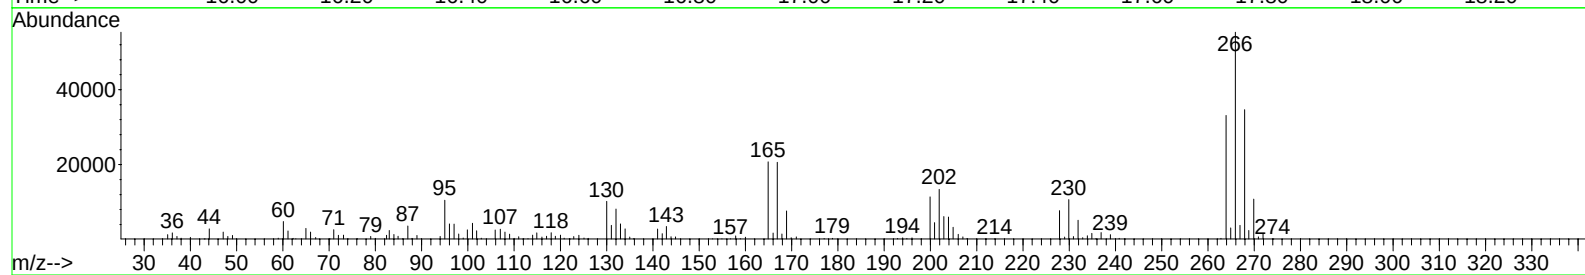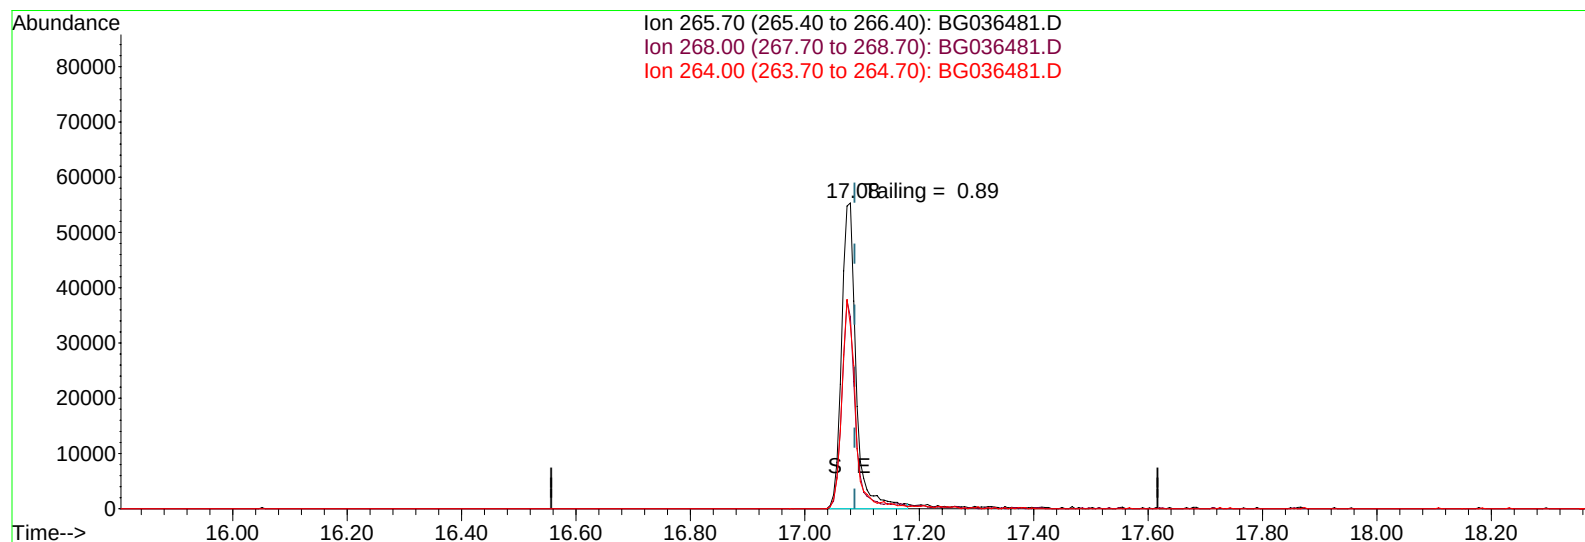

(69) Pentachlorophenol (C)

17.080min (-0.007) 196496.22ng

response 97526

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	62.67
264.00	61.10	59.84
0.00	0.00	0.00