

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG083018\
 Data File : BG036488.D
 Acq On : 30 Aug 2018 21:26
 Operator : JU/SJ
 Sample : J4663-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 6722AA

Quant Time: Aug 31 01:39:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 23 12:07:02 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	62638	20.00	ng	0.00
21) Naphthalene-d8	10.87	136	251170	20.00	ng	-0.02
38) Acenaphthene-d10	14.69	164	159548	20.00	ng	-0.02
63) Phenanthrene-d10	17.43	188	413911	20.00	ng	0.00
75) Chrysene-d12	21.69	240	450307	20.00	ng	-0.02
86) Perylene-d12	24.91	264	441295	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	455910	115.46	ng	0.00
7) Phenol-d6	7.22	99	585086	103.49	ng	0.00
23) Nitrobenzene-d5	9.22	82	428258	92.51	ng	-0.02
41) 2,4,6-Tribromophenol	16.17	330	254886	133.89	ng	0.00
44) 2-Fluorobiphenyl	13.31	172	1008996	90.30	ng	-0.02
78) Terphenyl-d14	20.04	244	1691201	87.78	ng	-0.02
Target Compounds						Qvalue
49) Dimethylphthalate	14.13	163	101717	7.808	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG083018\
Data File : BG036488.D
Acq On : 30 Aug 2018 21:26
Operator : JU/SJ
Sample : J4663-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
6722AA

Quant Time: Aug 31 01:39:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 23 12:07:02 2018
Response via : Initial Calibration

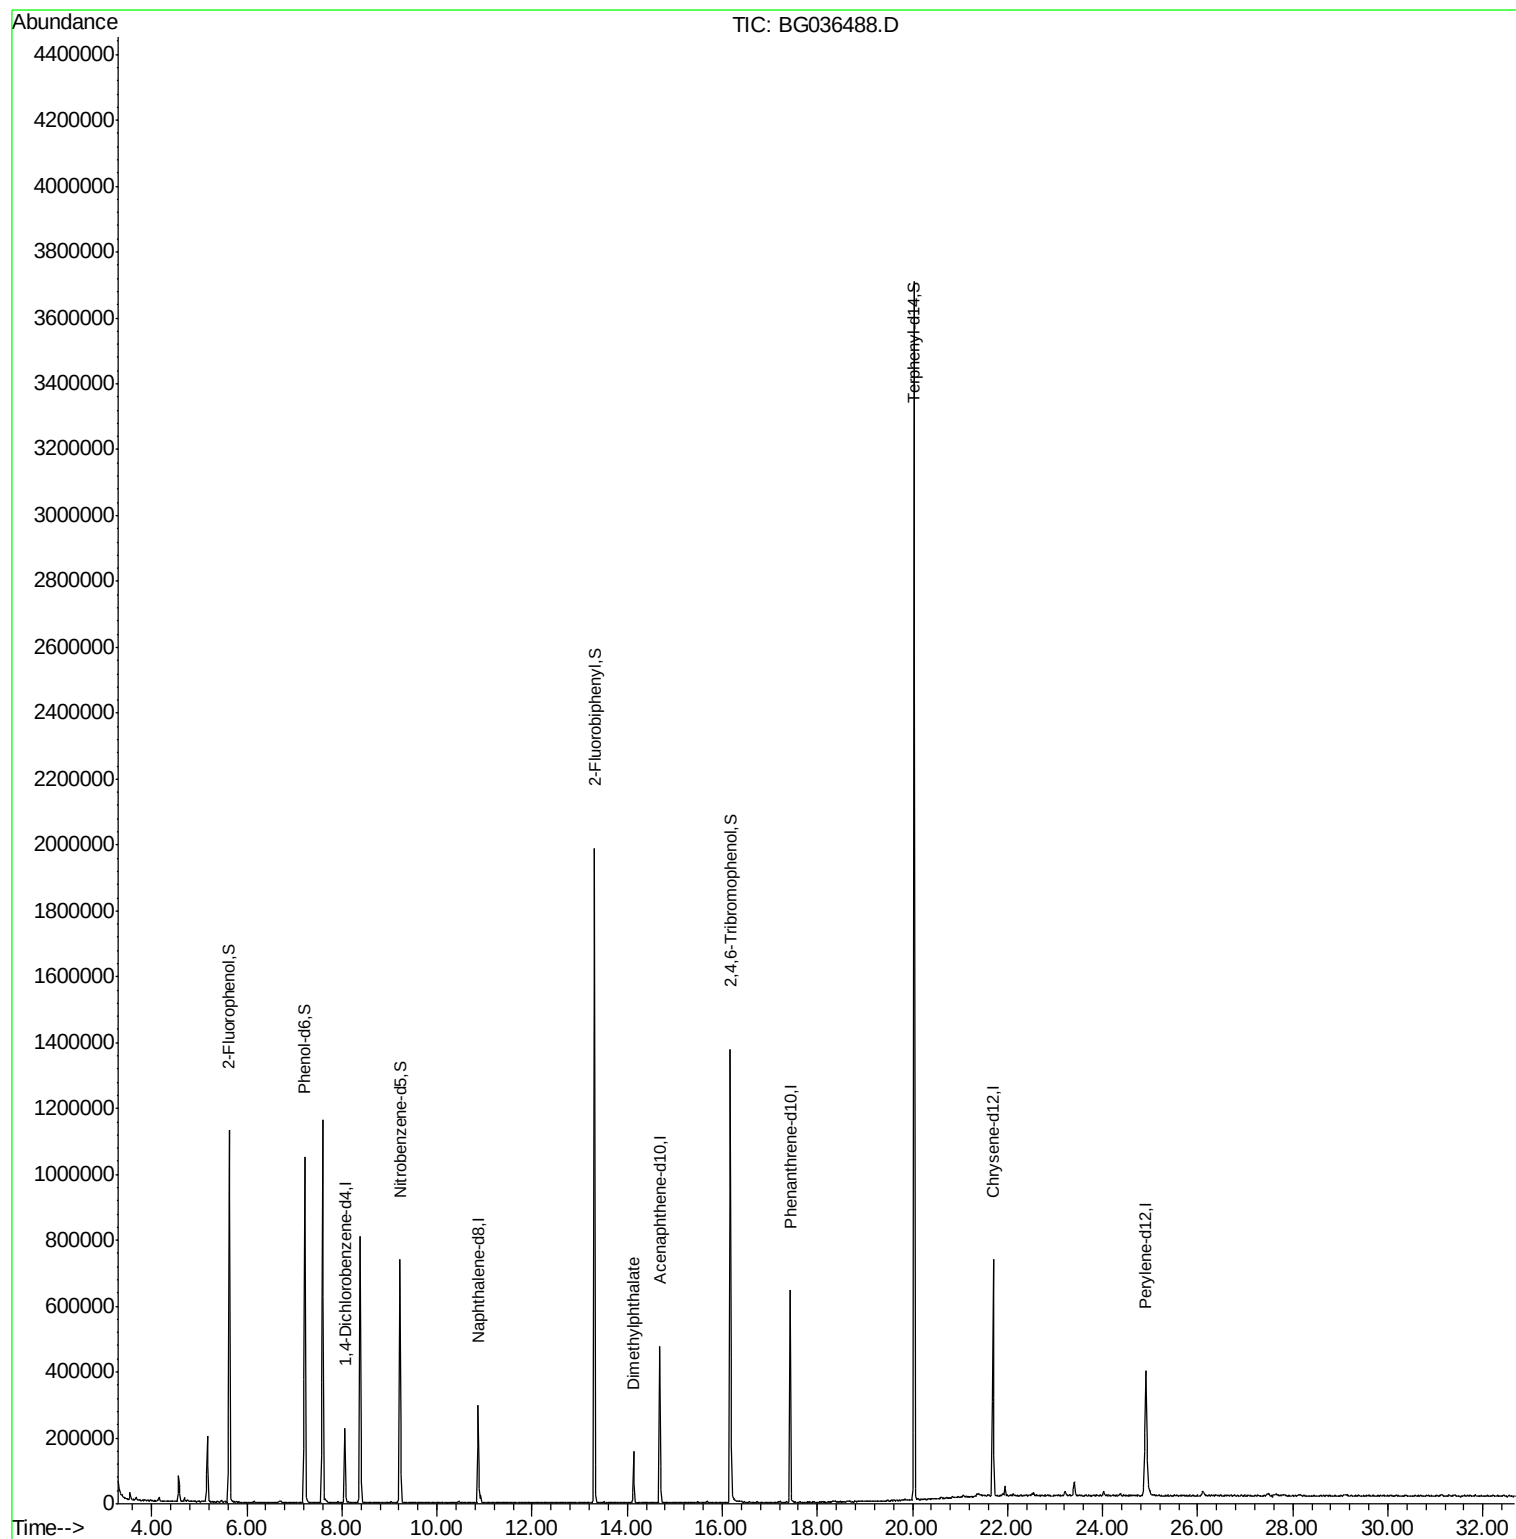

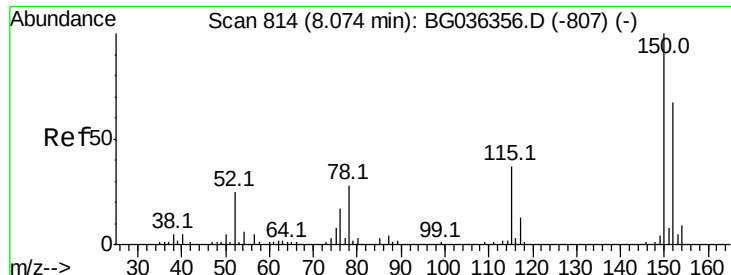


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.06 min Scan# 813
Delta R.T. -0.01 min
Lab File: BG036488.D
Acq: 30 Aug 2018 21:26

Instrument :
BNA_G
ClientSampleId :
6722AA

Tot Ion	Ratio	Lower	Upper
152	100		
150	145.9	119.5	179.3
115	56.5	44.5	66.7



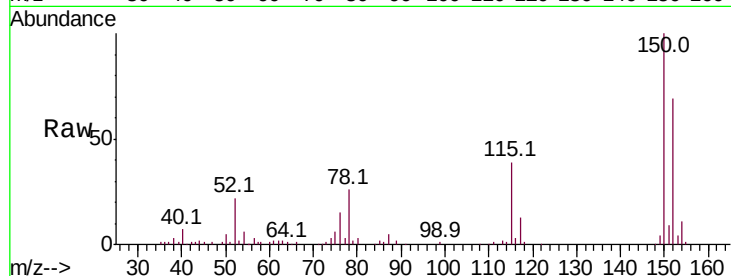


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

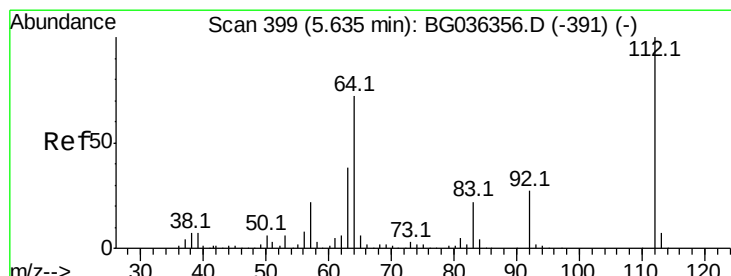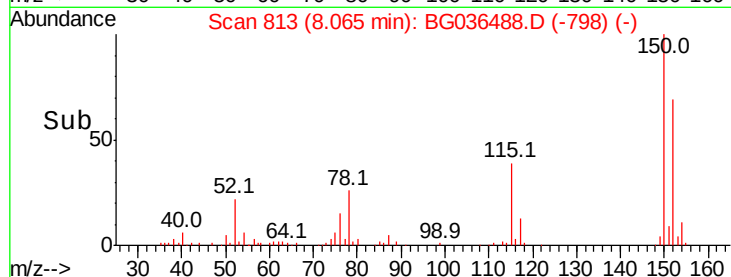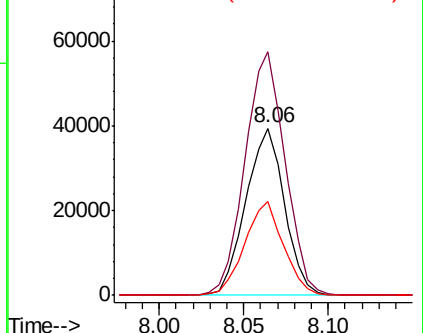

#5

2-Fluorophenol
Concen: 115.458 ng
RT: 5.63 min Scan# 399
Delta R.T. -0.00 min
Lab File: BG036488.D
Acq: 30 Aug 2018 21:26

Tgt Ion	Ratio	Lower	Upper
112	100		
64	69.8	57.2	85.8
63	37.9	30.8	46.2


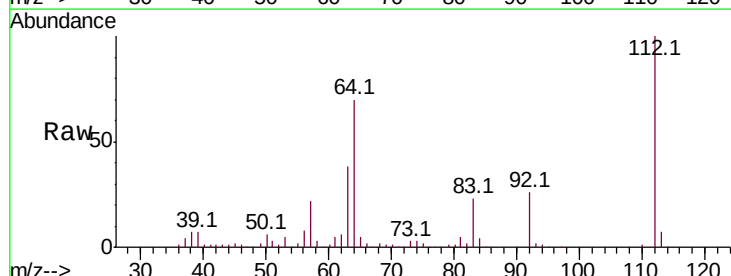



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

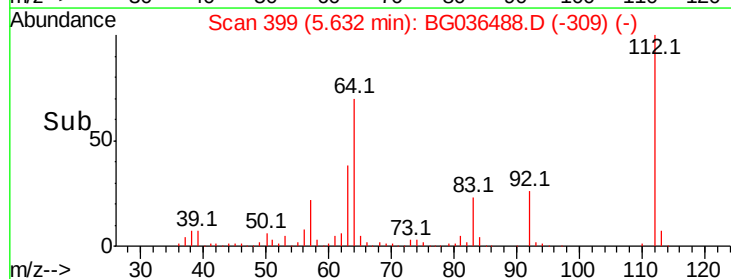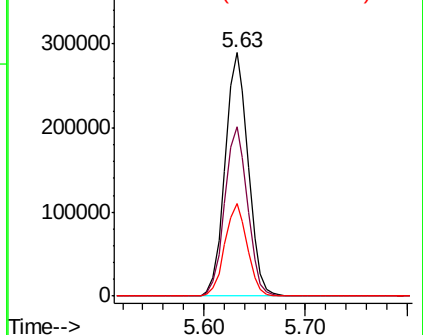

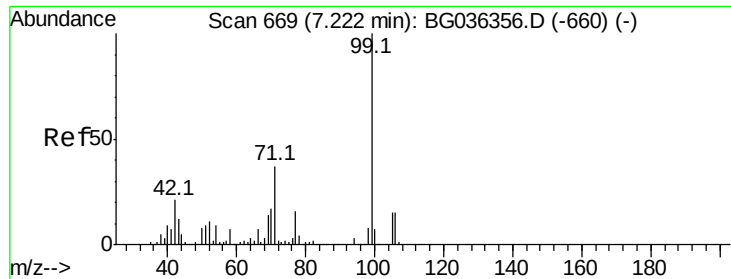

#7

Phenol-d6

Concen: 103.490 ng

RT: 7.22 min Scan# 669

Delta R.T. -0.00 min

Lab File: BG036488.D

Acq: 30 Aug 2018 21:26

Instrument :

BNA_G

ClientSampleId :

6722AA


Tot Ion: 99 Resp: 585086

Ion Ratio Lower Upper




99 100

42 20.8 16.5 24.7

71 36.2 29.4 44.2

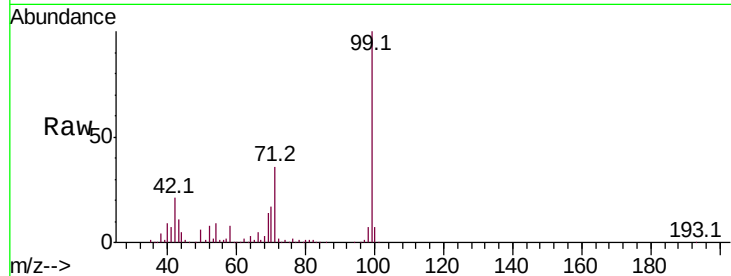

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

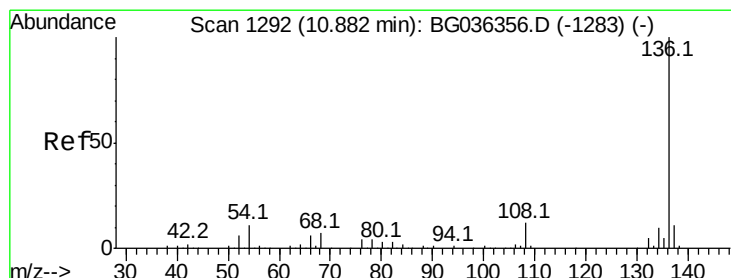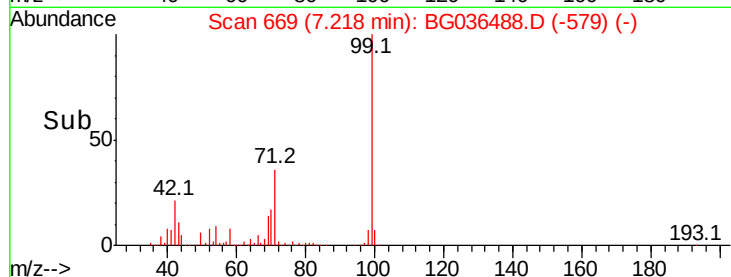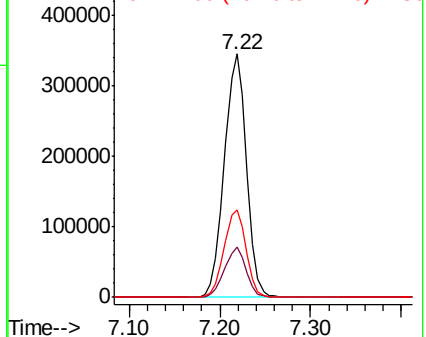

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.87 min Scan# 1290

Delta R.T. -0.02 min

Lab File: BG036488.D

Acq: 30 Aug 2018 21:26

Tgt Ion: 136 Resp: 251170


Ion Ratio Lower Upper

136 100



137 10.5 8.8 13.2


54 10.5 9.2 13.8

68 6.4 5.8 8.6

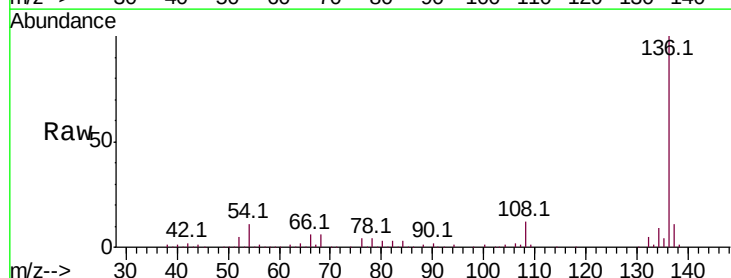

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



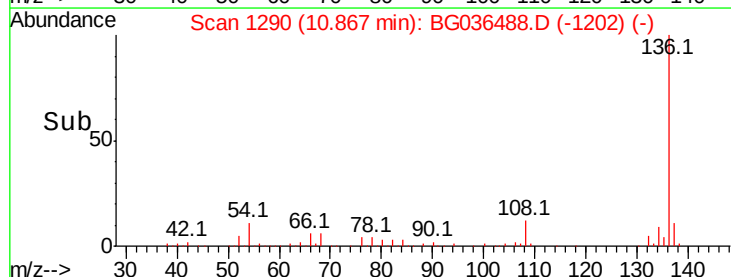
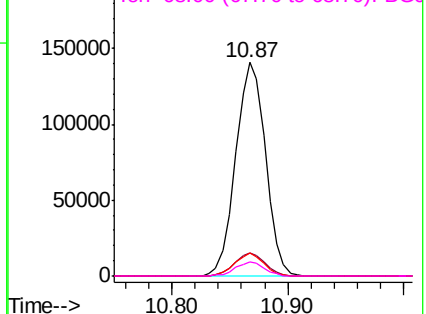


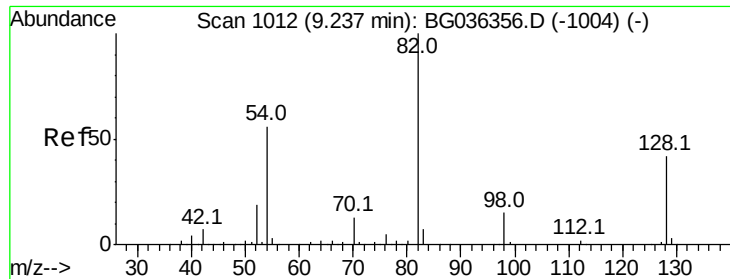

#23
Nitrobenzene-d5
Concen: 92.511 ng
RT: 9.22 min Scan# 1010
Delta R.T. -0.02 min
Lab File: BG036488.D
Acq: 30 Aug 2018 21:26




Instrument :
BNA_G
ClientSampleId :
6722AA


Tot Ion	Ratio	Lower	Upper
82	100		
128	40.4	33.3	49.9
54	54.7	45.1	67.7

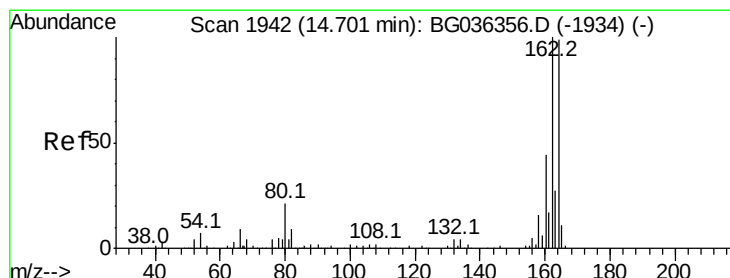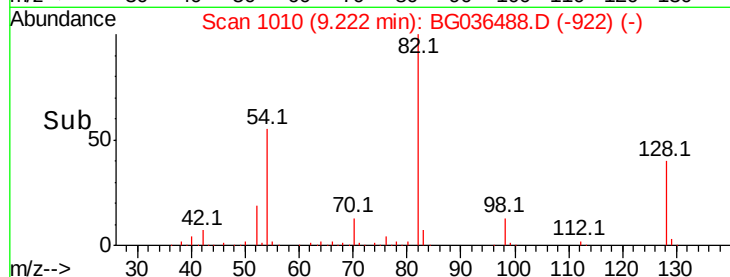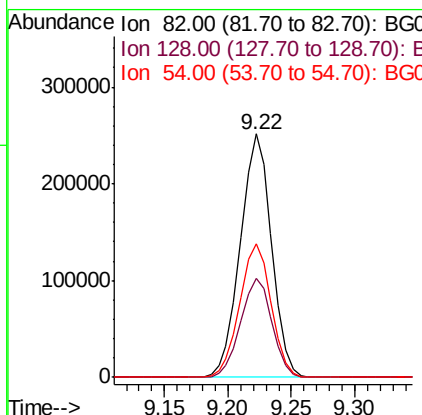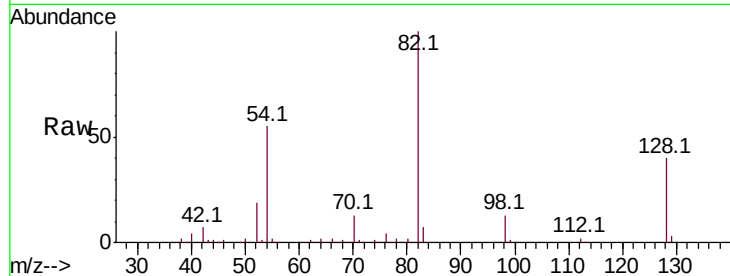

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.69 min Scan# 1940
Delta R.T. -0.02 min
Lab File: BG036488.D
Acq: 30 Aug 2018 21:26

Tgt Ion	Ratio	Lower	Upper
164	100		
162	105.9	80.7	121.1
160	45.8	35.3	52.9

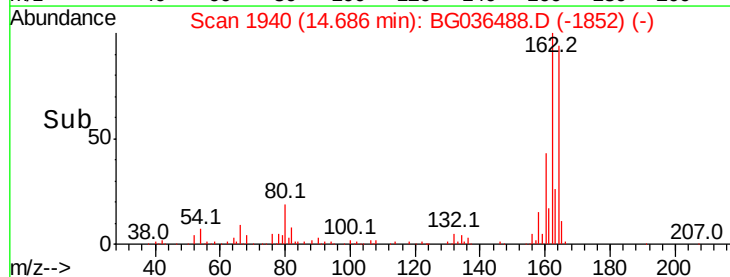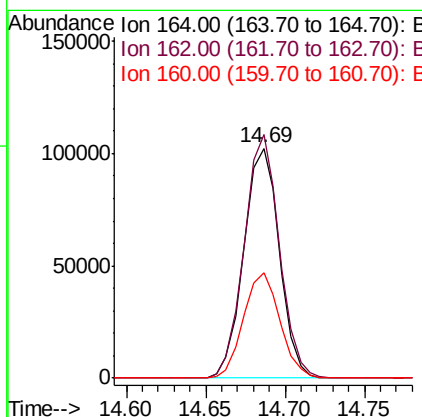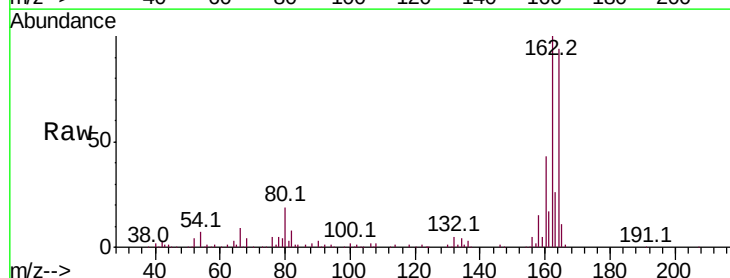


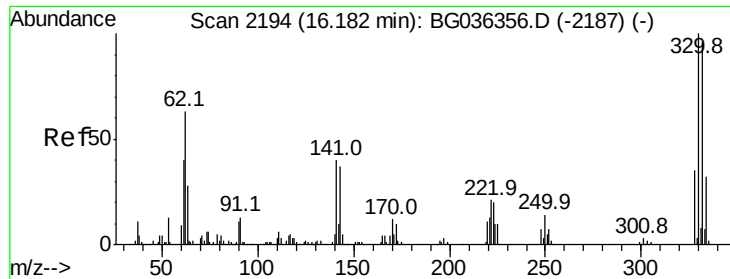




#41
 2,4,6-Tribromophenol
 Concen: 133.885 ng
 RT: 16.17 min Scan# 2193
 Delta R.T. -0.01 min
 Lab File: BG036488.D
 Acq: 30 Aug 2018 21:26

Instrument :
 BNA_G
 ClientSampled :
 6722AA

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.7	75.4	113.2
141	37.7	30.7	46.1

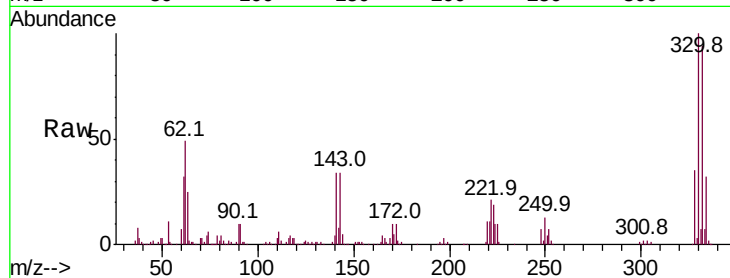


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

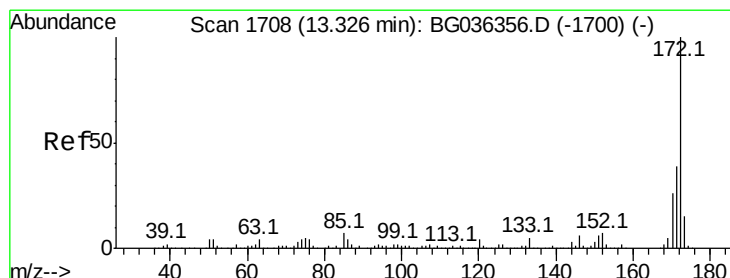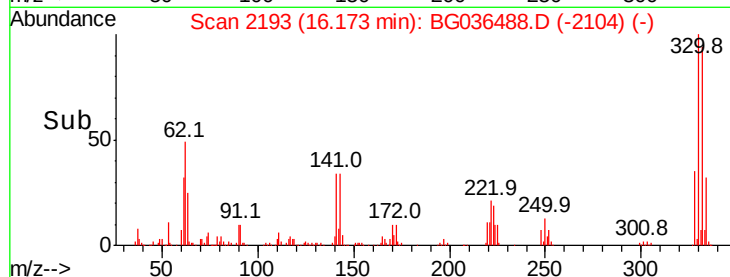
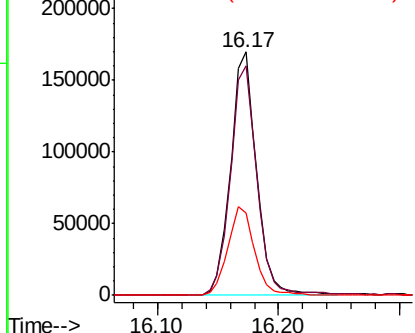



#44
 2-Fluorobiphenyl
 Concen: 90.297 ng
 RT: 13.31 min Scan# 1706
 Delta R.T. -0.02 min
 Lab File: BG036488.D
 Acq: 30 Aug 2018 21:26

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.4	31.3	46.9
170	25.2	21.0	31.6

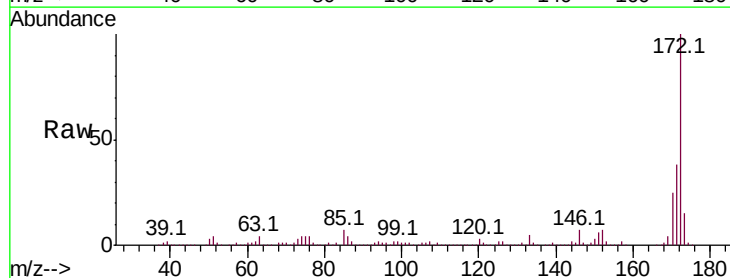

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

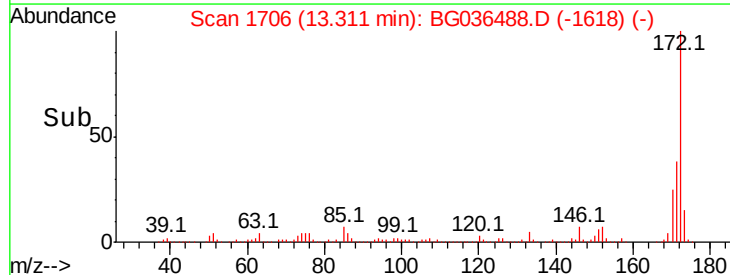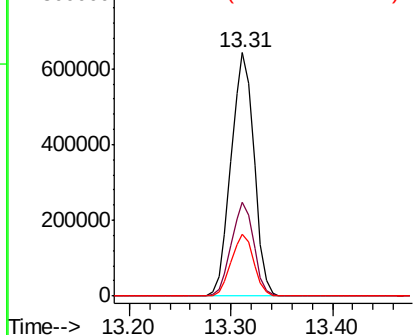

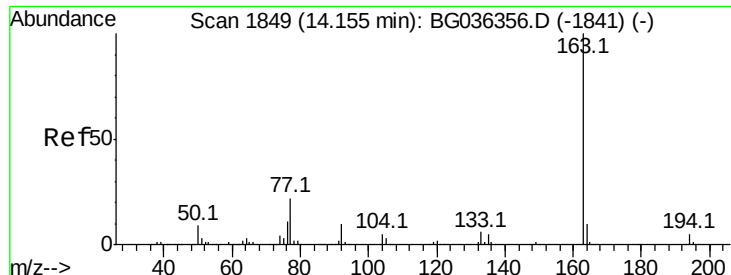

#49

Dimethylphthalate

Concen: 7.808 ng

RT: 14.13 min Scan# 1846

Delta R.T. -0.02 min

Lab File: BG036488.D

Acq: 30 Aug 2018 21:26

Instrument :

BNA_G

ClientSampleId :

6722AA


Tot Ion:163 Resp: 101717

Ion Ratio Lower Upper

163 100

194 5.7 4.0 6.0




164 10.0 8.1 12.1

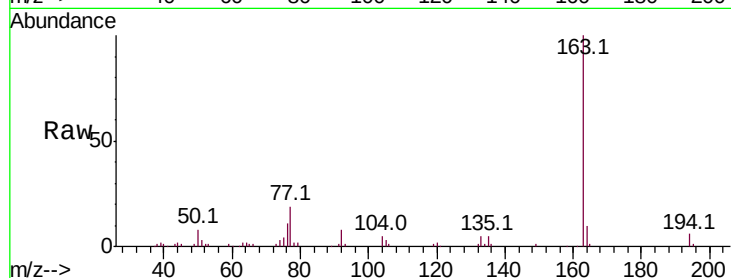

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

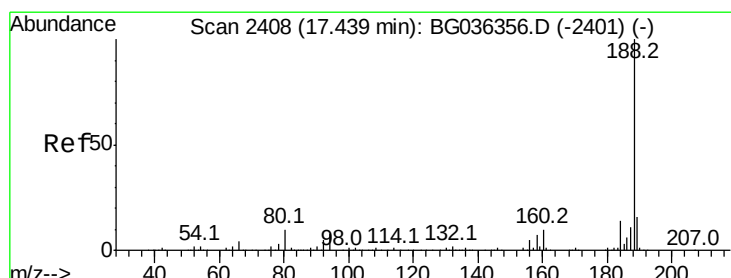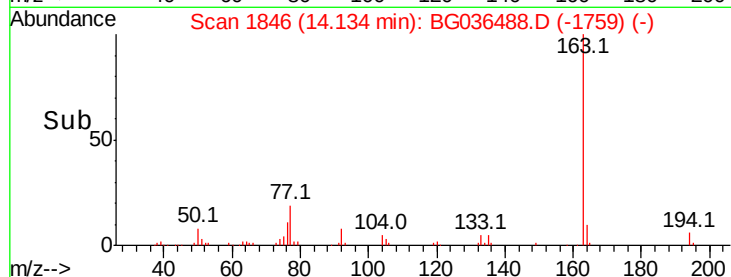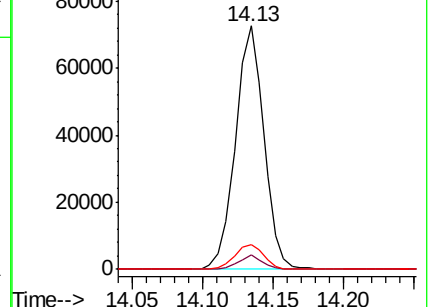

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.43 min Scan# 2407

Delta R.T. -0.01 min

Lab File: BG036488.D

Acq: 30 Aug 2018 21:26


Tgt Ion:188 Resp: 413911

Ion Ratio Lower Upper

188 100

94 7.6 6.7 10.1



80 8.6 8.1 12.1

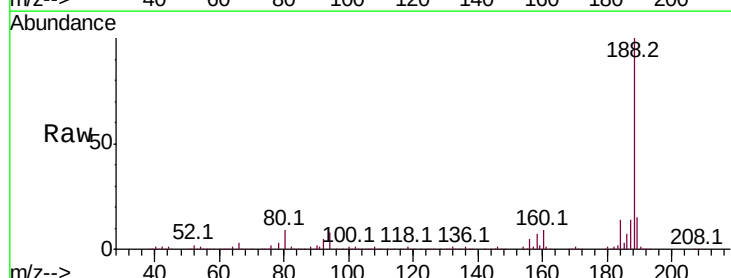


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

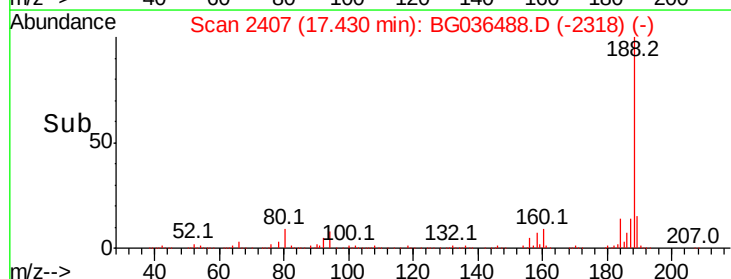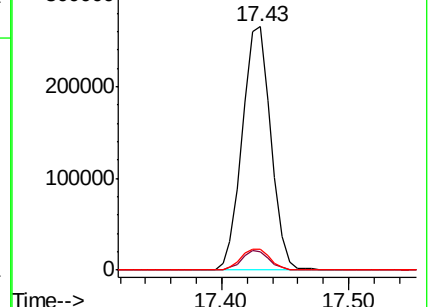

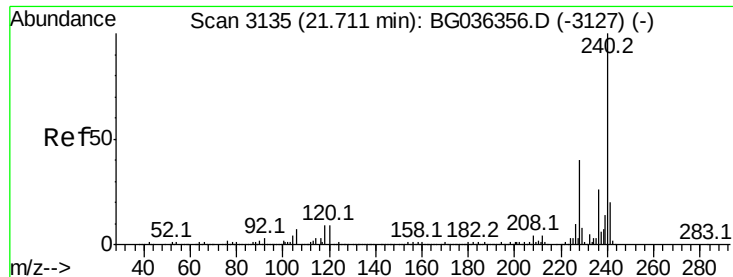

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.69 min Scan# 3132

Delta R.T. -0.02 min

Lab File: BG036488.D

Acq: 30 Aug 2018 21:26

Instrument :

BNA_G

ClientSampleId :

6722AA


Tot Ion:240 Resp: 450307

Ion Ratio Lower Upper

240 100

120 8.6 6.9 10.3




236 25.5 21.2 31.8

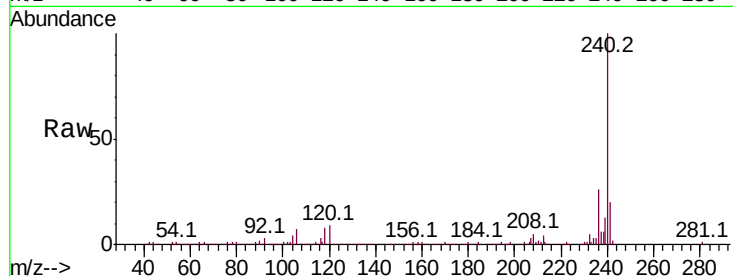

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

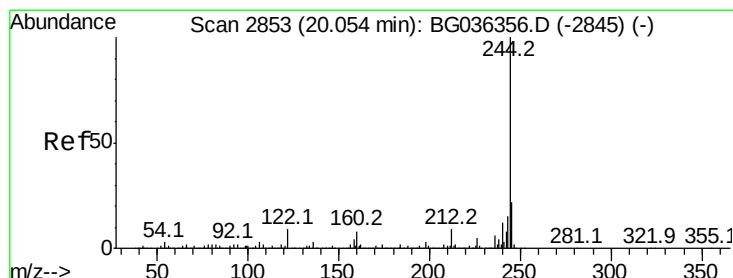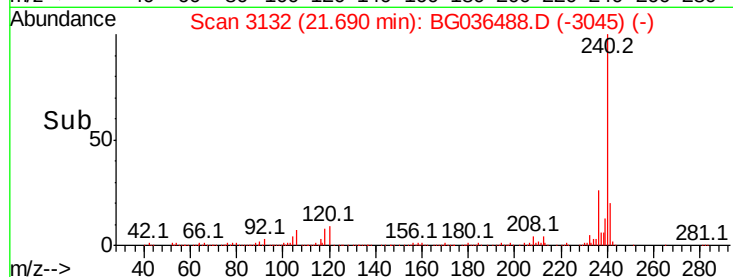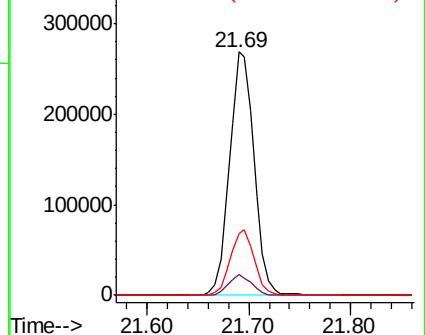

#78

Terphenyl-d14

Concen: 87.783 ng

RT: 20.04 min Scan# 2851

Delta R.T. -0.02 min

Lab File: BG036488.D

Acq: 30 Aug 2018 21:26


Tgt Ion:244 Resp: 1691201

Ion Ratio Lower Upper

244 100

212 9.5 7.0 10.6



122 9.3 7.1 10.7

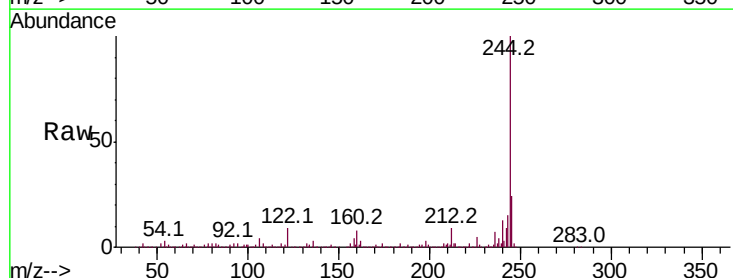


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

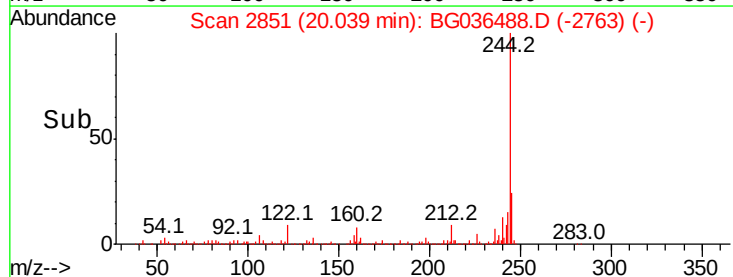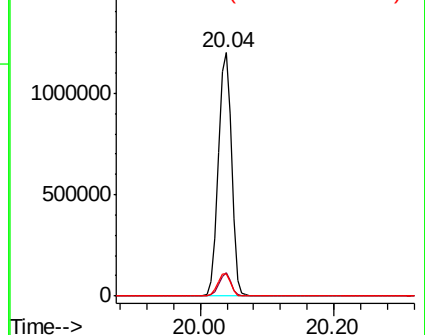

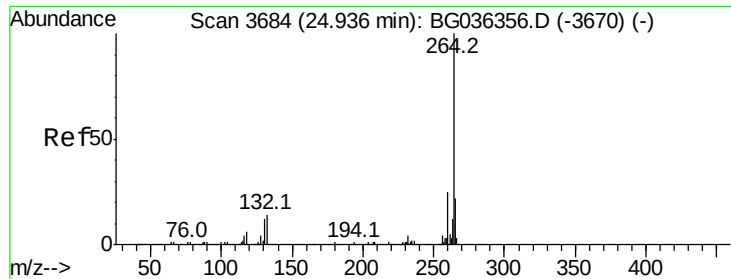

#86
Pervlene-d12
Concen: 20.000 ng
RT: 24.91 min Scan# 3680
Delta R.T. -0.03 min
Lab File: BG036488.D
Acq: 30 Aug 2018 21:26

Instrument :
BNA_G
ClientSampleId :
6722AA

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.9	19.6	29.4
265	21.4	17.4	26.0

