

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG083018\
 Data File : BG036497.D
 Acq On : 31 Aug 2018 3:19
 Operator : JU/SJ
 Sample : PB112500BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB112500BL

Quant Time: Aug 31 05:00:34 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 23 12:07:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	56089	20.00	ng	-0.01
21) Naphthalene-d8	10.86	136	237812	20.00	ng	-0.02
38) Acenaphthene-d10	14.68	164	163513	20.00	ng	-0.02
63) Phenanthrene-d10	17.43	188	436935	20.00	ng	-0.01
75) Chrysene-d12	21.69	240	478884	20.00	ng	-0.02
86) Perylene-d12	24.91	264	460220	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	432951	122.45	ng	0.00
7) Phenol-d6	7.22	99	612097	120.91	ng	0.00
23) Nitrobenzene-d5	9.22	82	353335	80.61	ng	-0.02
41) 2,4,6-Tribromophenol	16.17	330	220211	112.87	ng	-0.01
44) 2-Fluorobiphenyl	13.31	172	867745	75.77	ng	-0.02
78) Terphenyl-d14	20.04	244	1598744	78.03	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG083018\
Data File : BG036497.D
Acq On : 31 Aug 2018 3:19
Operator : JU/SJ
Sample : PB112500BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB112500BL

Quant Time: Aug 31 05:00:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 23 12:07:02 2018
Response via : Initial Calibration

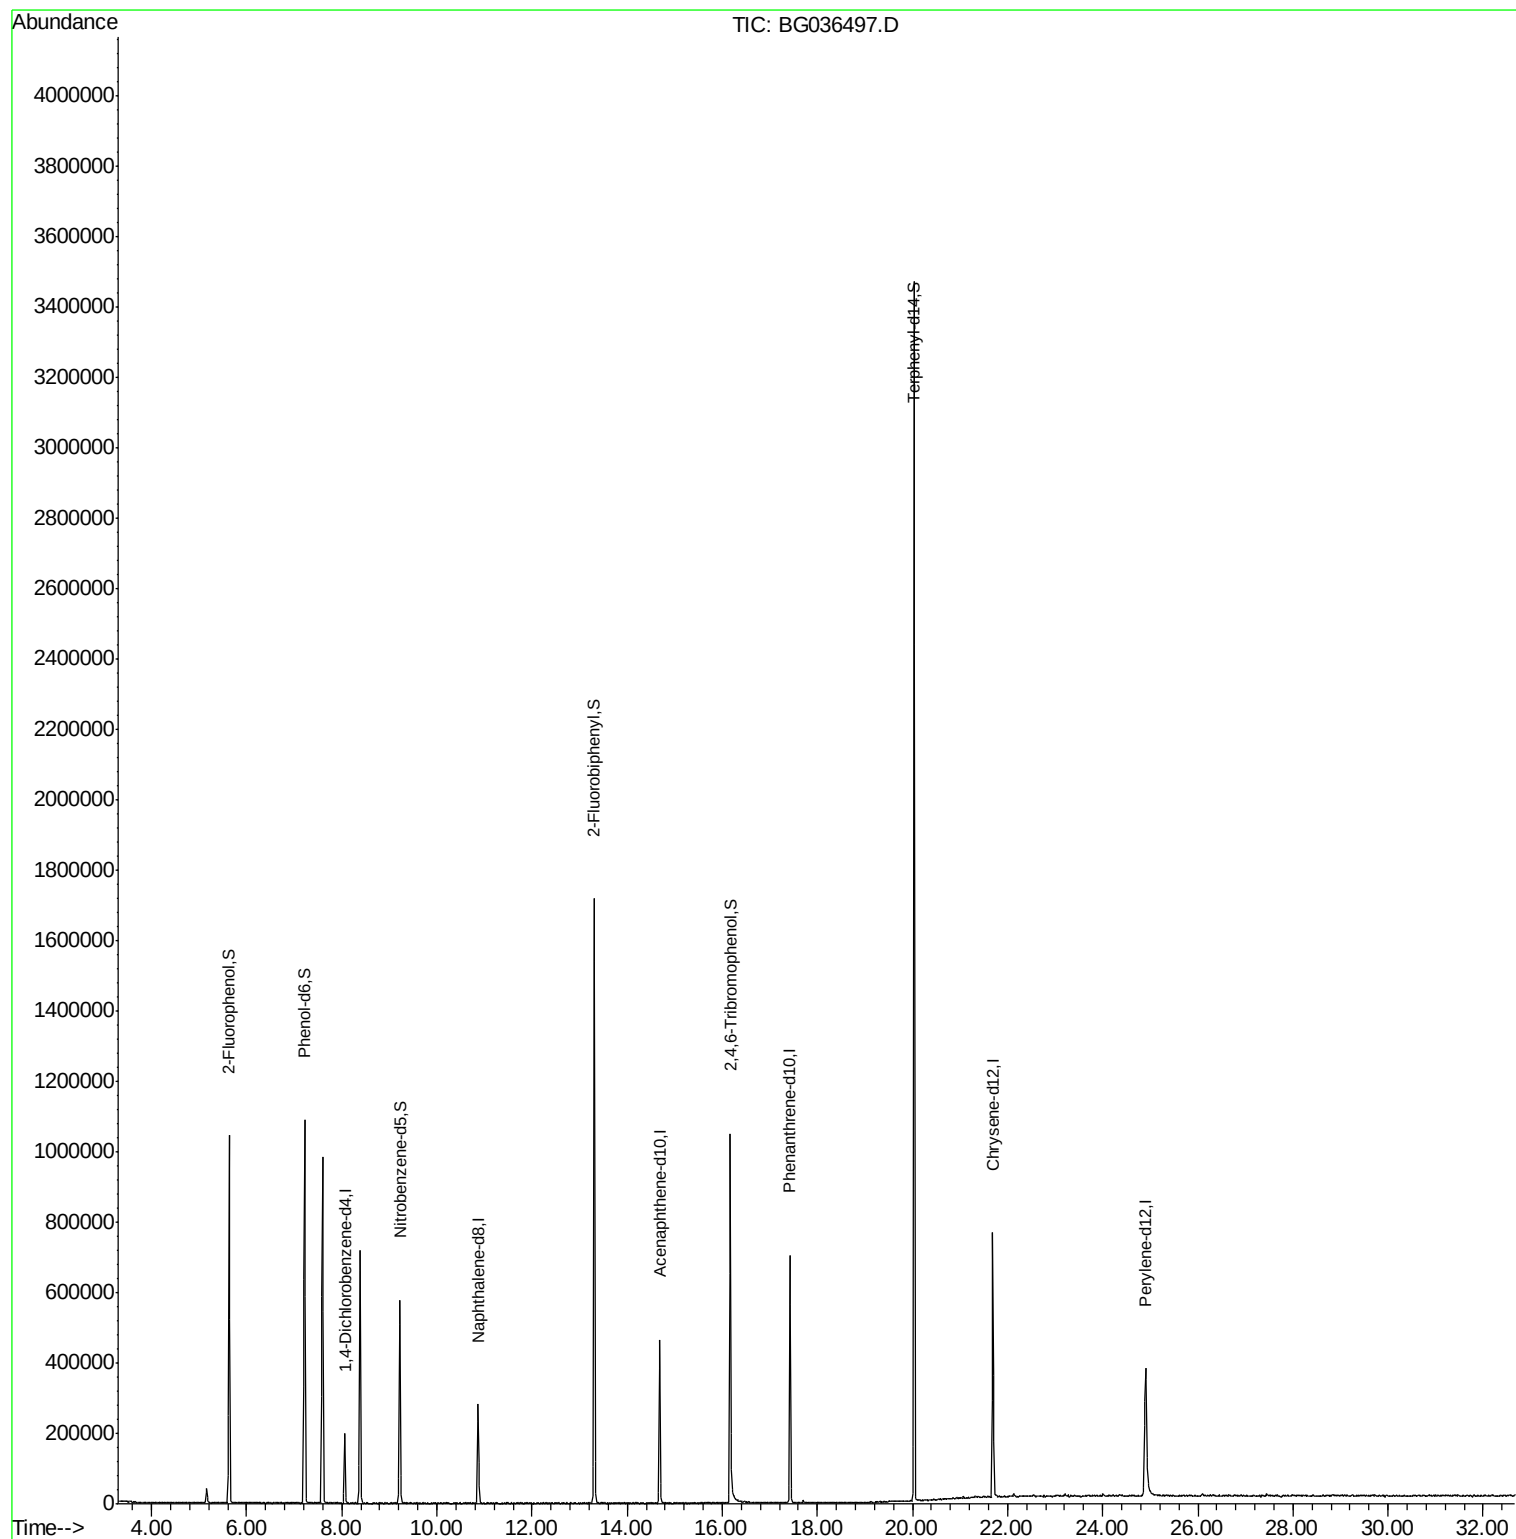

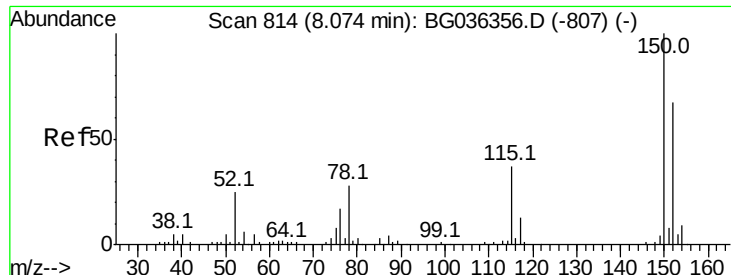


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.06 min Scan# 812
Delta R.T. -0.01 min
Lab File: BG036497.D
Acq: 31 Aug 2018 3:19

Instrument :
BNA_G
ClientSampleId :
PB112500BL

Tot Ion	Ratio	Lower	Upper
152	100		
150	148.3	119.5	179.3
115	58.9	44.5	66.7



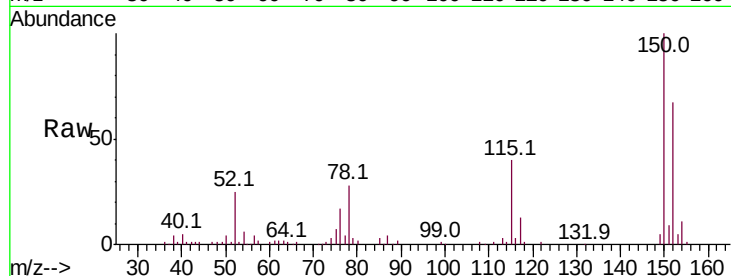


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

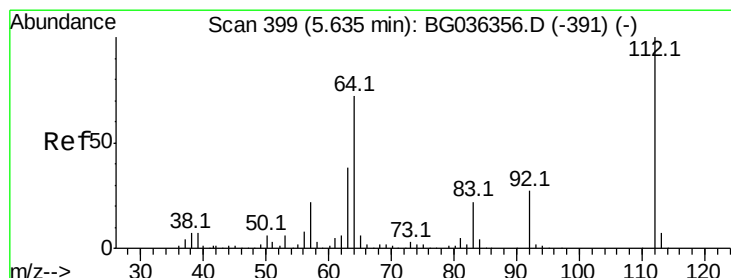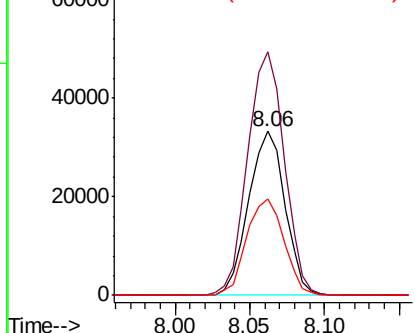

#5

2-Fluorophenol
Concen: 122.446 ng
RT: 5.63 min Scan# 398
Delta R.T. -0.01 min
Lab File: BG036497.D
Acq: 31 Aug 2018 3:19

Tgt Ion	Ratio	Lower	Upper
112	100		
64	68.8	57.2	85.8
63	37.3	30.8	46.2


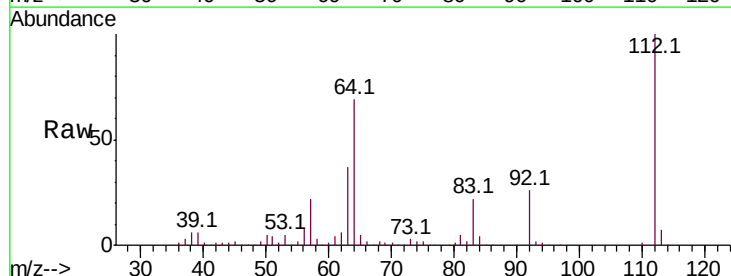



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

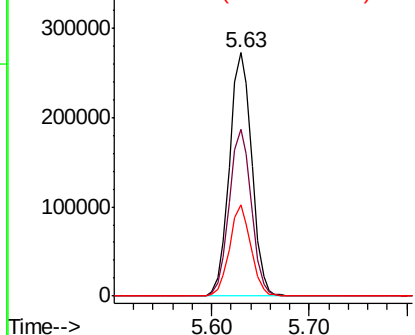

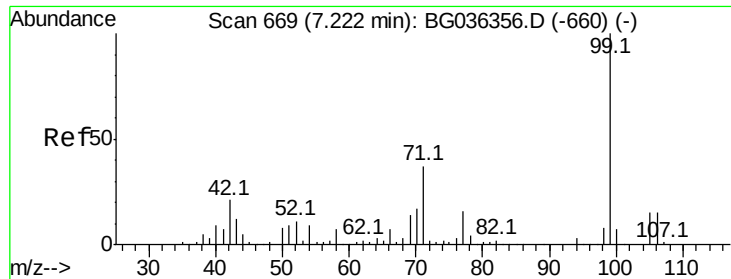

#7

Phenol-d6

Concen: 120.909 ng

RT: 7.22 min Scan# 668

Delta R.T. -0.01 min

Lab File: BG036497.D

Acq: 31 Aug 2018 3:19

Instrument :

BNA_G

ClientSampleId :

PB112500BL


Tot Ion: 99 Resp: 612097

Ion Ratio Lower Upper




99 100

42 18.6 16.5 24.7

71 35.1 29.4 44.2

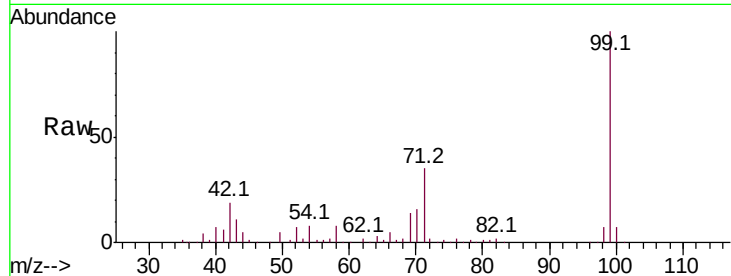

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

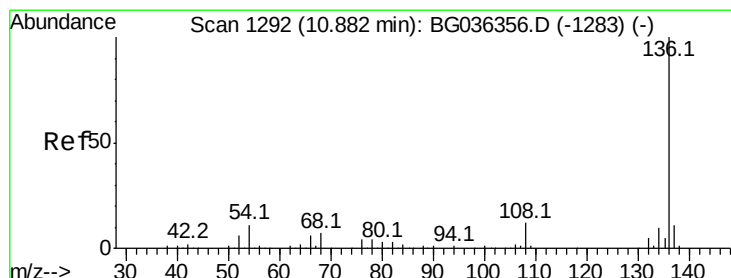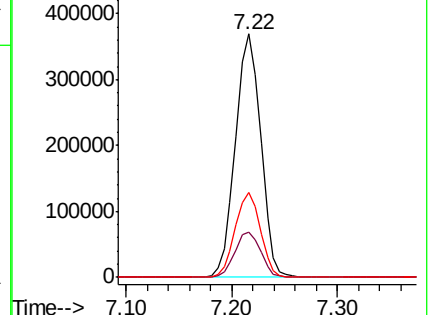

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1289

Delta R.T. -0.02 min

Lab File: BG036497.D

Acq: 31 Aug 2018 3:19

Tgt Ion: 136 Resp: 237812


Ion Ratio Lower Upper

136 100



137 11.8 8.8 13.2


54 10.7 9.2 13.8

68 6.5 5.8 8.6

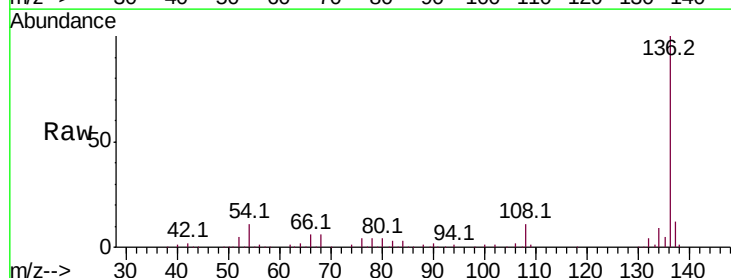

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



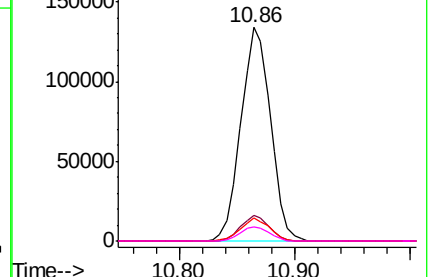





#23
 Nitrobenzene-d5
 Concen: 80.613 ng
 RT: 9.22 min Scan# 1009
 Delta R.T. -0.02 min
 Lab File: BG036497.D
 Acq: 31 Aug 2018 3:19




Instrument :
 BNA_G
 ClientSampleId :
 PB112500BL


Tot Ion	Ratio	Lower	Upper
82	100		
128	41.0	33.3	49.9
54	54.4	45.1	67.7

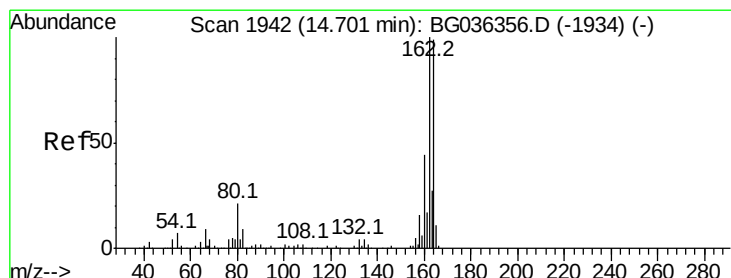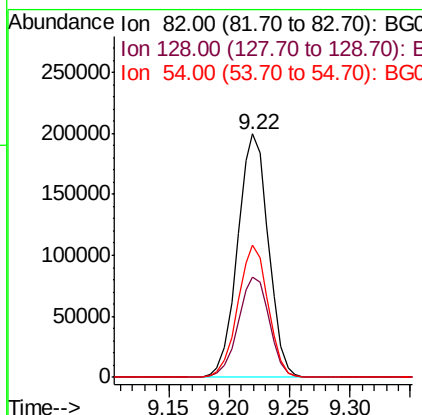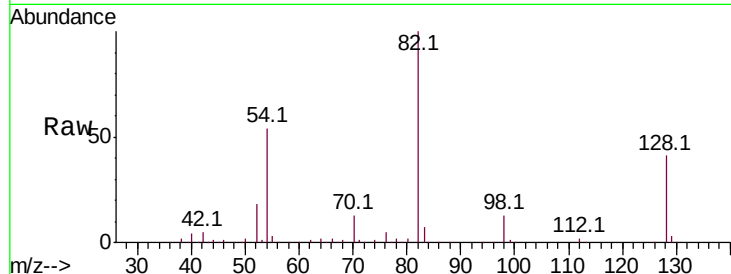

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.68 min Scan# 1939
 Delta R.T. -0.02 min
 Lab File: BG036497.D
 Acq: 31 Aug 2018 3:19

Tgt Ion	Ratio	Lower	Upper
164	100		
162	99.0	80.7	121.1
160	45.2	35.3	52.9

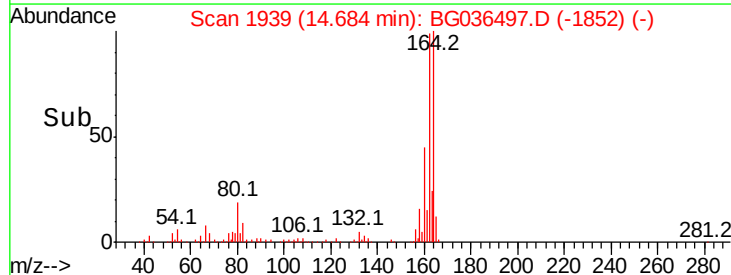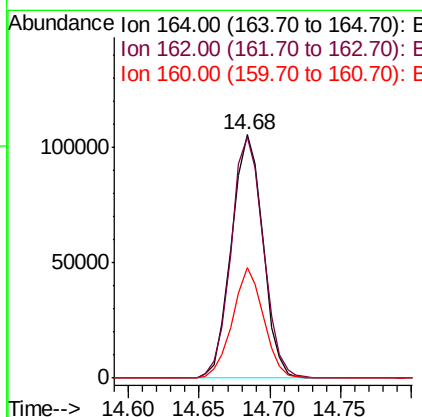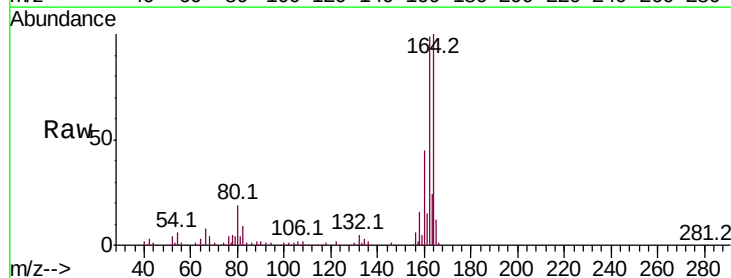


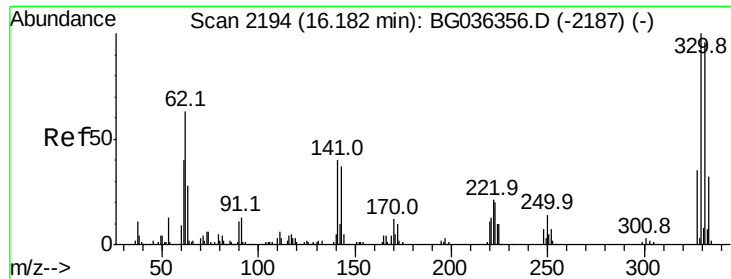




#41
 2,4,6-Tribromophenol
 Concen: 112.866 ng
 RT: 16.17 min Scan# 2192
 Delta R.T. -0.01 min
 Lab File: BG036497.D
 Acq: 31 Aug 2018 3:19

Instrument :
 BNA_G
 ClientSampleId :
 PB112500BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	93.0	75.4	113.2
141	35.1	30.7	46.1

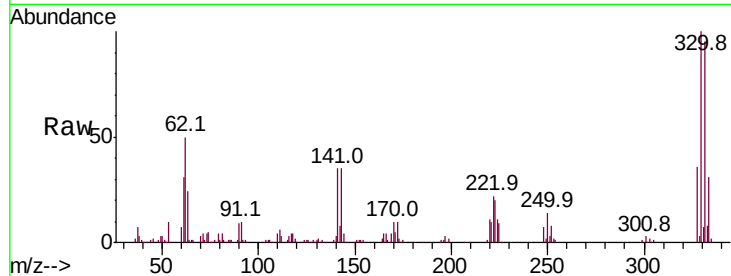


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

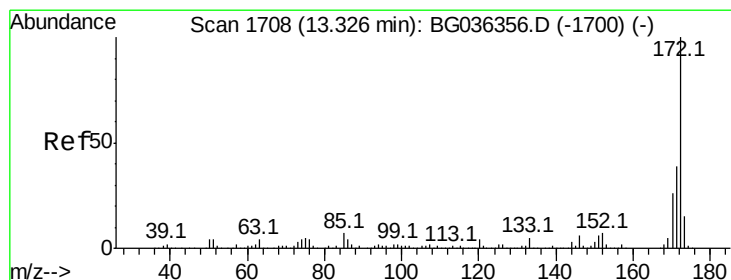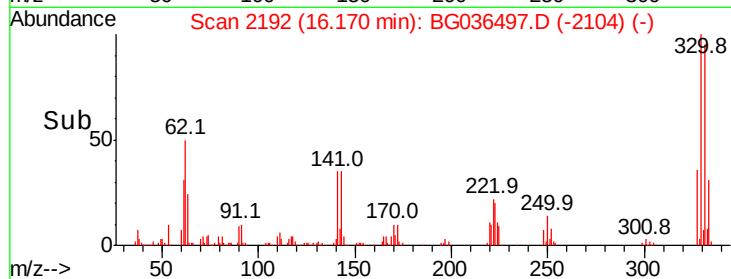
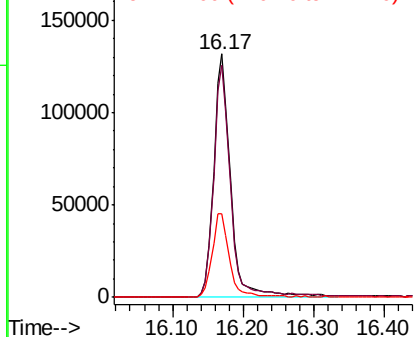



#44
 2-Fluorobiphenyl
 Concen: 75.773 ng
 RT: 13.31 min Scan# 1705
 Delta R.T. -0.02 min
 Lab File: BG036497.D
 Acq: 31 Aug 2018 3:19

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.9	31.3	46.9
170	24.9	21.0	31.6

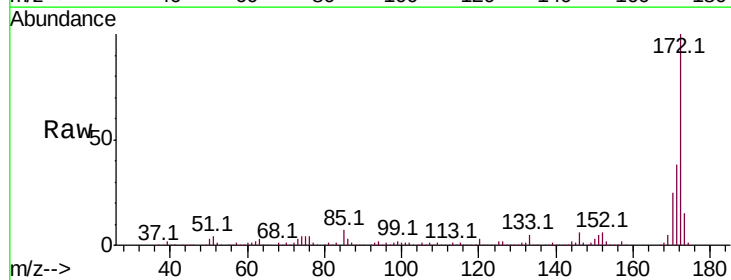

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E




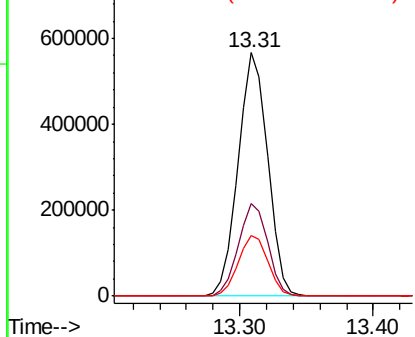




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.43 min Scan# 2406
Delta R.T. -0.01 min
Lab File: BG036497.D
Acq: 31 Aug 2018 3:19




Instrument :
BNA_G
ClientSampleId :
PB112500BL


Tot Ion:188 Resp: 436935
Ion Ratio Lower Upper
188 100
94 7.7 6.7 10.1
80 9.1 8.1 12.1

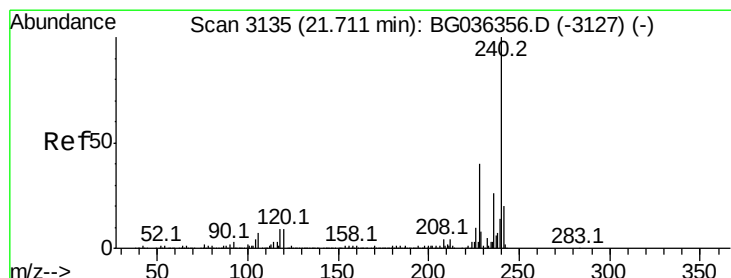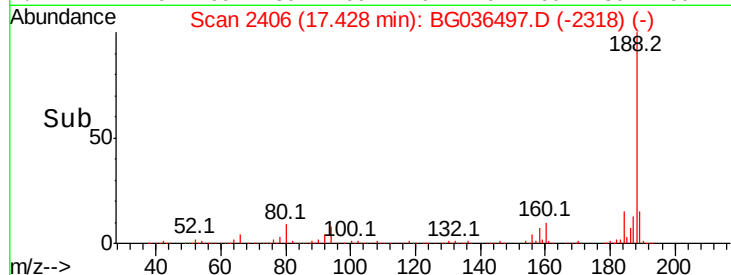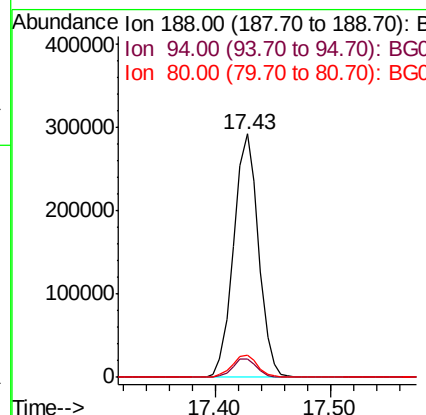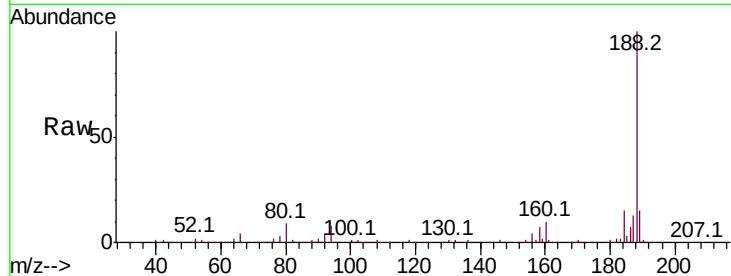

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.69 min Scan# 3132
Delta R.T. -0.02 min
Lab File: BG036497.D
Acq: 31 Aug 2018 3:19

Tgt Ion:240 Resp: 478884
Ion Ratio Lower Upper
240 100
120 8.0 6.9 10.3
236 25.6 21.2 31.8

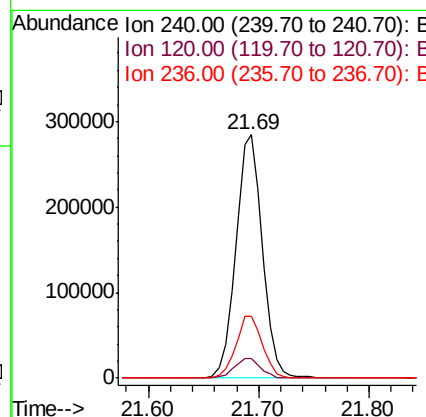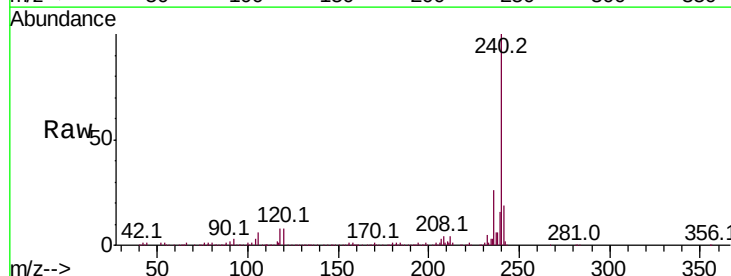



#78

Terphenyl-d14

Concen: 78.032 ng

RT: 20.04 min Scan# 2850

Delta R.T. -0.02 min

Lab File: BG036497.D

Acq: 31 Aug 2018 3:19

Instrument :

BNA_G

ClientSampleId :

PB112500BL


Tot Ion:244 Resp: 1598744

Ion Ratio Lower Upper




244 100

212 9.0 7.0 10.6

122 9.5 7.1 10.7

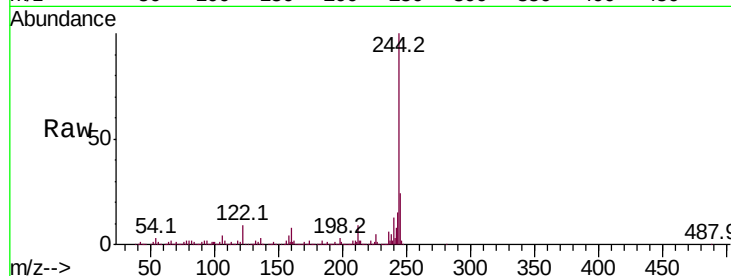

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

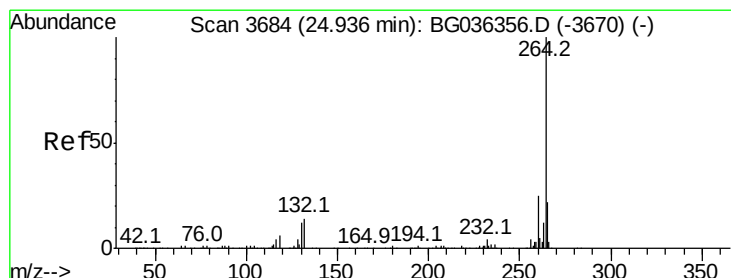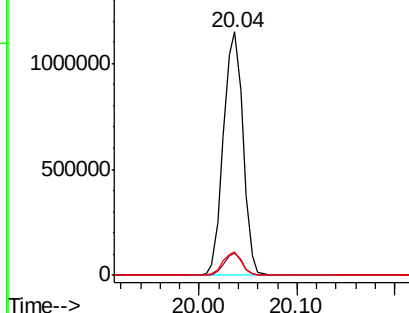

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.91 min Scan# 3679

Delta R.T. -0.03 min

Lab File: BG036497.D

Acq: 31 Aug 2018 3:19


Tgt Ion:264 Resp: 460220

Ion Ratio Lower Upper

264 100

260 24.2 19.6 29.4

265 21.5 17.4 26.0

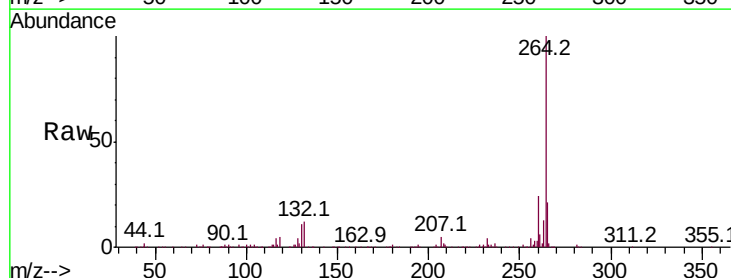

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

