


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG083018\
 Data File : BG036481.D
 Acq On : 30 Aug 2018 16:52
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 31 13:03:20 2018

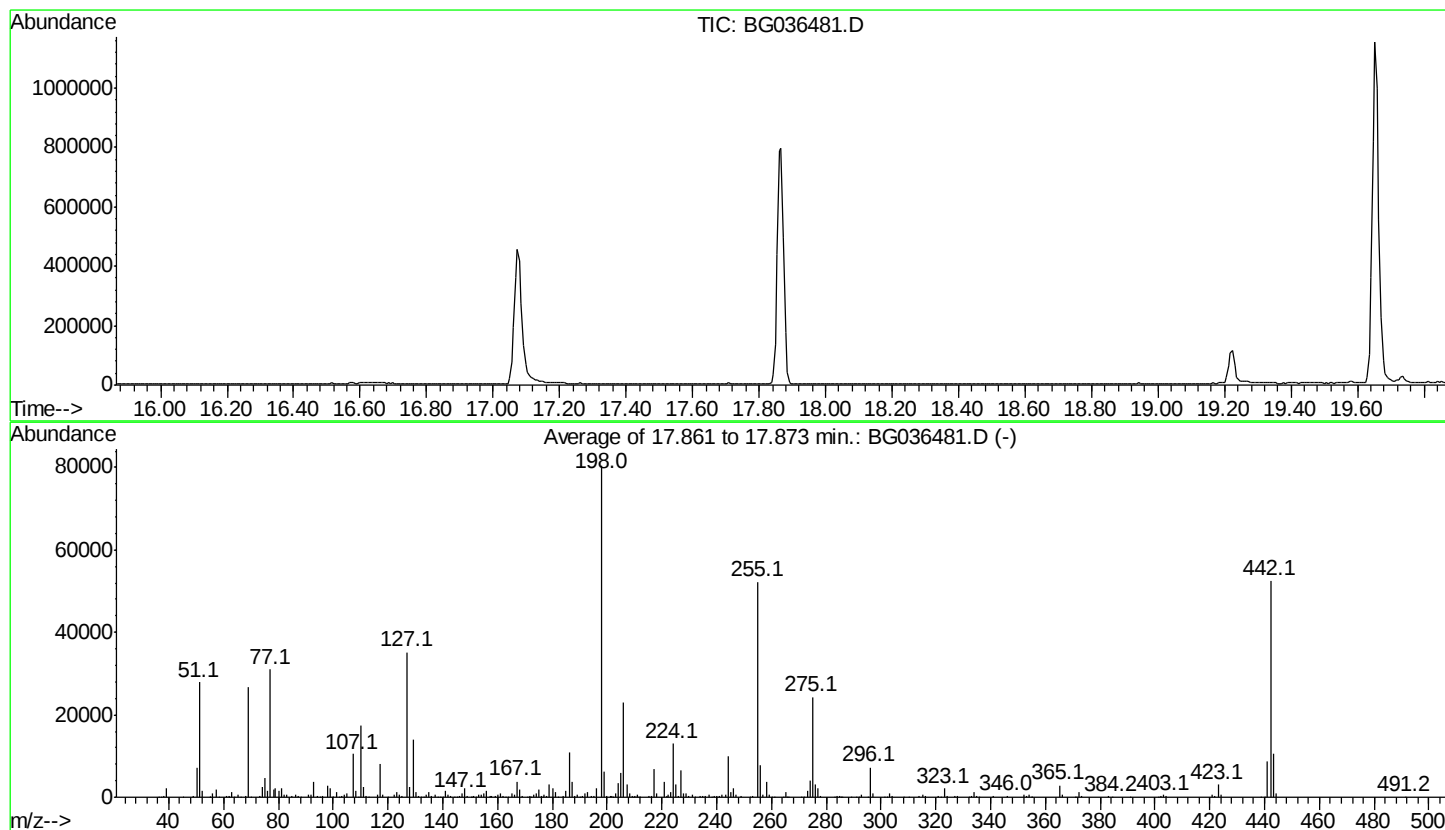

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	27914	PASS
68	69	0.00	2	0.6	171	PASS
69	198	0.00	100	33.4	26864	PASS
70	69	0.00	2	0.6	151	PASS
127	198	10	80	43.6	35109	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	80458	PASS
199	198	5	9	7.7	6161	PASS
275	198	10	60	30.3	24357	PASS
365	198	1	100	3.6	2909	PASS
441	198	0.01	100	10.8	8658	PASS
442	198	50	100	65.3	52514	PASS
443	442	15	24	20.1	10559	PASS