
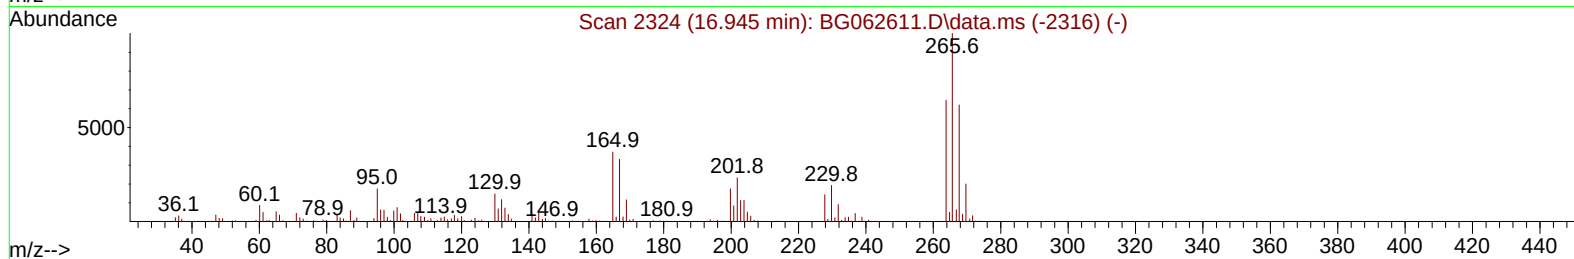
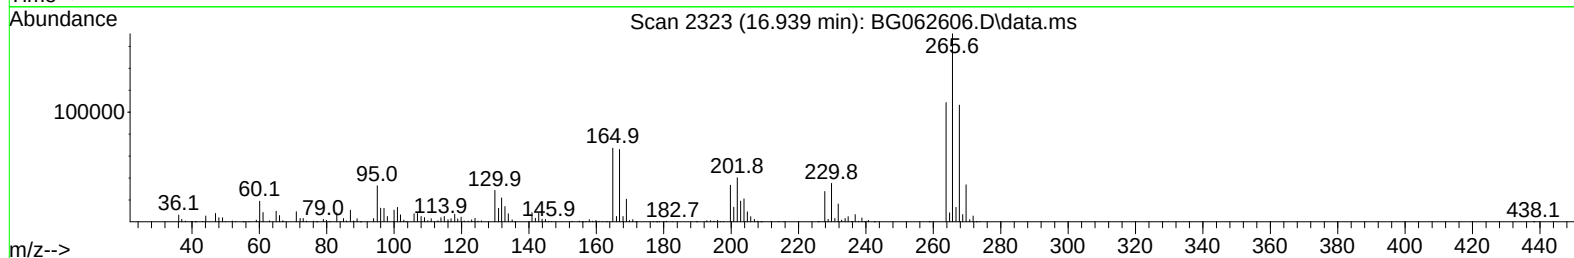


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG083024\  
Data File : BG062606.D  
Acq On : 30 Aug 2024 6:44  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 30 12:54:31 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG083024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 30 12:30:23 2024  
Response via : Initial Calibration

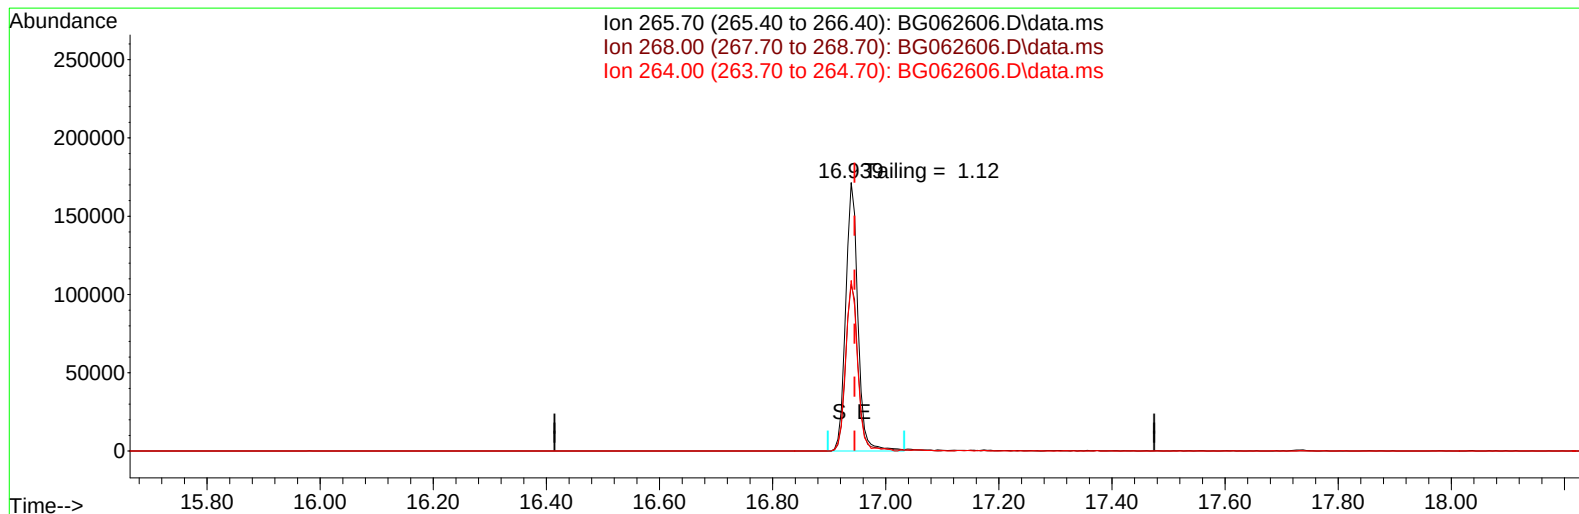

TIC: BG062606.D\data.ms

**(70) Pentachlorophenol (C)**




16.939min (-0.006) 54426.83 ng

response 257427

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.80  | 65.96  |
| 264.00 | 64.50  | 63.48  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG083024\  
Data File : BG062606.D  
Acq On : 30 Aug 2024 6:44  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 30 12:54:31 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG083024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 30 12:30:23 2024  
Response via : Initial Calibration

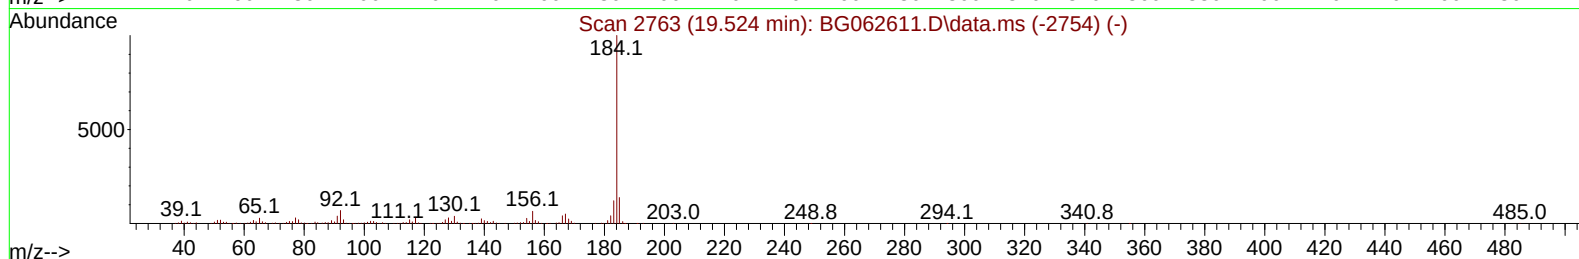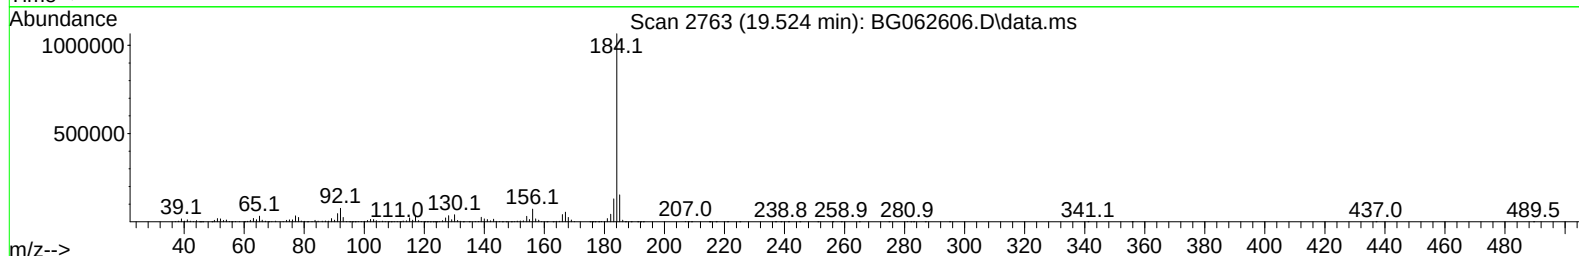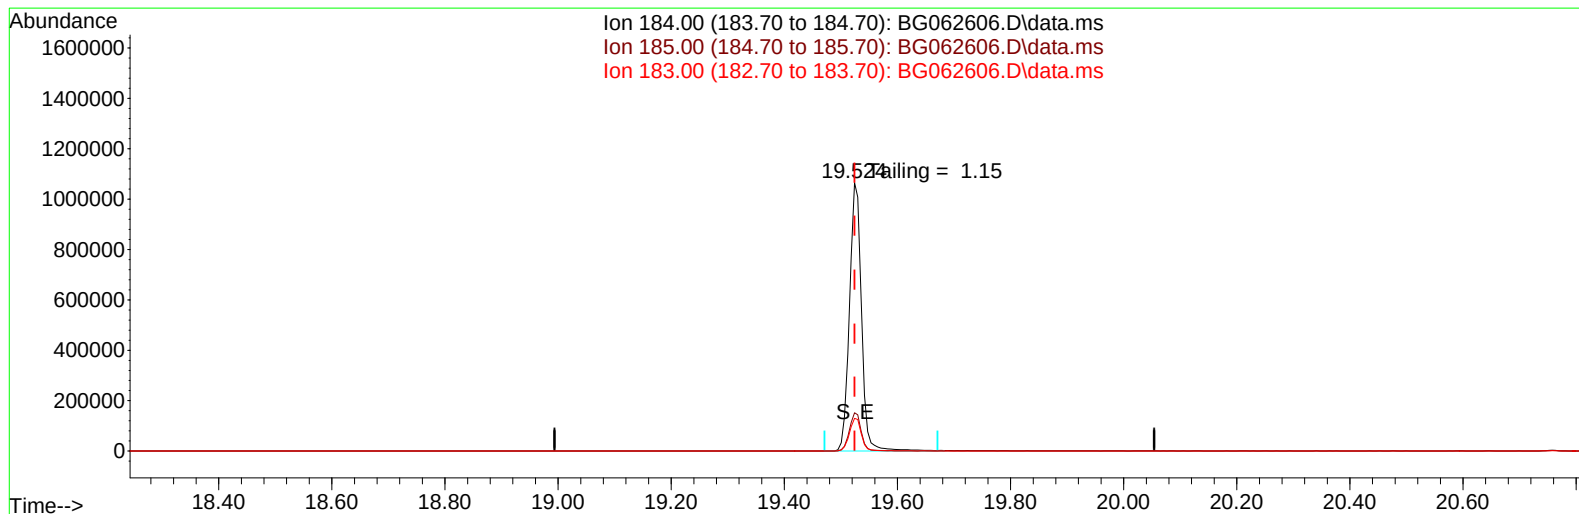

TIC: BG062606.D\data.ms

**(77) Benzidine****19.524min (-0.000) 64758.98 ng****response 1577897**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.80  | 14.30  |
| 183.00 | 12.10  | 12.18  |
| 0.00   | 0.00   | 0.00   |