
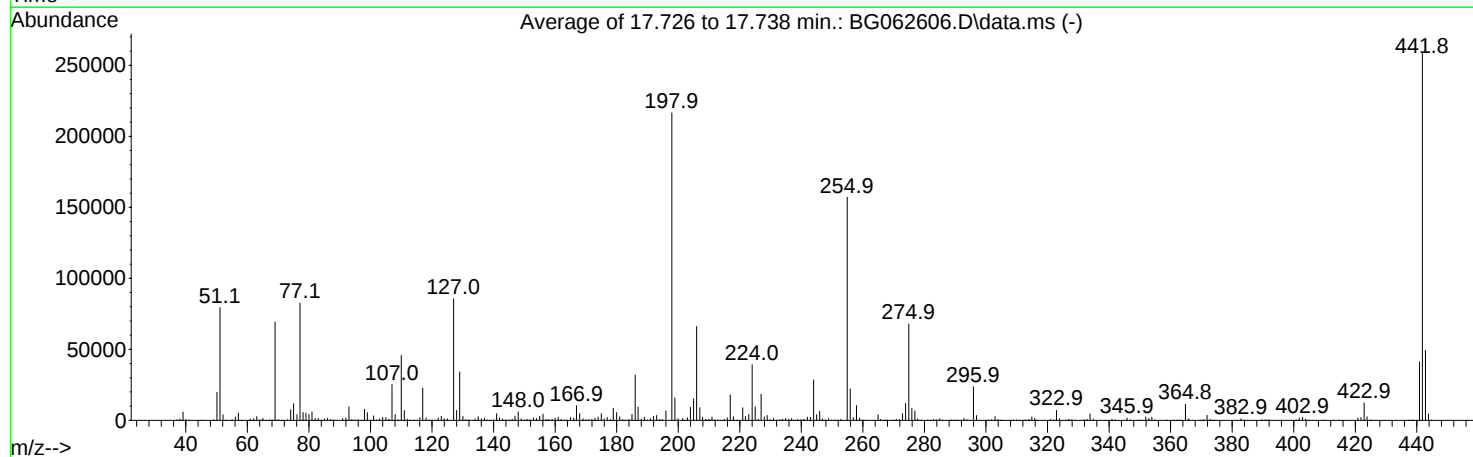


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083024\
Data File : BG062606.D
Acq On : 30 Aug 2024 6:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Aug 31 02:36:01 2024

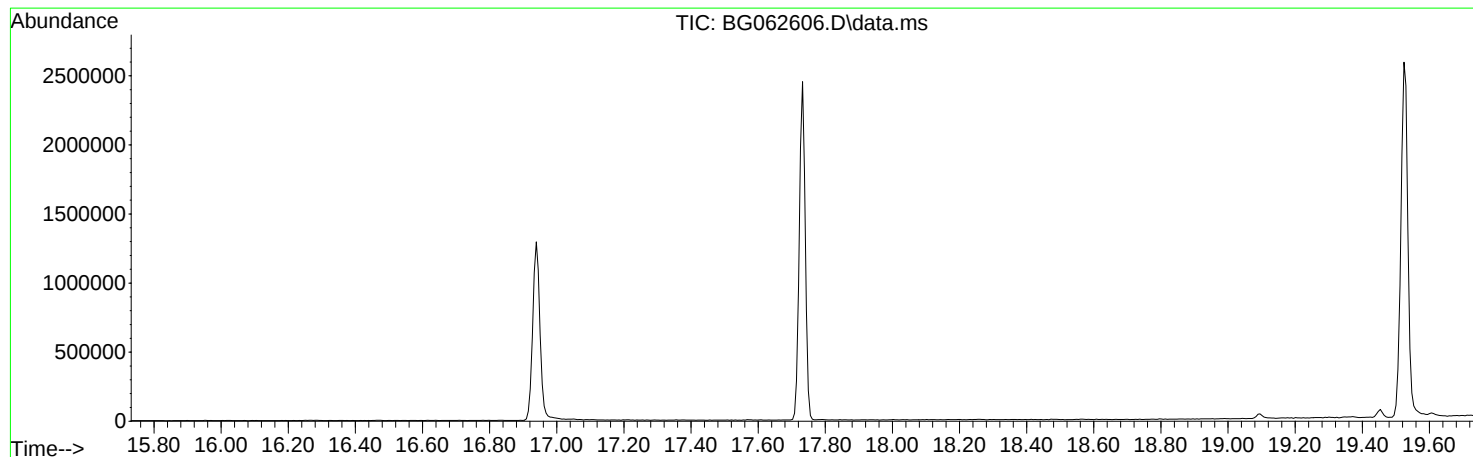

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	79339	PASS
68	69	0.00	2	0.4	301	PASS
69	198	0.00	100	32.0	69323	PASS
70	69	0.00	2	0.7	456	PASS
127	198	10	80	39.5	85587	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	216533	PASS
199	198	5	9	7.3	15730	PASS
275	198	10	60	31.3	67848	PASS
365	198	1	100	5.2	11343	PASS
441	198	0.01	100	19.1	41293	PASS
442	442	50	100	100.0	258987	PASS
443	442	15	24	19.1	49341	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/30/2024	BNA_G	<u>BG062606.D</u>
Compound Name	Response	Retention Time
DDT	614161	20.758
DDD	11670	20.37
DDE	272	19.454
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11942	626103	1.91

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083024\
Data File : BG062606.D
Acq On : 30 Aug 2024 6:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 30 12:54:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 30 12:30:23 2024
Response via : Initial Calibration

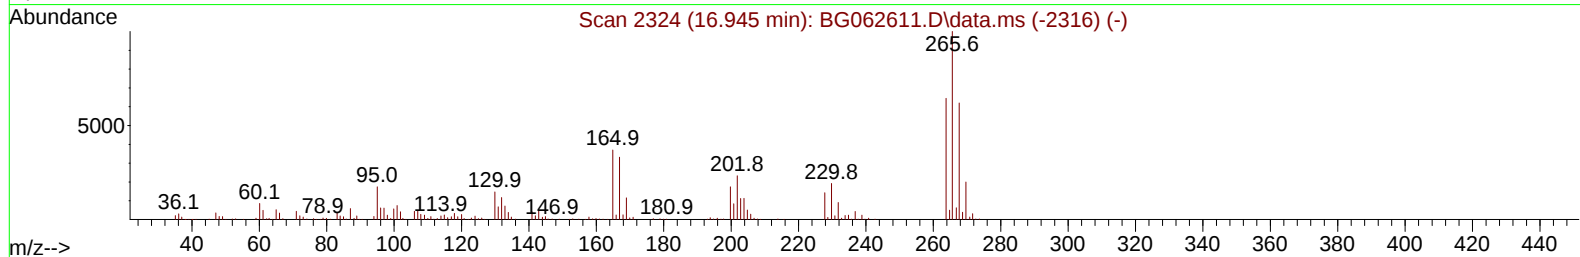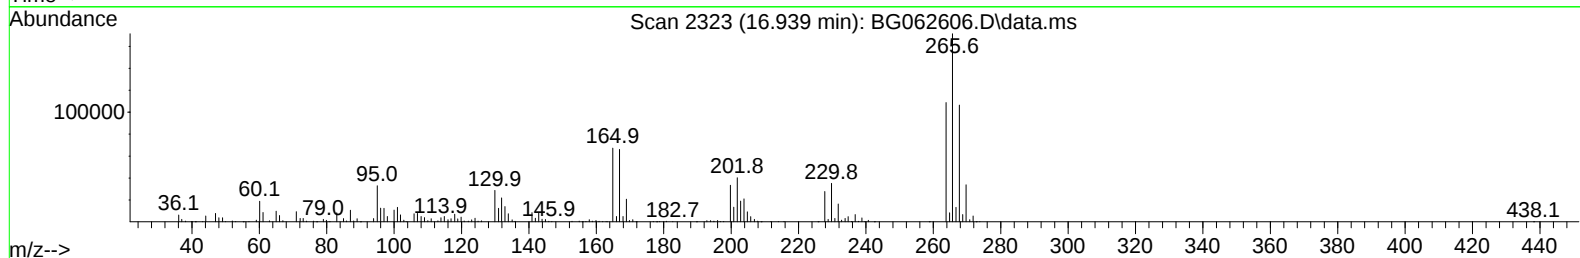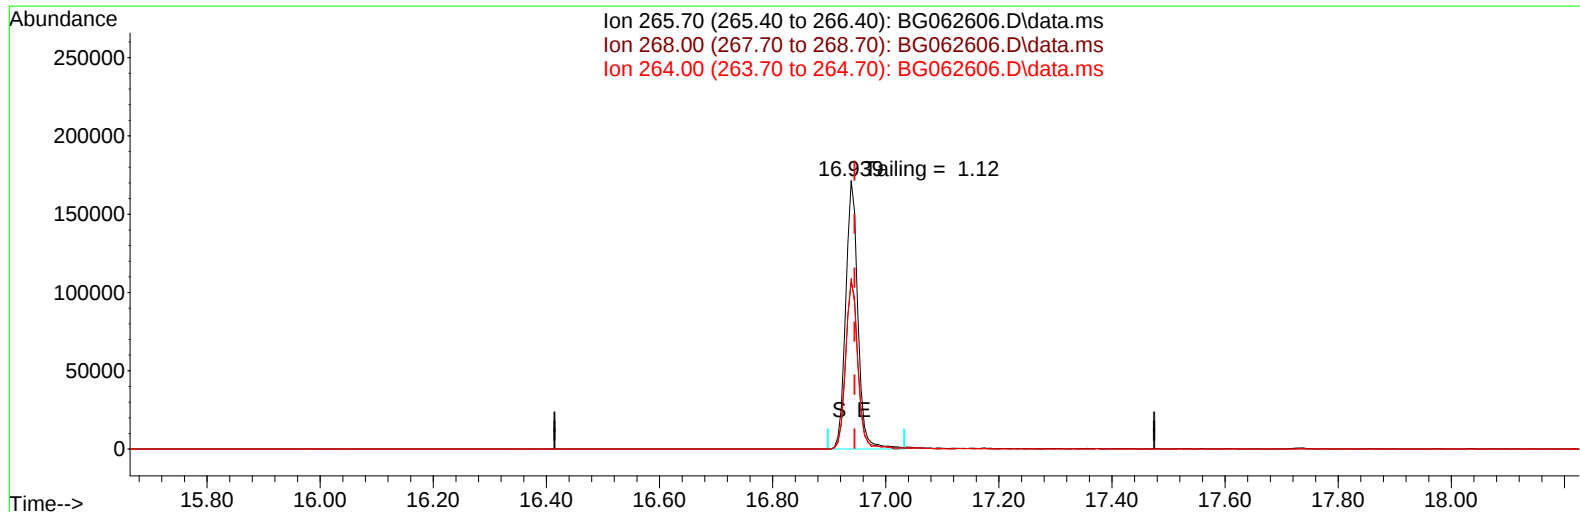

TIC: BG062606.D\data.ms

(70) Pentachlorophenol (C)

16.939min (-0.006) 54426.83 ng




response 257427

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	65.96
264.00	64.50	63.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083024\
Data File : BG062606.D
Acq On : 30 Aug 2024 6:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 30 12:54:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 30 12:30:23 2024
Response via : Initial Calibration

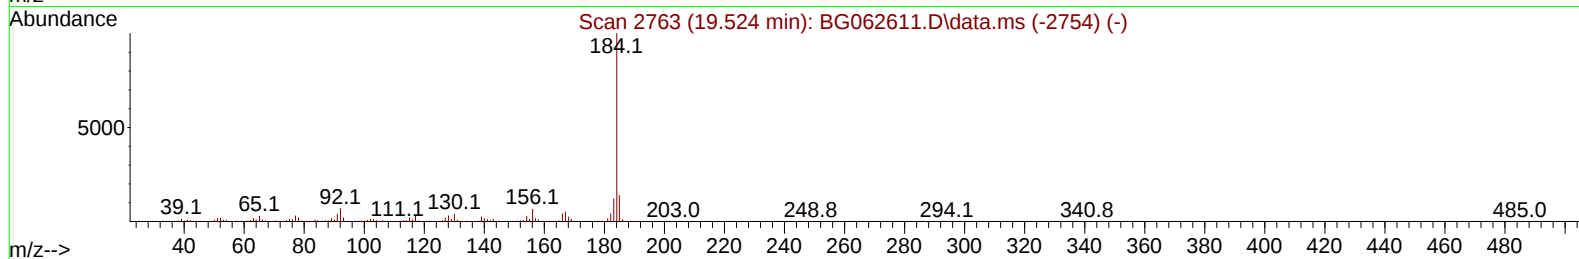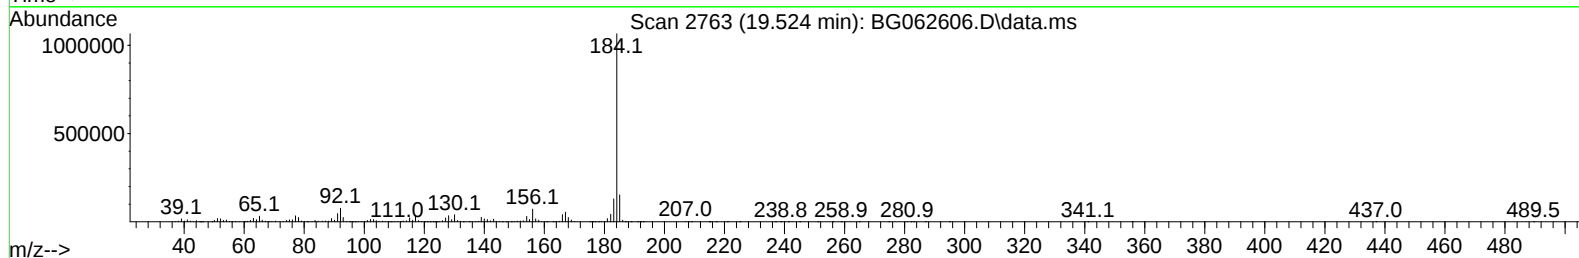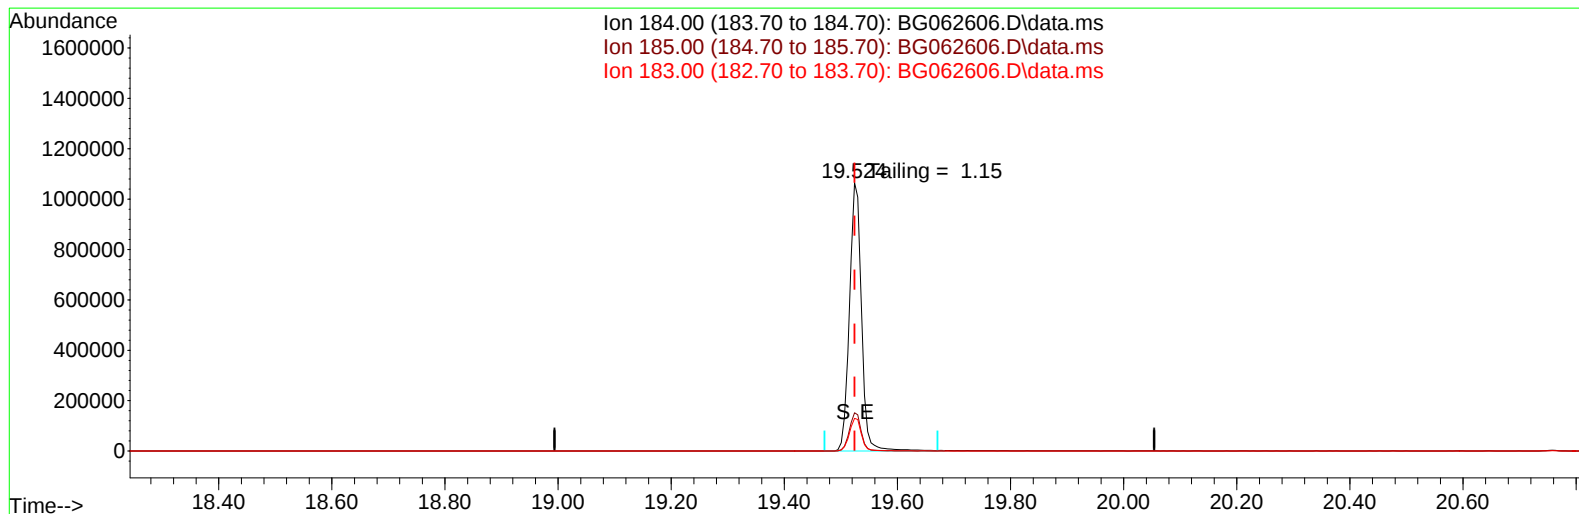

TIC: BG062606.D\data.ms

(77) Benzidine

19.524min (-0.000) 64758.98 ng

response 1577897

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.30
183.00	12.10	12.18
0.00	0.00	0.00