

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG083115\
 Data File : BG018553.D
 Acq On : 31 Aug 2015 18:43
 Operator : UM/IZ
 Sample : G3448-12RE
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE6RE

Quant Time: Sep 01 10:22:14 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 01 00:57:18 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	83653	20.00	ng/ul	0.00
18) Naphthalene-d8	10.82	136	338835	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	157860	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.38	188	631994	20.00	ng/ul	0.00
78) Chrysene-d12	21.64	240	520308	20.00	ng/ul	0.00
86) Perylene-d12	24.83	264	97778	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.44	96	2789	1.47	ng/uL	0.00
5) Phenol-d5	7.17	99	57012	7.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	155852	33.13	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	164940	28.37	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	107596	16.87	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	104548	39.58	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	112817	41.94	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	229507	40.20	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	0.00
44) Dimethylphthalate-d6	14.04	166	792475	59.67	ng/ul	0.00
47) Acenaphthylene-d8	14.33	160	328818	19.66	ng/ul	0.00
52) 4-Nitrophenol-d4	14.82	143	30931	12.95	ng/ul	0.00
58) Fluorene-d10	15.63	176	646864	55.92	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.74	200	121866	39.20	ng/ul	0.00
71) Anthracene-d10	17.48	188	531638	17.59	ng/ul	0.00
79) Pyrene-d10	19.76	212	476679	17.66	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.61	264	148185	28.55	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
33) 4-Chloro-3-methylphenol	12.09	107	11553	1.86	ng/ul	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG083115\
Data File : BG018553.D
Acq On : 31 Aug 2015 18:43
Operator : UM/IZ
Sample : G3448-12RE
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE6RE

Quant Time: Sep 01 10:22:14 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 01 00:57:18 2015
Response via : Initial Calibration

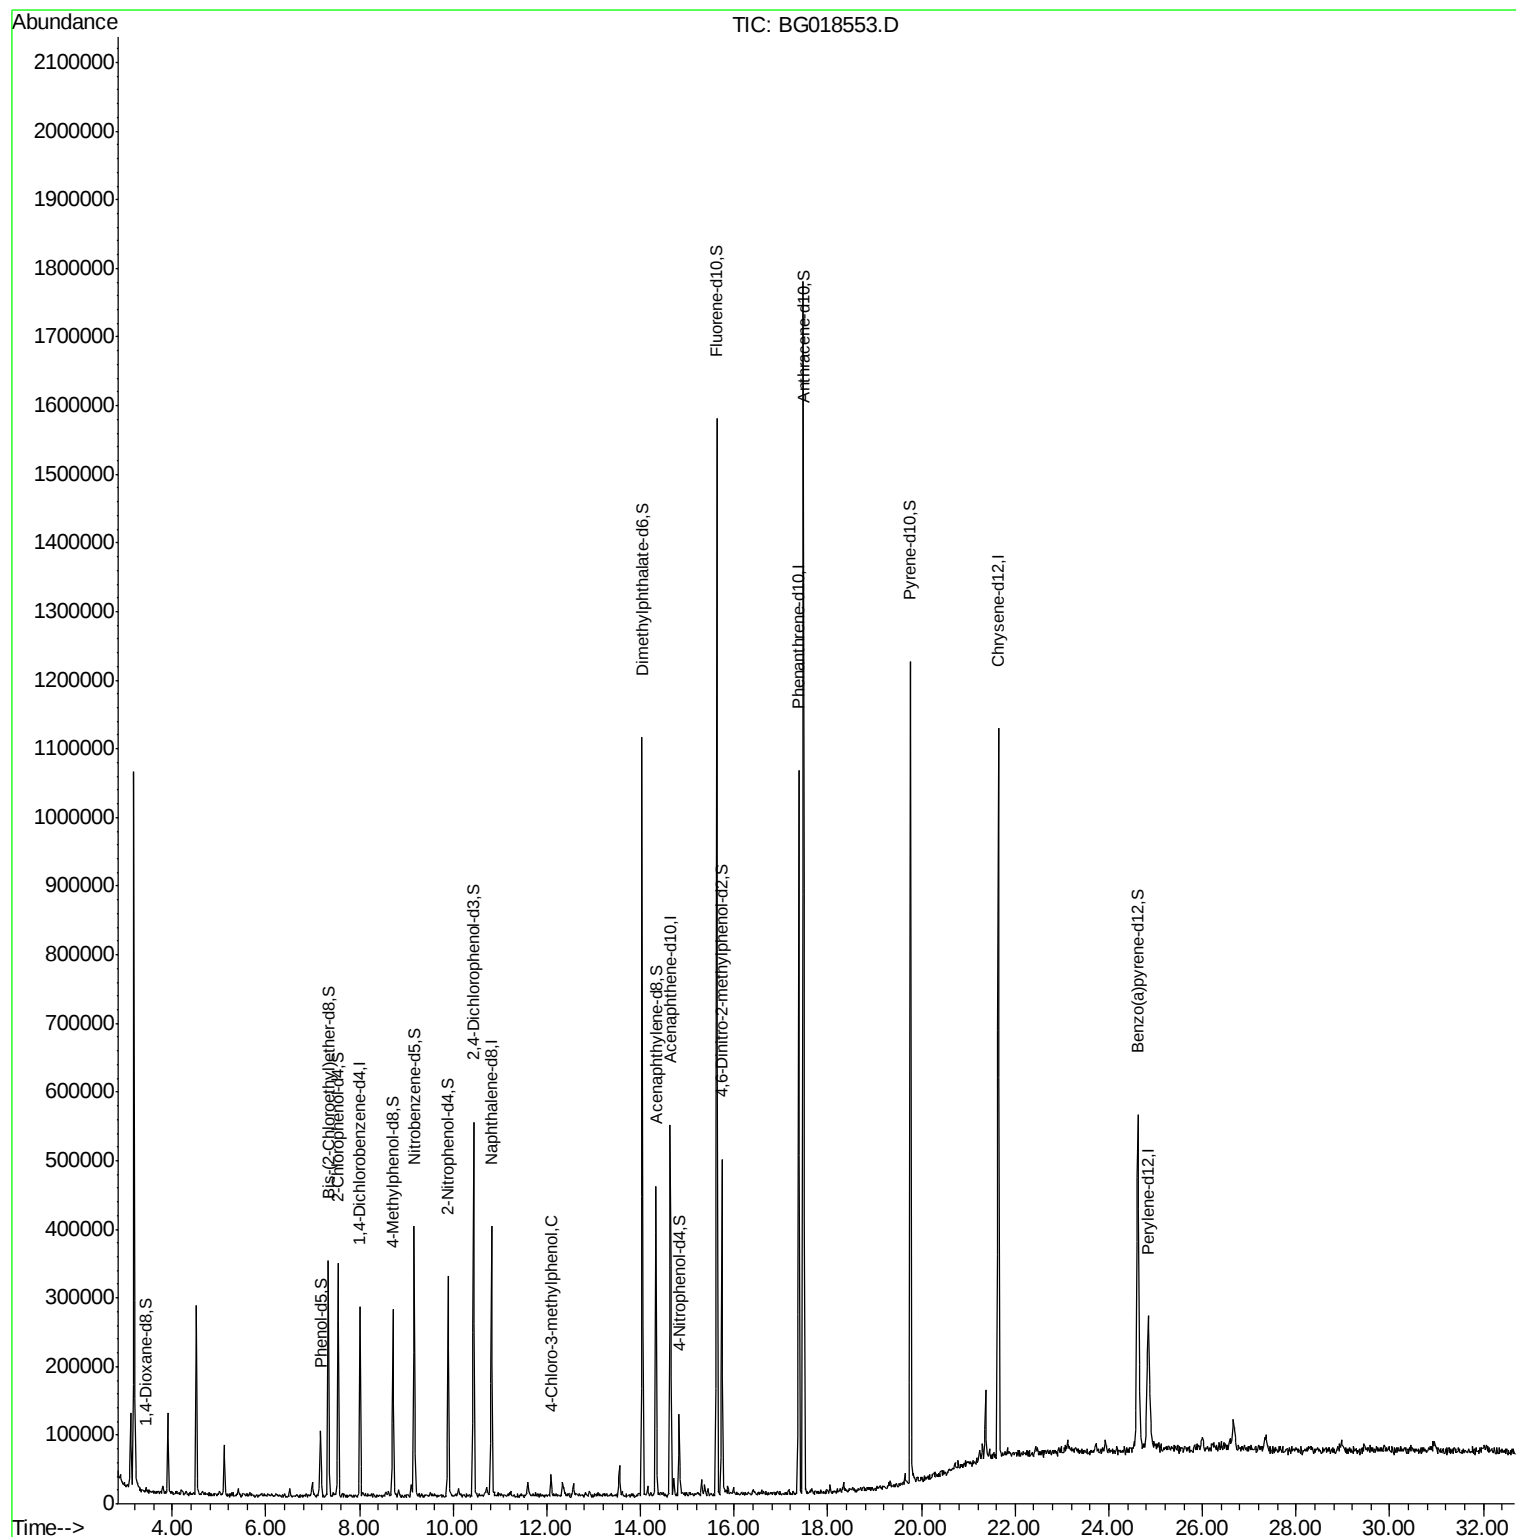

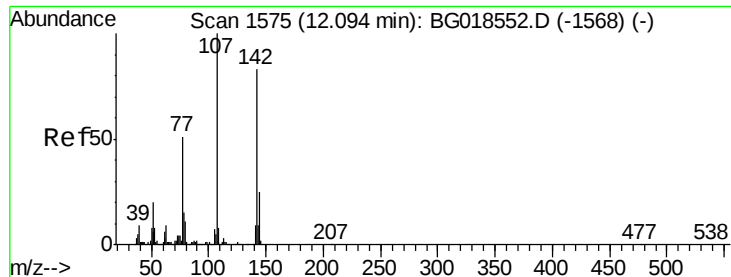

#33
 4-Chloro-3-methylphenol
 Concen: 1.86 ng/ul
 RT: 12.09 min Scan# 1574
 Delta R.T. -0.01 min
 Lab File: BG018553.D
 Acq: 31 Aug 2015 18:43

Instrument :
 BNA_G
 ClientSampleId :
 C0AE6RE

Tgt Ion	Ratio	Lower	Upper
107	100		
144	27.5	21.4	32.2
142	70.8	66.0	99.0

