


Data Path : Z:\HPCHEM1\BNA_G\Data\BG083115\
 Data File : BG018551.D
 Acq On : 31 Aug 2015 17:26
 Operator : UM/IZ
 Sample : DFTPP42
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP42

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
 Title : SVOA CALIBRATION
 Last Update : Tue Sep 01 00:57:18 2015

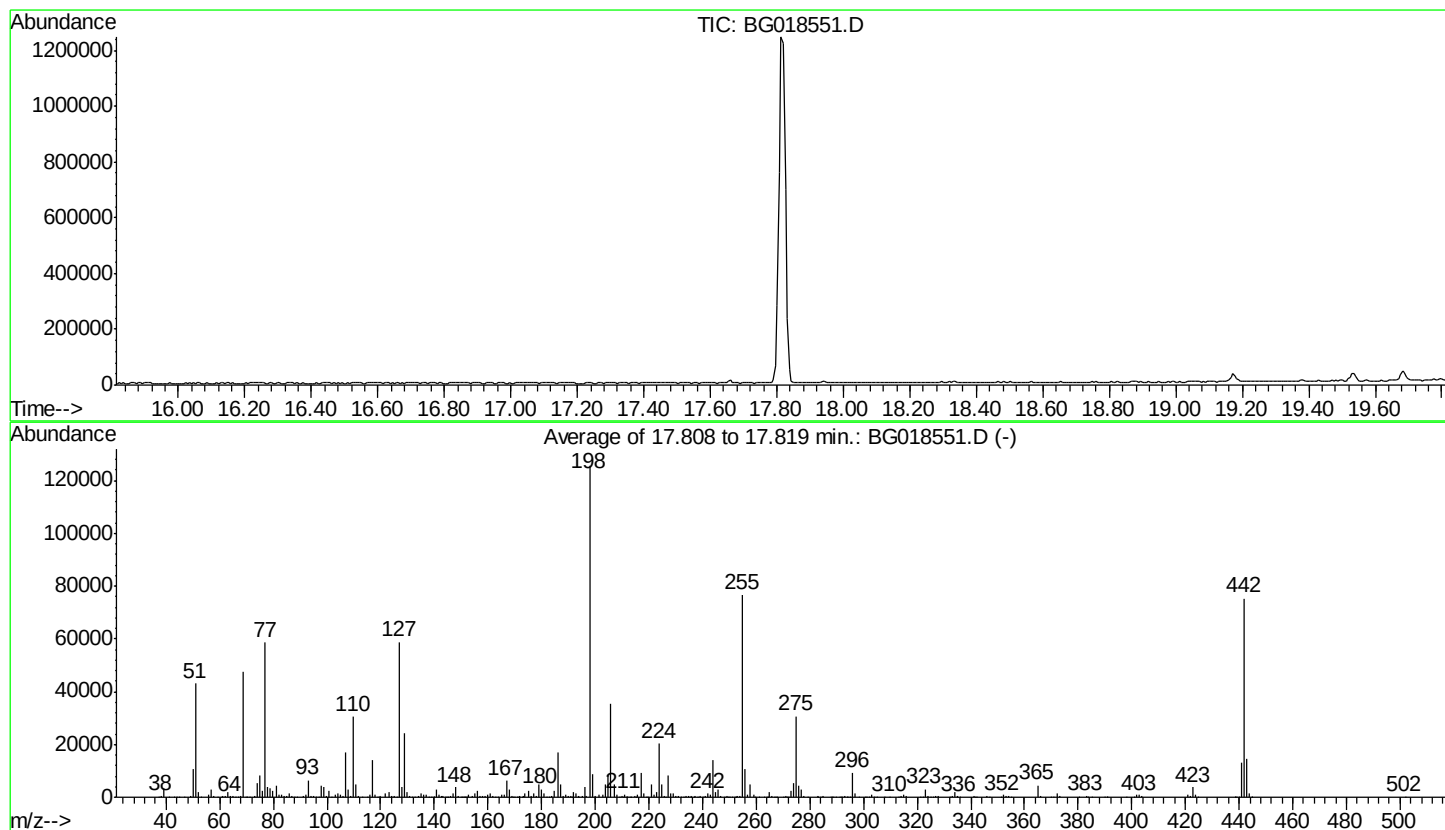

AutoFind: Scans 2548, 2549, 2550; Background Corrected with Scan 2543

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	43139	PASS
68	69	0.00	2	0.6	279	PASS
69	198	0.00	100	38.0	47763	PASS
70	69	0.00	2	0.5	219	PASS
127	198	10	80	46.8	58840	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	125597	PASS
199	198	5	9	6.9	8701	PASS
275	198	10	60	24.5	30725	PASS
365	198	1	100	3.5	4395	PASS
441	442	0.01	24	17.3	13034	PASS
442	198	50	100	59.8	75168	PASS
443	442	15	24	19.7	14799	PASS

m/z	Abundance
38.00	382.0
39.00	2256.0
39.90	1311.0
41.00	156.0
43.00	159.0
43.90	972.0
45.00	419.0
47.00	227.0
48.90	523.0
50.00	8295.0
51.00	36048.0
51.90	1873.0
55.00	367.0
55.90	1073.0
56.90	2704.0
57.90	423.0
59.90	190.0
60.80	368.0
62.00	323.0
63.00	2072.0
63.90	290.0
64.90	635.0
67.00	154.0
68.00	839.0
68.90	39424.0
69.80	403.0
71.00	161.0
72.90	690.0
74.00	4395.0
75.00	6999.0
76.00	2422.0
77.00	47272.0
78.00	3268.0
79.00	2942.0
79.90	2112.0
80.90	3357.0
81.90	1051.0
82.90	793.0
83.90	596.0
85.00	338.0
85.90	1663.0
87.00	372.0
87.90	202.0
90.90	724.0
92.00	612.0
92.90	5377.0
94.00	169.0
95.00	182.0
95.90	231.0
96.90	166.0
97.90	3817.0
98.90	2458.0
99.90	218.0
100.90	2110.0
102.90	602.0
103.90	909.0
104.90	1030.0
106.00	503.0
106.90	12940.0
107.90	2562.0
109.00	415.0
109.90	23600.0
110.90	4468.0
111.80	248.0
113.00	169.0
114.90	175.0
115.90	893.0
117.00	10377.0
117.90	804.0
119.90	372.0
121.90	1121.0
122.90	1355.0
124.00	712.0
124.80	305.0
127.00	45696.0
127.90	3698.0
128.90	17800.0
129.90	1267.0
130.90	177.0
134.00	498.0
134.90	936.0
135.90	576.0
137.00	553.0
138.10	226.0
138.90	200.0
140.00	289.0
140.90	1970.0
141.90	705.0
142.80	541.0
144.00	157.0
144.80	223.0

Instrument :
BNA_G
ClientSampleId :
DFTPP42

146.00	492.0
147.00	1226.0
147.90	2587.0
148.90	516.0
150.90	249.0
152.20	204.0
152.90	605.0
153.90	610.0
155.00	1474.0
155.90	2147.0
157.10	299.0
157.80	535.0
158.90	163.0
159.90	494.0
161.00	846.0
161.90	235.0
163.00	291.0
164.90	693.0
165.90	693.0
166.90	4922.0
167.90	2209.0
169.00	390.0
172.00	514.0
172.80	353.0
173.90	739.0
175.00	1471.0
176.00	681.0
176.90	1212.0
177.90	336.0
178.90	3461.0
179.90	1927.0
181.00	1144.0
181.90	316.0
184.90	2127.0
185.90	12011.0
186.90	3158.0
187.90	733.0
188.90	742.0
190.00	241.0
190.90	248.0
191.20	223.0
192.00	1707.0
192.90	1043.0
193.80	332.0
195.90	3062.0
197.90	88600.0
198.90	6018.0
199.80	477.0
201.40	773.0
203.00	565.0
204.00	3499.0
204.90	5615.0
205.90	23752.0
207.00	3267.0
207.90	814.0
210.20	364.0
211.00	501.0
214.80	508.0
215.90	494.0
216.90	5868.0
217.90	1056.0
218.90	205.0
219.70	259.0
220.90	2370.0
221.80	911.0
222.90	1551.0
224.00	13304.0
224.90	2998.0
225.90	271.0
226.90	5637.0
227.90	708.0
228.90	519.0
230.00	231.0
231.00	447.0
232.90	152.0
234.00	378.0
234.90	576.0
235.60	176.0
236.80	412.0
238.00	214.0
238.90	244.0
239.90	316.0
240.90	313.0
242.00	1069.0
242.90	808.0
243.90	10662.0
244.90	1042.0
245.90	1650.0
246.80	617.0
248.80	368.0
253.70	275.0
254.90	50280.0
255.90	7859.0
256.90	1153.0
257.90	3173.0

Instrument :
BNA_G
ClientSampleId :
DFTPP42

258.90	810.0
263.00	215.0
264.90	1206.0
266.90	153.0
271.00	200.0
272.90	1655.0
273.90	3621.0
274.90	19888.0
275.90	2943.0
276.80	1719.0
278.00	191.0
281.00	261.0
282.90	557.0
284.00	180.0
285.00	485.0
292.00	259.0
292.90	519.0
294.20	156.0
295.90	6309.0
296.90	558.0
303.00	501.0
309.90	216.0
313.90	299.0
314.90	451.0
315.90	449.0
320.90	154.0
322.90	1939.0
324.00	477.0
328.00	252.0
333.00	245.0
333.80	1089.0
334.80	539.0
340.90	274.0
346.00	469.0
351.90	512.0
353.00	480.0
354.00	170.0
364.80	2694.0
366.00	488.0
371.90	965.0
373.00	381.0
380.20	178.0
382.90	430.0
389.90	287.0
402.10	291.0
402.90	336.0
403.90	260.0
421.00	361.0
421.90	462.0
422.90	2214.0
424.00	493.0
441.00	6574.0
442.00	39056.0
442.90	7805.0
444.00	1025.0
444.70	207.0

Instrument :
BNA_G
ClientSampleId :
DFTPP42

m/z	Abundance
37.00	341.0
38.00	809.0
39.00	3889.0
39.90	1202.0
41.10	204.0
41.90	188.0
42.90	505.0
43.90	1022.0
45.10	345.0
48.90	1089.0
50.00	12473.0
51.00	51632.0
52.00	2273.0
54.90	330.0
55.90	1504.0
56.90	3412.0
57.90	398.0
59.10	207.0
61.00	1048.0
62.00	738.0
62.90	1757.0
63.90	263.0
65.00	1092.0
66.80	163.0
68.90	57232.0
70.00	343.0
72.90	668.0
74.00	6076.0
74.90	8574.0
75.90	2761.0
77.00	68376.0
78.00	4675.0
78.90	4490.0
79.90	3472.0
80.90	5717.0
81.90	1096.0
83.00	1141.0
83.80	725.0
85.00	711.0
85.90	1893.0
86.90	628.0
87.90	267.0
88.90	165.0
91.00	1277.0
91.90	1155.0
92.90	7048.0
93.90	442.0
94.90	382.0
96.00	465.0
96.90	224.0
97.90	4593.0
98.90	4931.0
99.90	446.0
100.90	2267.0
101.80	327.0
102.90	1027.0
103.90	1872.0
104.90	1666.0
105.90	745.0
106.90	19664.0
107.90	2718.0
109.10	652.0
109.90	35432.0
110.90	5794.0
111.90	746.0
113.00	225.0
116.00	1295.0
116.90	16800.0
118.00	1419.0
118.90	267.0
120.00	191.0
121.90	896.0
122.90	1831.0
123.80	541.0
124.90	859.0
126.90	69200.0
127.90	4609.0
128.90	27920.0
129.90	1901.0
130.80	672.0
131.90	249.0
133.90	958.0
134.90	2123.0
135.80	1094.0
136.90	775.0
139.00	167.0
139.70	250.0
140.90	3204.0
142.00	1182.0
143.00	845.0
143.90	186.0

Instrument :
BNA_G
ClientSampleId :
DFTPP42

145.00	309.0
145.90	833.0
147.00	2094.0
147.90	4965.0
148.90	745.0
149.90	248.0
151.00	367.0
151.90	359.0
152.90	1486.0
153.90	750.0
155.00	1025.0
155.90	2664.0
157.00	859.0
157.90	564.0
158.90	441.0
159.90	1315.0
160.90	1967.0
161.90	645.0
162.80	204.0
163.90	223.0
164.90	1453.0
165.90	985.0
166.90	6846.0
167.90	3321.0
168.90	628.0
170.10	180.0
171.20	388.0
171.90	581.0
173.00	748.0
173.90	1429.0
175.00	2946.0
175.90	637.0
176.80	1506.0
177.90	498.0
178.90	5334.0
179.90	3742.0
181.00	1605.0
181.90	233.0
182.90	519.0
183.90	392.0
184.90	2377.0
185.90	20000.0
186.90	5874.0
187.90	539.0
188.90	1320.0
190.00	270.0
190.90	826.0
191.90	2213.0
192.90	1931.0
194.00	451.0
194.90	404.0
195.90	4227.0
196.50	1263.0
197.90	144512.0
198.90	11035.0
199.90	739.0
201.30	1332.0
202.90	1489.0
203.90	6057.0
204.90	9511.0
205.90	41192.0
207.00	5549.0
207.90	1361.0
208.90	312.0
209.80	632.0
210.80	1053.0
211.40	389.0
212.00	321.0
212.90	303.0
214.80	431.0
215.90	1130.0
216.90	11451.0
218.00	1793.0
219.00	170.0
220.90	5603.0
221.90	1118.0
222.90	2022.0
223.90	23928.0
225.00	5733.0
226.10	445.0
226.90	9247.0
227.90	1882.0
228.90	1633.0
229.90	530.0
230.90	974.0
231.90	218.0
233.80	342.0
234.90	471.0
235.90	589.0
237.00	683.0
237.80	153.0
239.00	476.0
239.90	244.0
240.80	626.0
241.90	1127.0

Instrument :
BNA_G
ClientSampleId :
DFTPP42

243.00	1059.0
243.90	16552.0
245.00	1812.0
245.90	3448.0
246.90	821.0
247.90	258.0
248.90	691.0
249.60	271.0
251.00	293.0
252.00	173.0
252.20	169.0
252.90	365.0
253.80	489.0
254.90	90256.0
255.90	12428.0
256.90	1103.0
257.90	5857.0
258.90	902.0
259.80	183.0
263.80	397.0
264.90	2519.0
266.00	404.0
267.10	211.0
269.90	233.0
271.00	467.0
271.60	378.0
272.00	262.0
272.90	2776.0
273.90	6369.0
274.90	33640.0
275.90	5244.0
276.90	3579.0
277.80	491.0
279.10	226.0
282.80	317.0
284.90	557.0
287.90	186.0
289.80	393.0
290.90	181.0
293.00	367.0
293.70	302.0
295.00	407.0
295.90	11096.0
296.90	2004.0
298.00	175.0
301.30	154.0
302.00	274.0
302.90	1551.0
304.00	278.0
307.90	193.0
309.90	193.0
313.10	166.0
314.00	834.0
314.90	1169.0
315.90	348.0
320.90	269.0
322.10	256.0
323.00	3244.0
323.90	507.0
326.00	173.0
326.90	598.0
327.90	295.0
331.90	208.0
332.80	241.0
333.90	1600.0
335.10	446.0
335.90	236.0
340.80	190.0
342.20	154.0
345.90	892.0
347.00	166.0
351.00	286.0
351.90	719.0
352.90	601.0
353.90	797.0
354.90	222.0
364.90	5015.0
365.90	505.0
369.80	156.0
370.90	377.0
372.00	1404.0
372.90	247.0
382.90	750.0
383.80	331.0
389.80	293.0
391.00	160.0
401.90	818.0
402.90	905.0
403.80	479.0
420.90	1024.0
422.00	545.0
423.00	4541.0
423.90	629.0
438.60	474.0
439.80	207.0

Instrument :
BNA_G
ClientSampleId :
DFTPP42

440.90	14706.0
442.00	83448.0
443.00	16456.0
443.80	1619.0

Instrument :
BNA_G
ClientSampleId :
DFTPP42

m/z	Abundance
38.00	443.0
39.00	3785.0
39.90	1025.0
41.10	197.0
42.90	345.0
44.00	910.0
44.90	255.0
49.00	776.0
50.00	11832.0
51.00	42608.0
52.00	2017.0
53.00	197.0
55.10	400.0
56.00	1627.0
57.00	3351.0
58.00	294.0
59.80	325.0
60.90	638.0
61.90	494.0
63.00	1511.0
63.90	348.0
65.00	800.0
65.90	189.0
67.00	212.0
68.90	47456.0
69.90	316.0
72.80	424.0
74.00	5436.0
74.90	9162.0
76.00	2328.0
77.00	61000.0
78.00	3509.0
79.00	3331.0
79.90	2459.0
81.00	4179.0
81.90	733.0
82.90	1025.0
83.90	628.0
84.90	1069.0
85.90	1131.0
86.90	752.0
87.90	234.0
90.90	908.0
92.00	1305.0
92.90	6788.0
93.90	320.0
95.00	313.0
95.90	378.0
96.80	297.0
97.90	5161.0
98.90	3656.0
99.90	266.0
100.90	2384.0
101.80	287.0
103.00	940.0
103.90	1837.0
104.90	1338.0
106.00	502.0
106.90	17920.0
108.00	2835.0
108.90	653.0
109.90	32368.0
110.90	4140.0
111.90	707.0
112.90	163.0
115.90	1420.0
116.90	15951.0
117.90	1204.0
119.80	480.0
121.90	1687.0
122.90	2471.0
123.90	526.0
124.80	702.0
125.90	483.0
126.90	61624.0
127.90	3977.0
128.90	26664.0
129.90	2416.0
130.80	462.0
131.80	233.0
132.50	210.0
133.90	1202.0
135.00	1774.0
135.90	813.0
137.00	1122.0
137.90	332.0
139.90	313.0
140.90	3530.0
141.90	870.0
142.80	1038.0
144.00	171.0

Instrument :
BNA_G
ClientSampleId :
DFTPP42

145.00	185.0
146.00	526.0
146.90	1526.0
147.90	3652.0
149.00	851.0
150.10	156.0
151.20	364.0
151.40	345.0
152.90	1019.0
153.90	560.0
155.00	2380.0
155.90	2900.0
156.90	544.0
158.00	605.0
158.90	254.0
159.90	913.0
160.90	1436.0
162.00	429.0
163.90	174.0
165.00	1293.0
165.90	1289.0
166.90	7488.0
167.90	3246.0
169.00	659.0
169.60	162.0
170.80	421.0
171.90	527.0
173.00	715.0
173.90	1633.0
174.90	2847.0
175.90	832.0
176.80	1383.0
177.90	551.0
178.90	6000.0
179.90	3685.0
180.90	1722.0
182.00	202.0
182.90	266.0
183.90	420.0
184.90	3350.0
185.90	19208.0
186.90	5725.0
187.90	342.0
188.90	1292.0
189.90	350.0
190.90	716.0
191.90	1653.0
192.90	2055.0
193.90	703.0
195.00	389.0
195.90	4893.0
197.90	143680.0
198.90	9052.0
200.00	977.0
201.40	483.0
202.90	1270.0
203.90	5325.0
204.90	9462.0
205.90	41000.0
206.90	5709.0
207.90	1118.0
208.90	437.0
209.80	415.0
210.90	1495.0
211.70	185.0
213.10	208.0
215.00	780.0
215.90	1057.0
216.90	10506.0
217.90	1968.0
219.00	201.0
220.90	6484.0
221.80	1416.0
222.90	2492.0
223.90	23592.0
224.90	5304.0
225.90	895.0
226.90	9978.0
227.80	1184.0
228.90	1965.0
229.80	243.0
231.00	618.0
231.80	311.0
232.90	279.0
234.00	671.0
235.00	687.0
235.90	333.0
236.90	892.0
238.80	404.0
239.90	231.0
240.80	462.0
241.90	1570.0
243.00	1447.0
243.90	15655.0
244.90	2602.0

Instrument :
BNA_G
ClientSampleId :
DFTPP42

245.90	3338.0
246.90	683.0
248.90	891.0
249.90	172.0
250.80	315.0
253.00	603.0
253.70	443.0
254.90	89880.0
255.90	12245.0
256.90	1414.0
257.90	5987.0
258.90	854.0
260.80	223.0
264.20	199.0
264.90	1872.0
265.80	531.0
267.60	166.0
270.90	187.0
272.90	2869.0
273.90	5754.0
274.90	38648.0
275.90	5386.0
276.90	3148.0
277.90	339.0
279.00	160.0
280.90	200.0
282.80	186.0
283.10	288.0
283.90	372.0
285.00	619.0
288.10	151.0
288.90	185.0
291.70	230.0
292.90	989.0
294.00	305.0
295.00	359.0
295.90	10850.0
296.90	1905.0
300.70	325.0
301.80	183.0
303.00	1529.0
304.00	434.0
305.00	303.0
313.00	251.0
313.90	554.0
314.90	1323.0
315.90	635.0
320.90	248.0
322.90	3915.0
323.90	594.0
324.90	201.0
326.90	893.0
327.90	439.0
331.90	439.0
332.90	540.0
334.00	2848.0
334.90	640.0
341.00	843.0
341.80	221.0
345.90	636.0
352.00	1013.0
352.90	453.0
354.00	1151.0
354.90	196.0
364.90	5478.0
365.80	448.0
370.90	386.0
371.90	1741.0
372.90	306.0
383.00	467.0
385.00	175.0
390.60	221.0
397.90	174.0
400.90	234.0
401.90	1123.0
402.90	1248.0
403.80	280.0
420.90	1398.0
422.10	742.0
422.90	4793.0
423.90	1418.0
424.80	184.0
438.30	153.0
439.20	245.0
439.80	273.0
441.00	17824.0
442.00	103000.0
443.00	20136.0
443.90	2029.0
444.90	157.0
501.80	227.0

Instrument :
BNA_G
ClientSampleId :
DFTPP42

m/z	Abundance
35.80	173.0
40.00	1436.0
41.00	174.0
42.00	204.0
43.00	177.0
43.90	847.0
44.90	291.0
47.90	186.0
49.00	517.0
51.00	290.0
53.90	170.0
55.00	375.0
56.00	240.0
59.90	262.0
64.90	196.0
69.00	274.0
77.00	269.0
83.90	214.0
85.90	319.0
87.10	186.0
91.00	403.0
95.90	214.0
105.00	241.0
111.90	152.0
117.00	160.0
126.50	153.0
133.00	170.0
134.00	347.0
146.80	233.0
158.10	210.0
166.90	293.0
188.90	206.0
190.80	182.0
204.00	226.0
206.90	174.0
280.90	158.0
282.20	167.0
289.20	211.0

Instrument :
BNA_G
ClientSampleId :
DFTPP42