
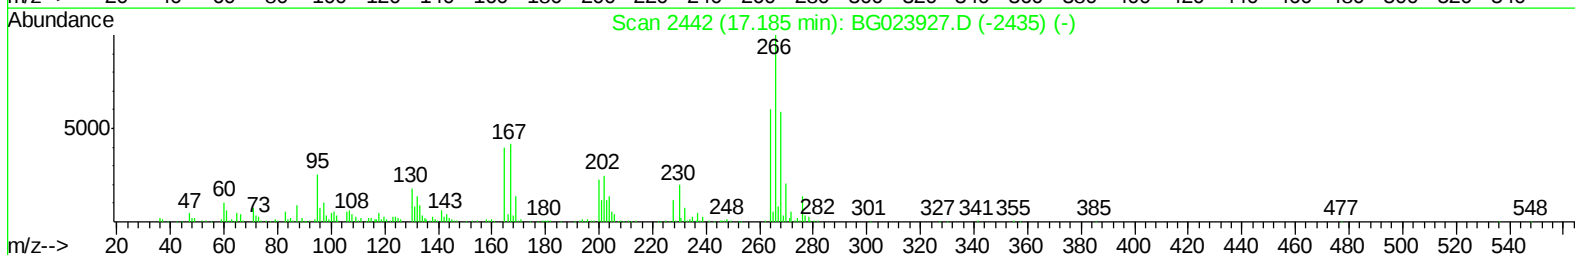
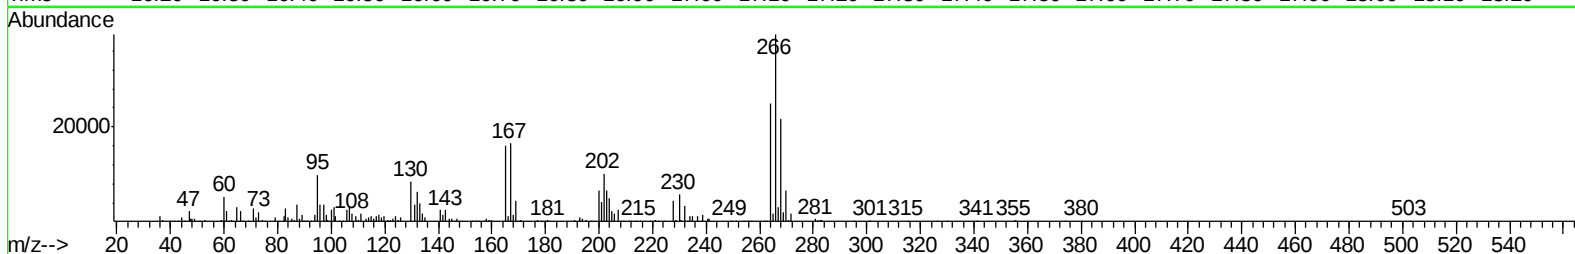


Data Path : Z:\HPCHEM1\BNA_G\Data\BG083116\
Data File : BG023923.D
Acq On : 31 Aug 2016 11:27
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 04:03:55 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 20:05:47 2016
Response via : Initial Calibration

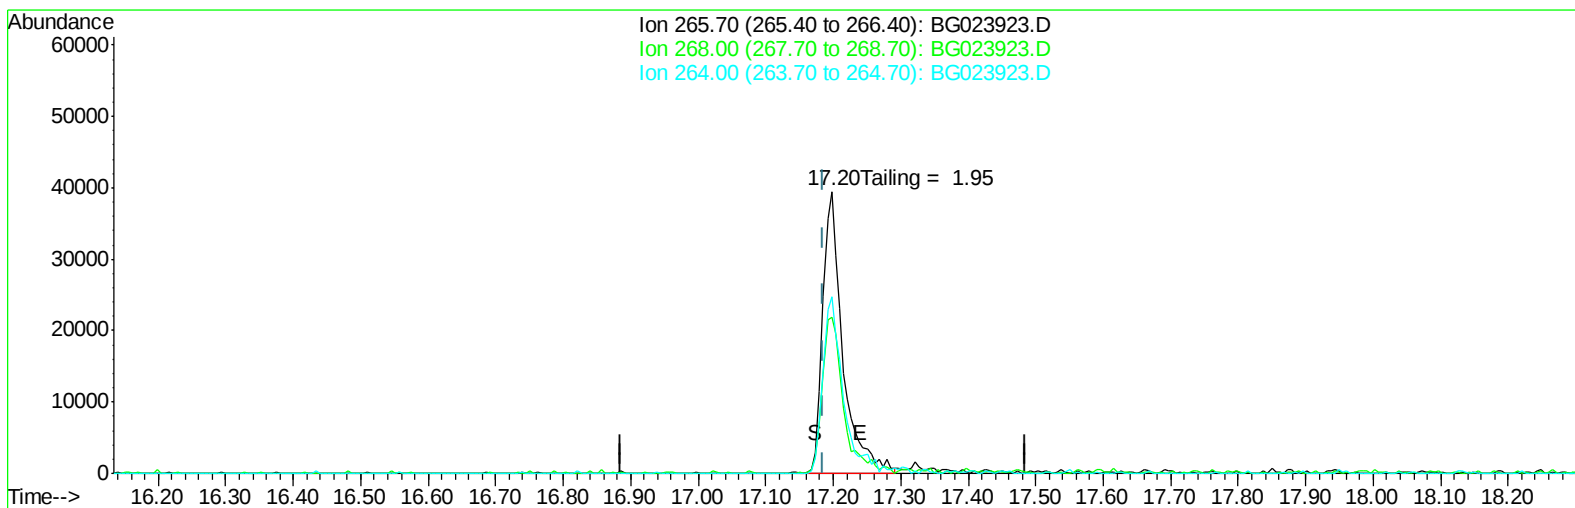

TIC: BG023923.D

(69) Pentachlorophenol (C)




17.197min (+0.012) 187671.73ng

response 81069

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	55.26
264.00	63.20	62.85
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG083116\
Data File : BG023923.D
Acq On : 31 Aug 2016 11:27
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 04:03:55 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 20:05:47 2016
Response via : Initial Calibration

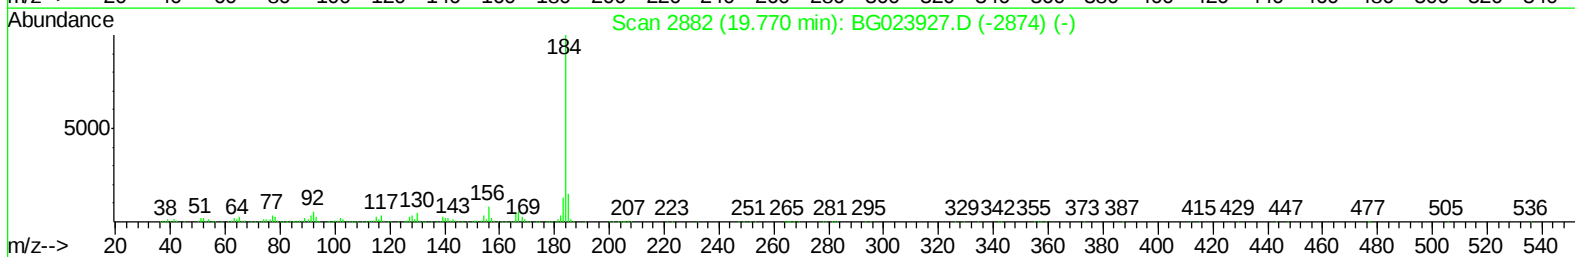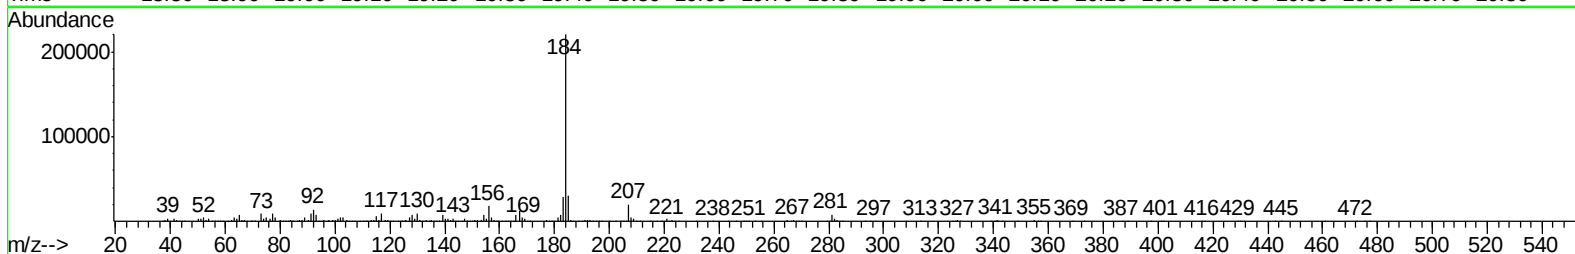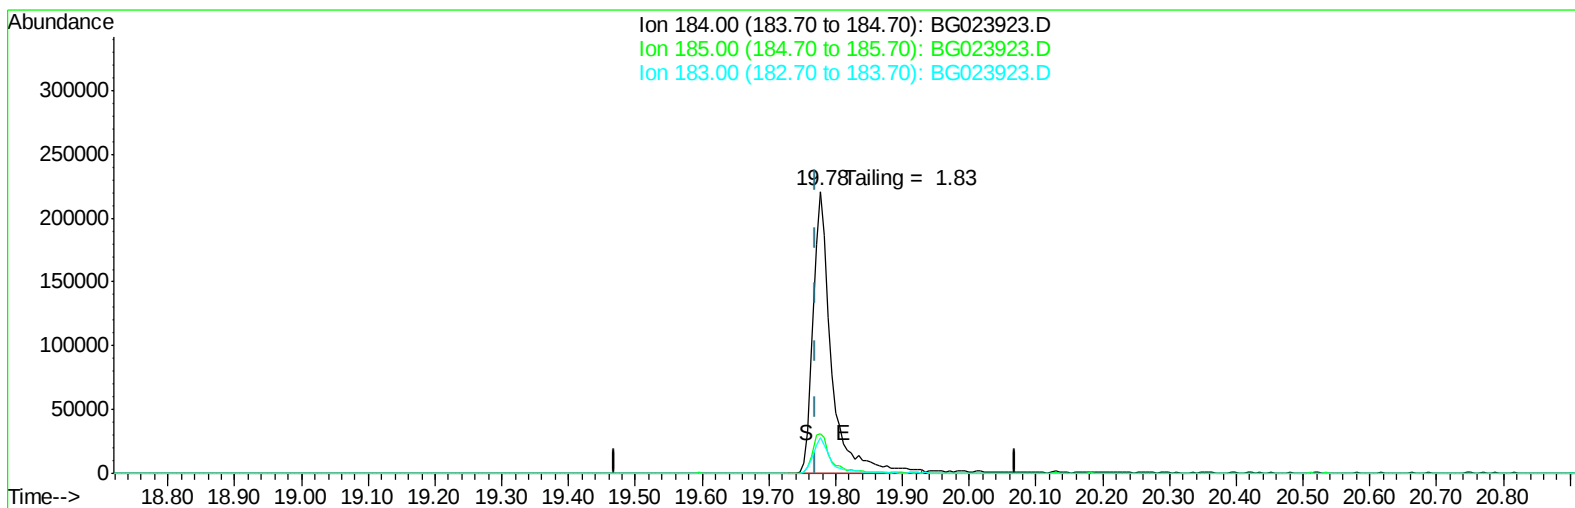

TIC: BG023923.D

(76) Benzidine

19.776min (+0.006) 73180.92ng

response 412431

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	13.89
183.00	13.40	12.81
0.00	0.00	0.00