


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG083116\
 Data File : BG023923.D
 Acq On : 31 Aug 2016 11:27
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 31 20:05:47 2016

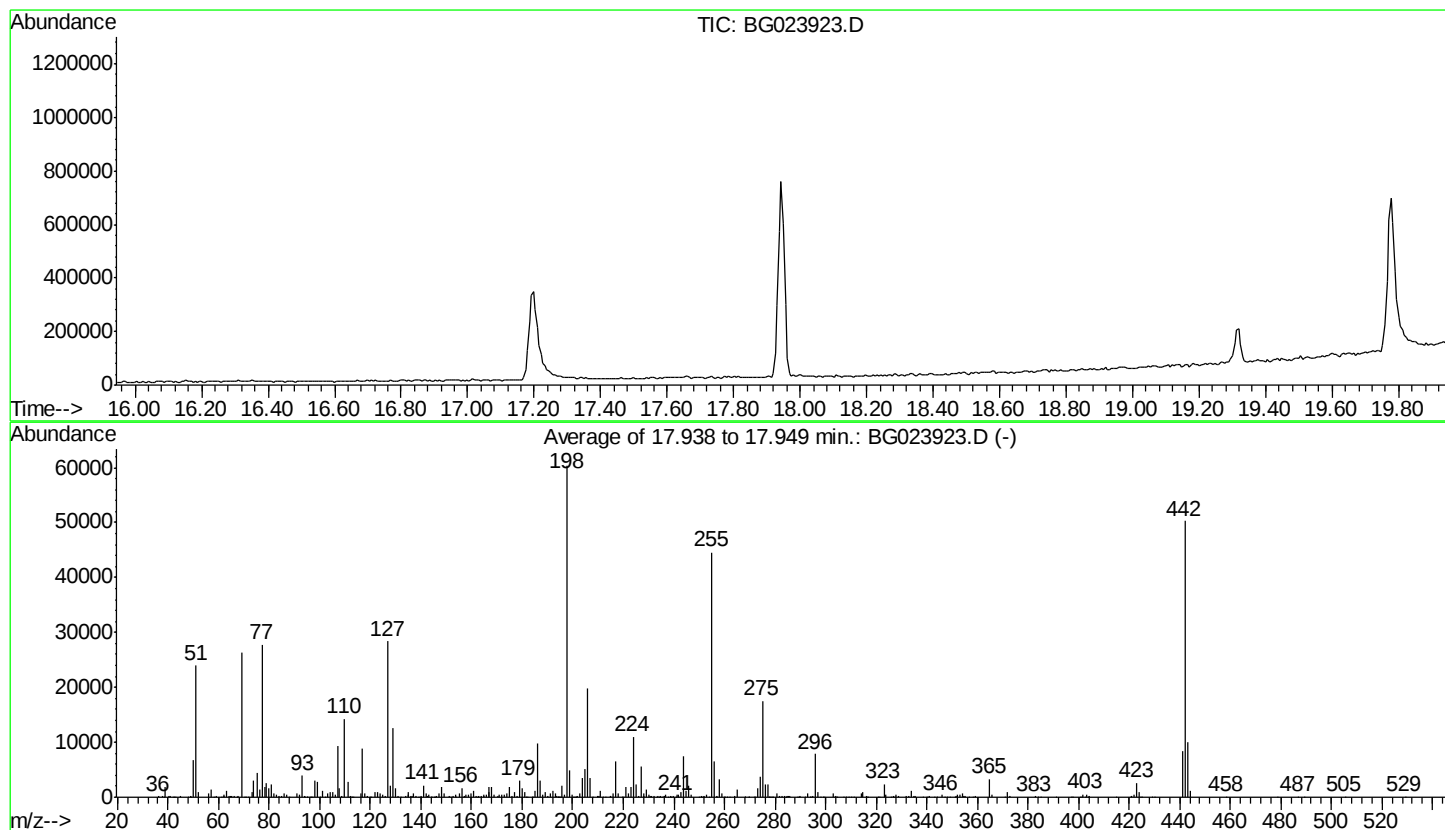

AutoFind: Scans 2570, 2571, 2572; Background Corrected with Scan 2560

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	23917	PASS
68	69	0.00	2	0.9	243	PASS
69	198	0.00	100	43.7	26370	PASS
70	69	0.00	2	0.1	32	PASS
127	198	10	80	46.9	28336	PASS
197	198	0.00	2	0.9	554	PASS
198	198	100	100	100.0	60370	PASS
199	198	5	9	8.1	4888	PASS
275	198	10	60	29.1	17570	PASS
365	198	1	100	5.6	3381	PASS
441	442	0.01	24	16.9	8497	PASS
442	198	50	100	83.2	50232	PASS
443	442	15	24	20.0	10049	PASS