

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG083120\
 Data File : BG046476.D
 Acq On : 31 Aug 2020 19:52
 Operator : CG/JU
 Sample : L3847-23
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 LINDEN-JOP-BH-11-C

Quant Time: Sep 01 04:08:19 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 31 16:05:33 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.93	152	75663	20.00	ng	0.00
21) Naphthalene-d8	10.73	136	310399	20.00	ng	0.00
39) Acenaphthene-d10	14.56	164	215599	20.00	ng	0.00
64) Phenanthrene-d10	17.30	188	545984	20.00	ng	0.00
76) Chrysene-d12	21.55	240	573242	20.00	ng	0.00
86) Perylene-d12	24.65	264	583165	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.51	112	373033	87.32	ng	0.00
7) Phenol-d6	7.10	99	499925	82.55	ng	0.00
23) Nitrobenzene-d5	9.09	82	318473	58.64	ng	0.00
42) 2,4,6-Tribromophenol	16.05	330	238757	81.73	ng	0.00
45) 2-Fluorobiphenyl	13.18	172	848250	60.06	ng	0.00
79) Terphenyl-d14	19.92	244	1443922	53.61	ng	0.00
Target Compounds						
50) Dimethylphthalate	14.01	163	213018	12.771	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG083120\
Data File : BG046476.D
Acq On : 31 Aug 2020 19:52
Operator : CG/JU
Sample : L3847-23
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
LINDEN-JOP-BH-11-C

Quant Time: Sep 01 04:08:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 31 16:05:33 2020
Response via : Initial Calibration

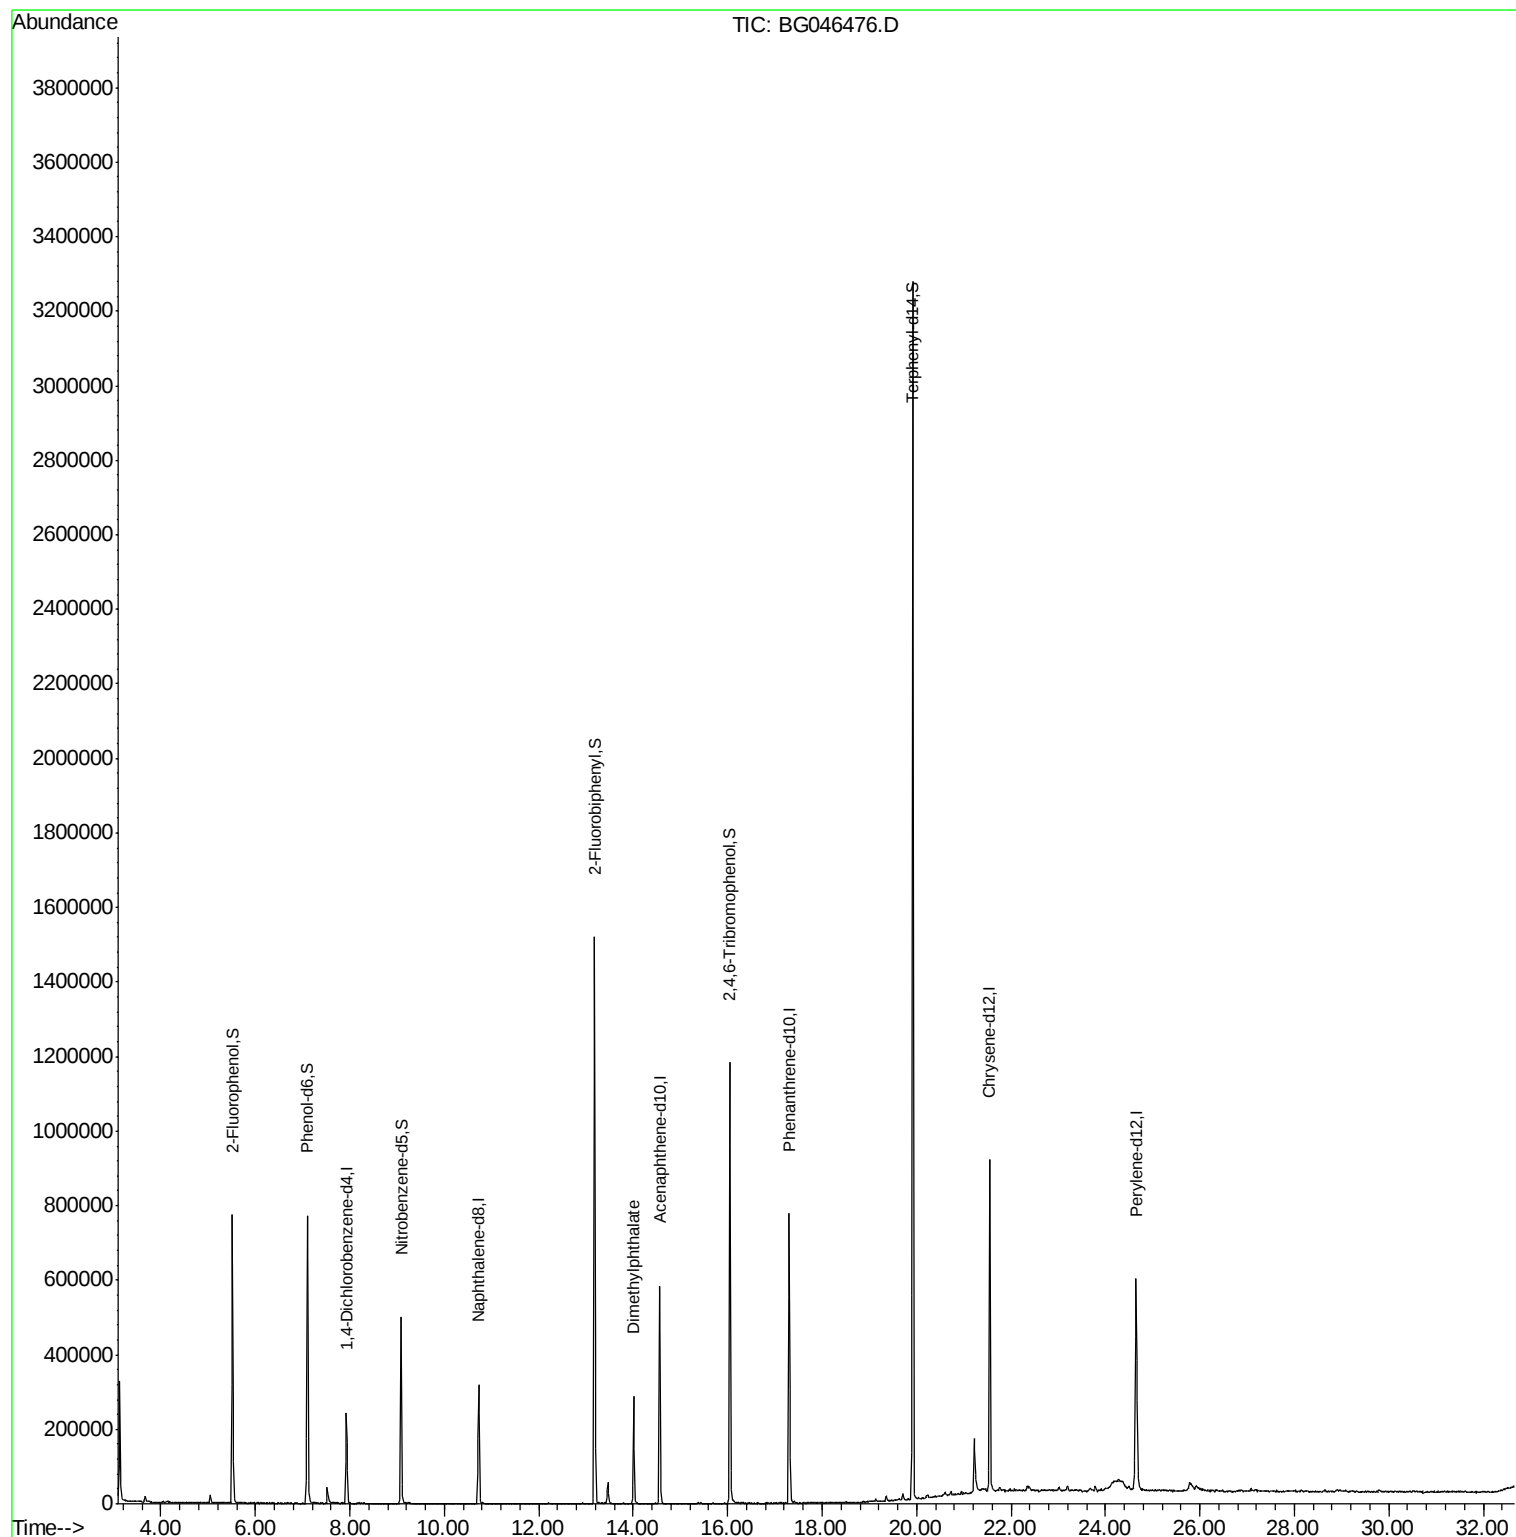

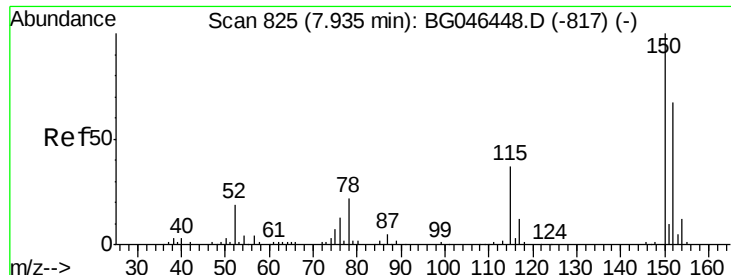


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.93 min Scan# 824
Delta R.T. -0.00 min
Lab File: BG046476.D
Acq: 31 Aug 2020 19:52

Instrument :
BNA_G
ClientSampleId :
LINDEN-JOP-BH-11-C

Tot Ion:152 Resp: 75663
Ion Ratio Lower Upper
152 100
150 150.5 119.5 179.3
115 54.5 44.3 66.5

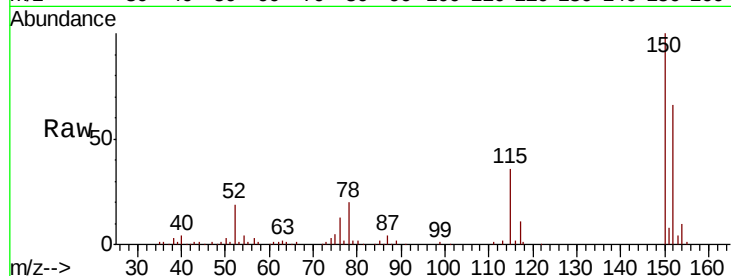


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

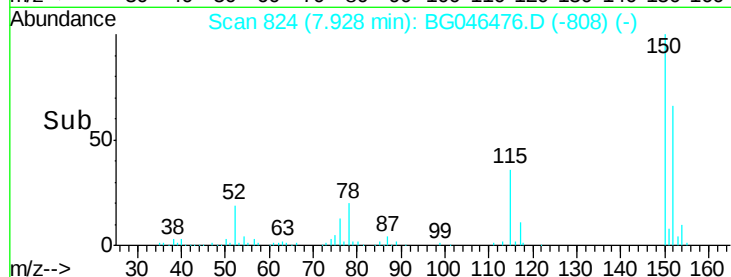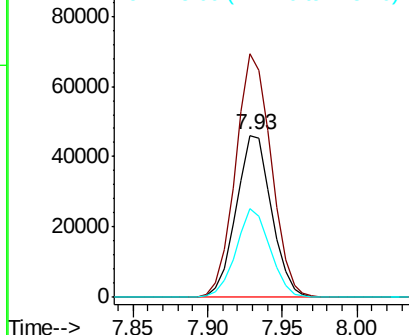



#5

2-Fluorophenol
Concen: 87.323 ng
RT: 5.51 min Scan# 413
Delta R.T. 0.00 min
Lab File: BG046476.D
Acq: 31 Aug 2020 19:52

Tgt Ion:112 Resp: 373033
Ion Ratio Lower Upper
112 100
64 61.0 47.0 70.6
63 30.4 23.5 35.3

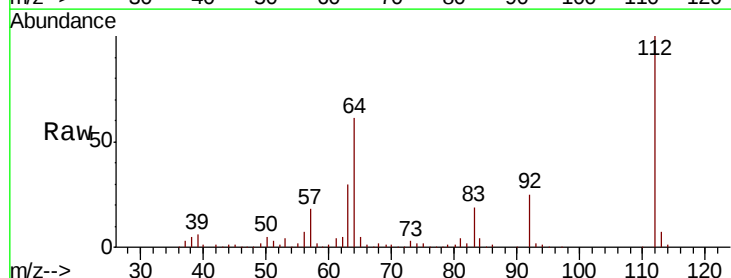

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

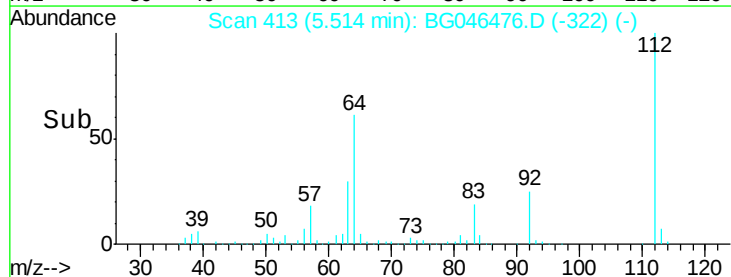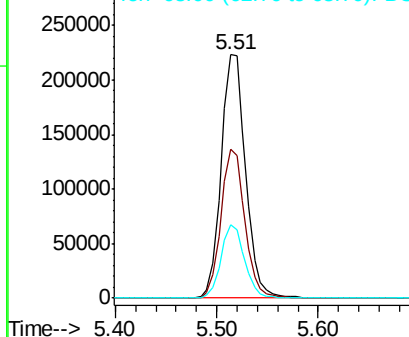



#7

Phenol-d6

Concen: 82.552 ng

RT: 7.10 min Scan# 683

Delta R.T. -0.00 min

Lab File: BG046476.D

Acq: 31 Aug 2020 19:52

Instrument :

BNA_G

ClientSampleId :

LINDEN-JOP-BH-11-C


Tot Ion: 99 Resp: 499925

Ion Ratio Lower Upper



99 100

42 16.4 13.3 19.9

71 32.1 25.3 37.9

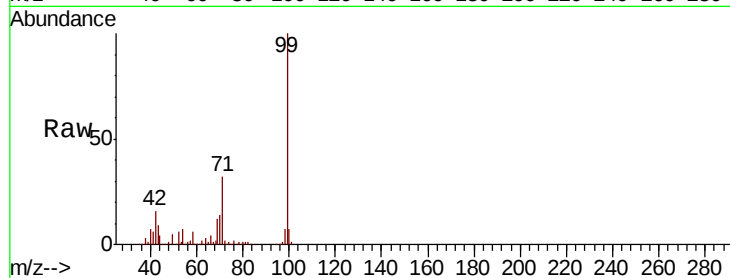

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

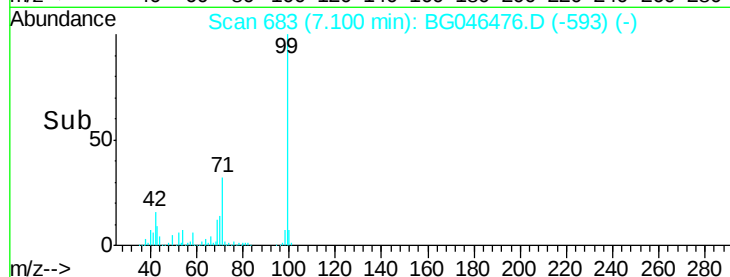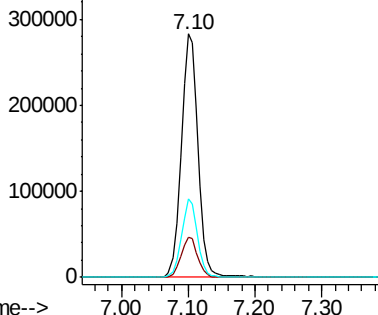

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.73 min Scan# 1301

Delta R.T. 0.00 min

Lab File: BG046476.D

Acq: 31 Aug 2020 19:52

Tgt Ion: 136 Resp: 310399


Ion Ratio Lower Upper

136 100



137 10.6 8.8 13.2


54 7.7 6.1 9.1

68 6.3 4.8 7.2

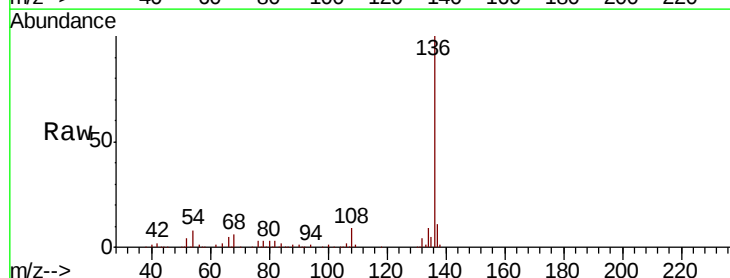

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

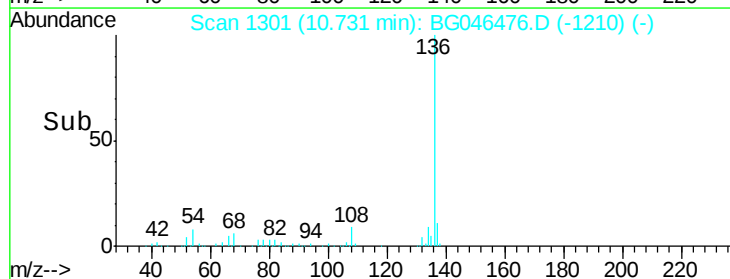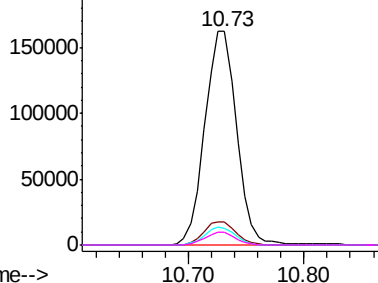


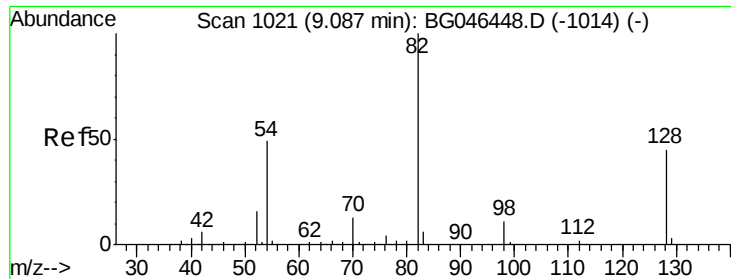




#23
 Nitrobenzene-d5
 Concen: 58.642 ng
 RT: 9.09 min Scan# 1021
 Delta R.T. 0.00 min
 Lab File: BG046476.D
 Acq: 31 Aug 2020 19:52

Instrument :
 BNA_G
 ClientSampleId :
 LINDEN-JOP-BH-11-C

Tot Ion: 82 Resp: 318473
 Ion Ratio Lower Upper
 82 100
 128 45.7 35.7 53.5
 54 48.1 39.4 59.0

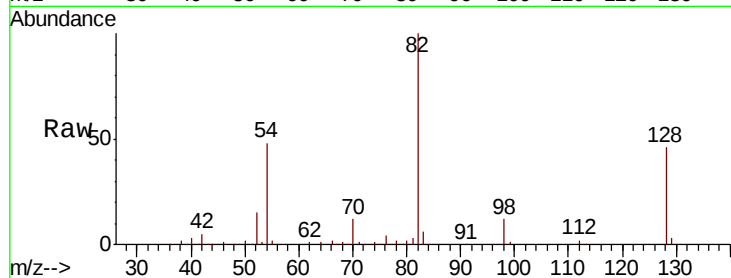


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

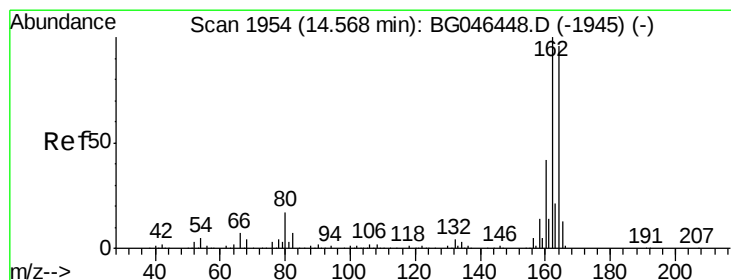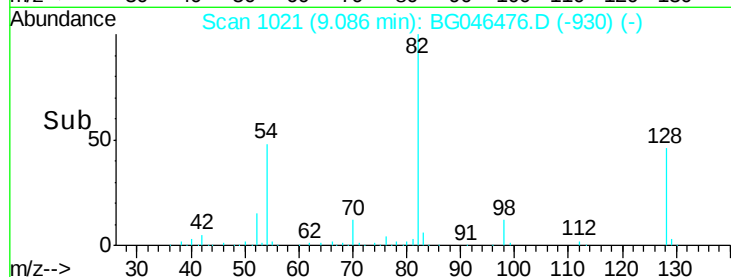
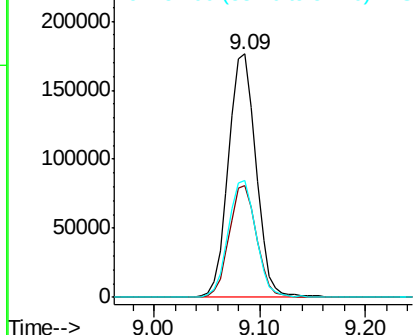



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.56 min Scan# 1953
 Delta R.T. 0.00 min
 Lab File: BG046476.D
 Acq: 31 Aug 2020 19:52

Tgt Ion:164 Resp: 215599
 Ion Ratio Lower Upper
 164 100
 162 103.8 83.3 124.9
 160 45.8 35.0 52.6

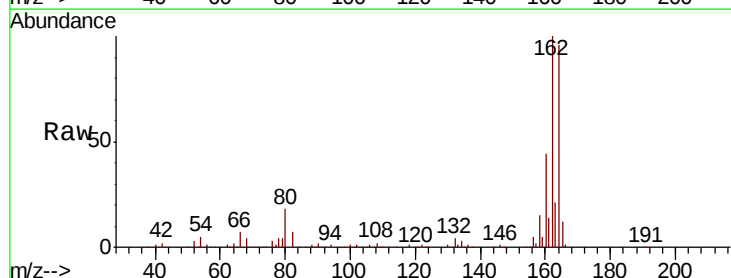

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

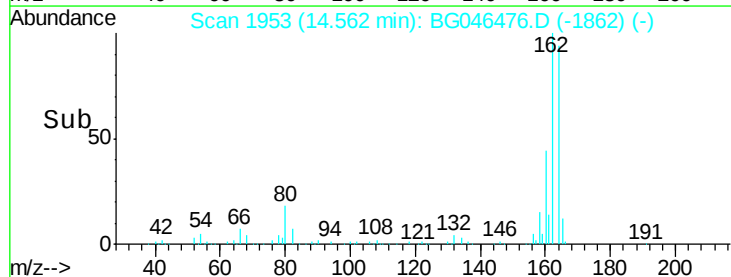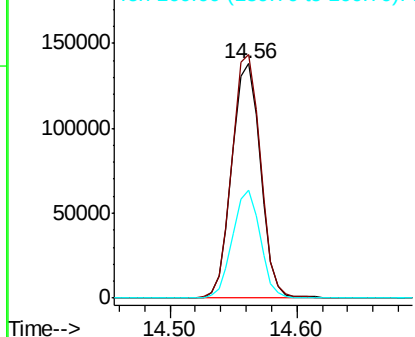


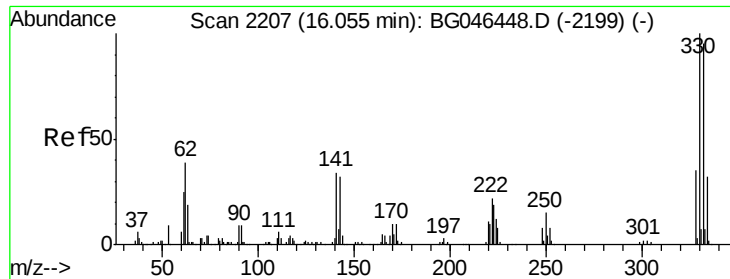




#42
 2,4,6-Tribromophenol
 Concen: 81.732 ng
 RT: 16.05 min Scan# 2206
 Delta R.T. -0.00 min
 Lab File: BG046476.D
 Acq: 31 Aug 2020 19:52

Instrument :
 BNA_G
 ClientSampleId :
 LINDEN-JOP-BH-11-C

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.4	76.1	114.1
141	33.0	26.1	39.1

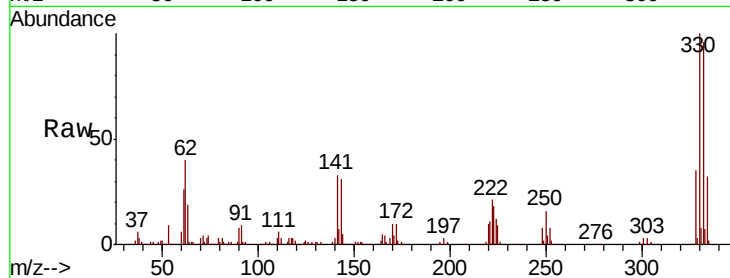


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

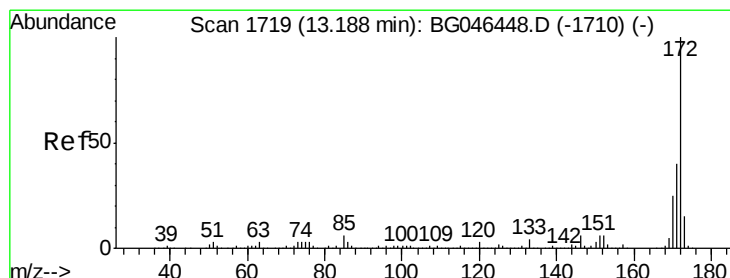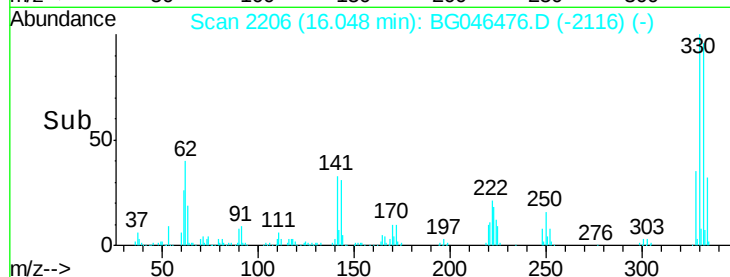
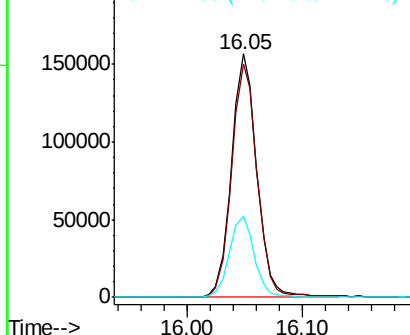



#45
 2-Fluorobiphenyl
 Concen: 60.061 ng
 RT: 13.18 min Scan# 1718
 Delta R.T. -0.00 min
 Lab File: BG046476.D
 Acq: 31 Aug 2020 19:52

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.0	31.8	47.6
170	24.8	20.3	30.5

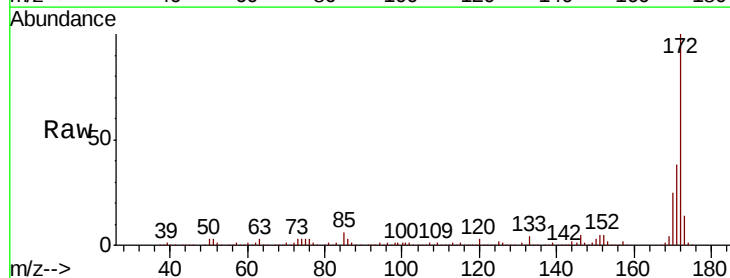

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

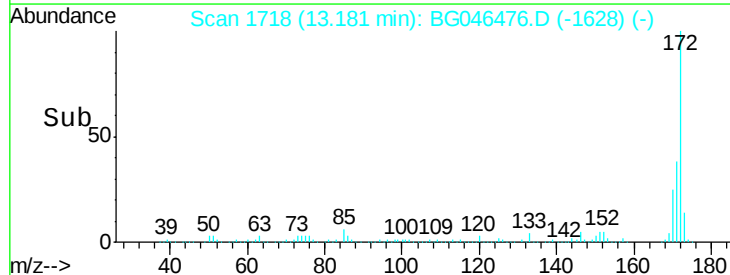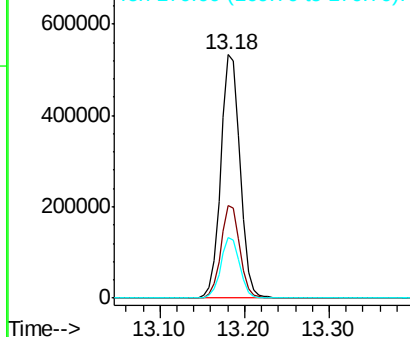

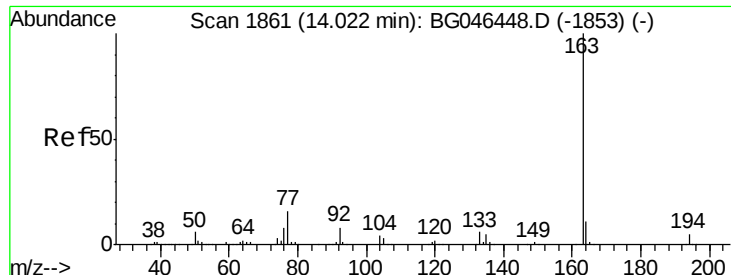

#50

Dimethylphthalate

Concen: 12.771 ng

RT: 14.01 min Scan# 1859

Delta R.T. -0.01 min

Lab File: BG046476.D

Acq: 31 Aug 2020 19:52

Instrument :

BNA_G

ClientSampleId :

LINDEN-JOP-BH-11-C


Tot Ion:163 Resp: 213018

Ion Ratio Lower Upper

163 100

194 4.4 3.7 5.5




164 10.8 8.6 12.8

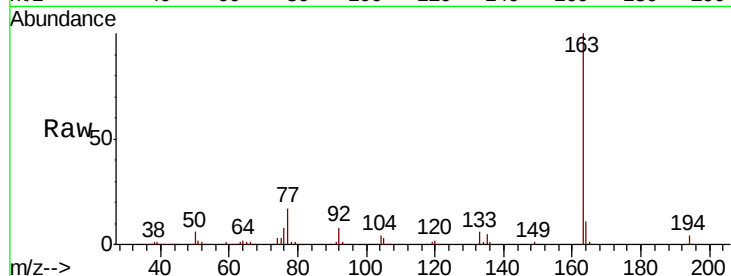

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

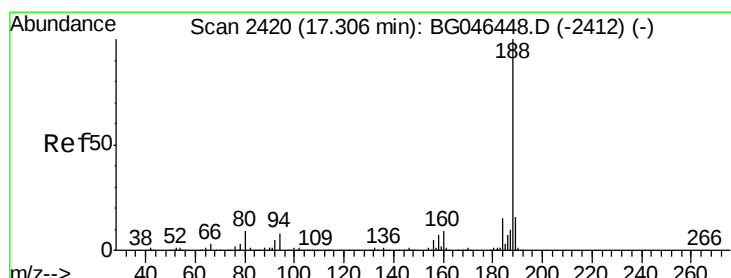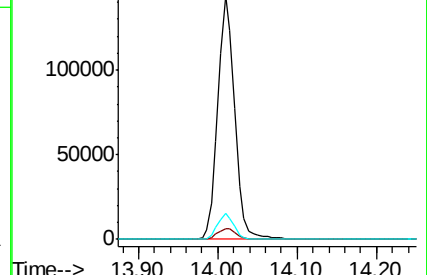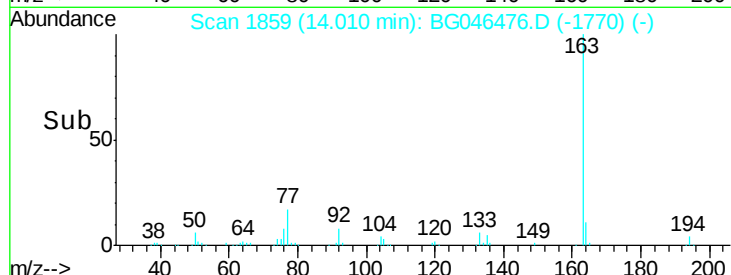

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.30 min Scan# 2419

Delta R.T. -0.00 min

Lab File: BG046476.D

Acq: 31 Aug 2020 19:52


Tgt Ion:188 Resp: 545984

Ion Ratio Lower Upper

188 100

94 7.3 6.3 9.5



80 8.6 6.9 10.3

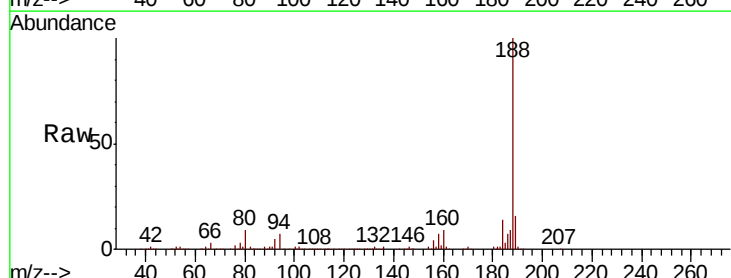


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG0

Ion 80.00 (79.70 to 80.70): BG0

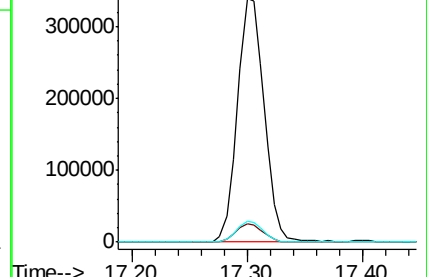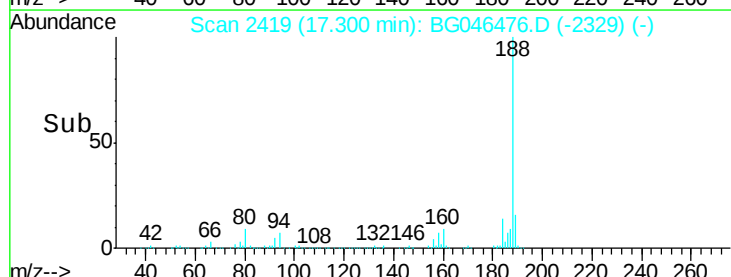

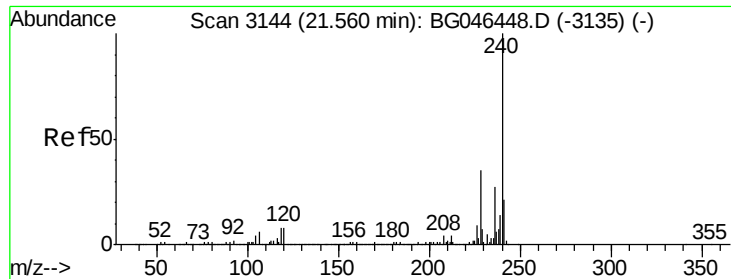

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.55 min Scan# 3142

Delta R.T. -0.01 min

Lab File: BG046476.D

Acq: 31 Aug 2020 19:52

Instrument :

BNA_G

ClientSampleId :

LINDEN-JOP-BH-11-C


Tot Ion:240 Resp: 573242

Ion Ratio Lower Upper

240 100

120 8.5 6.6 10.0




236 25.4 21.4 32.2

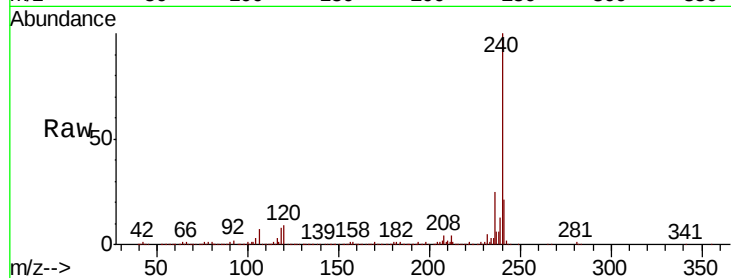

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

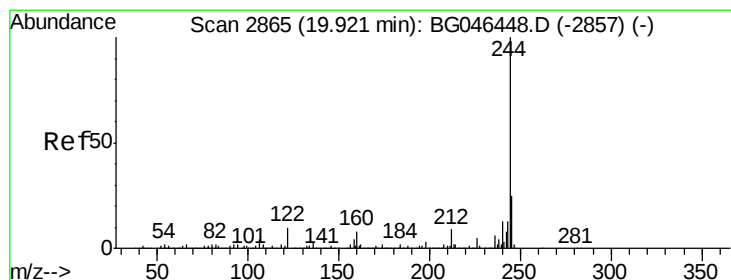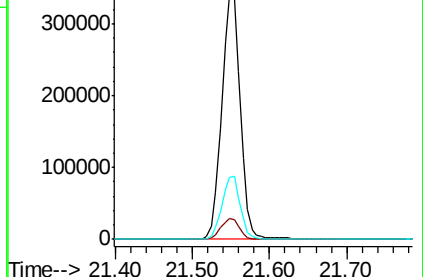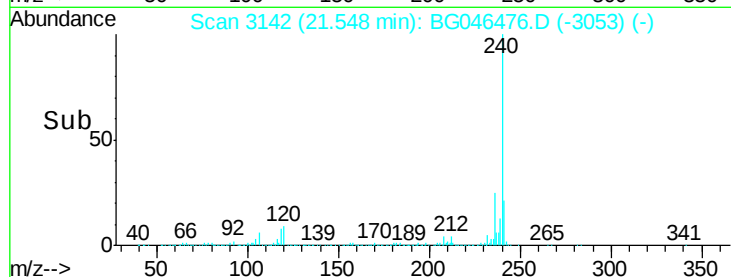

#79

Terphenyl-d14

Concen: 53.606 ng

RT: 19.92 min Scan# 2865

Delta R.T. 0.00 min

Lab File: BG046476.D

Acq: 31 Aug 2020 19:52


Tgt Ion:244 Resp: 1443922

Ion Ratio Lower Upper

244 100

212 7.9 6.9 10.3



122 9.2 8.2 12.4

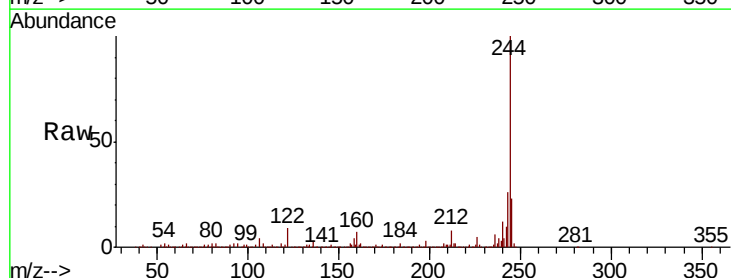


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

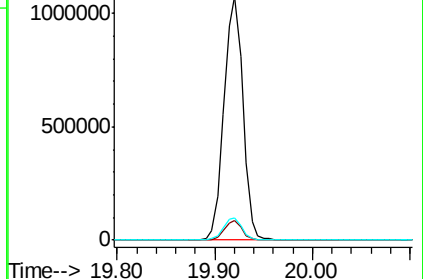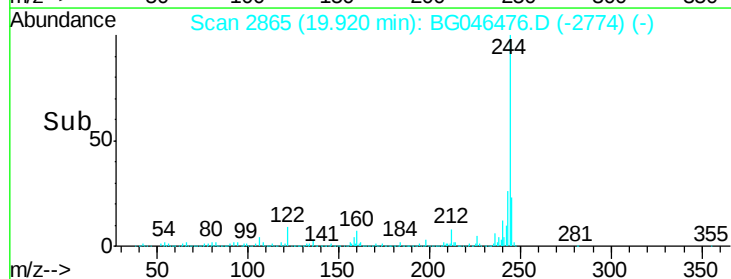

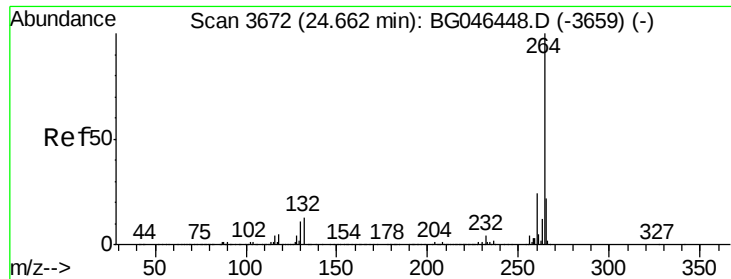

#86
Pervlene-d12
Concen: 20.000 ng
RT: 24.65 min Scan# 3670
Delta R.T. -0.00 min
Lab File: BG046476.D
Acq: 31 Aug 2020 19:52

Instrument :
BNA_G
ClientSampleId :
LINDEN-JOP-BH-11-C

Tot Ion:	264	Resp:	583165
Ion	Ratio	Lower	Upper
264	100		
260	23.3	19.2	28.8
265	22.4	17.9	26.9

