


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG083120\
 Data File : BG046469.D
 Acq On : 31 Aug 2020 14:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 31 16:05:33 2020

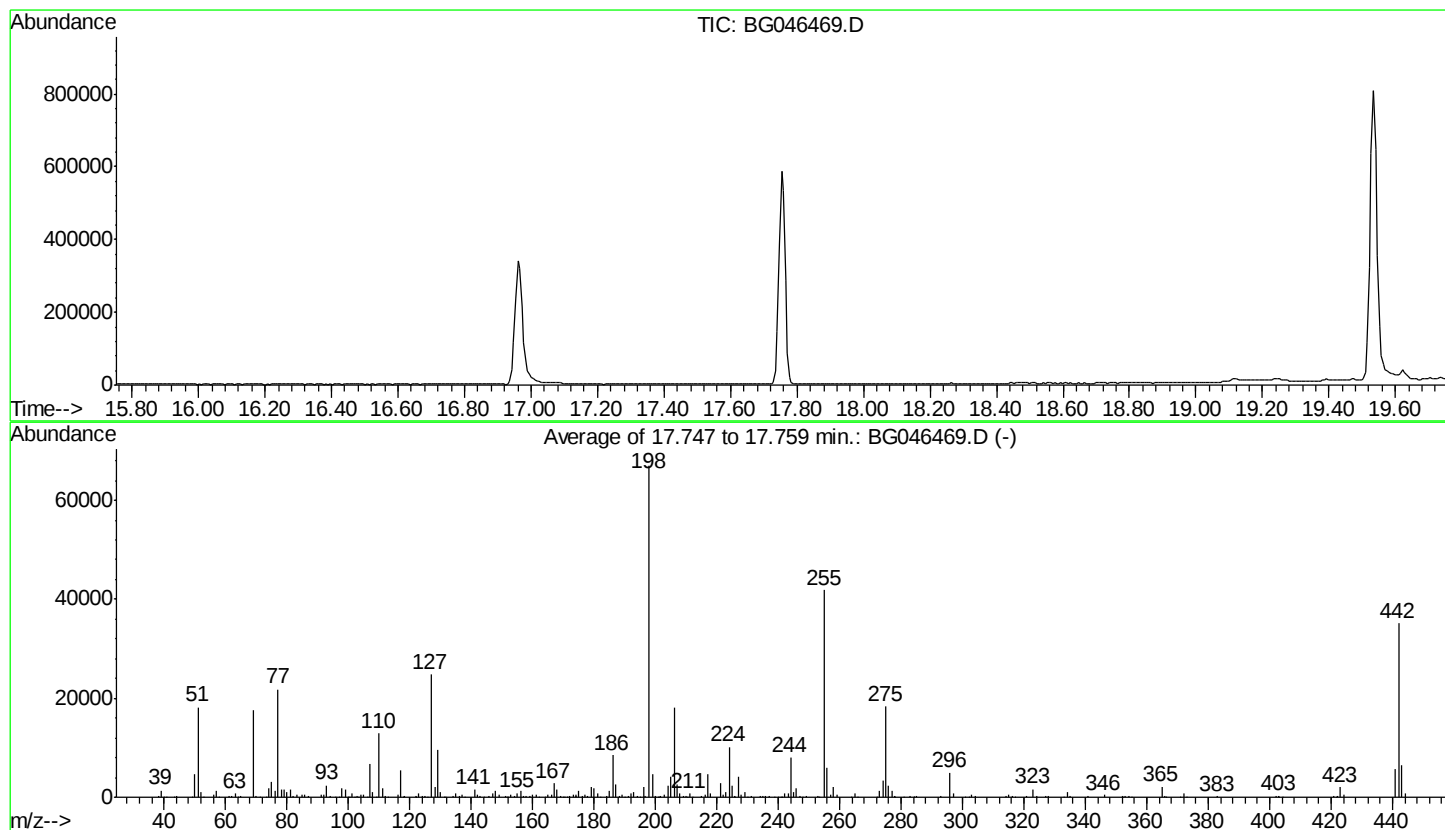

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.0	18123	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	26.2	17540	PASS
70	69	0.00	2	0.8	140	PASS
127	198	10	80	36.9	24752	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67008	PASS
199	198	5	9	7.0	4705	PASS
275	198	10	60	27.2	18258	PASS
365	198	1	100	3.1	2083	PASS
441	198	0.01	100	8.5	5686	PASS
442	198	50	100	52.5	35178	PASS
443	442	15	24	18.4	6487	PASS