
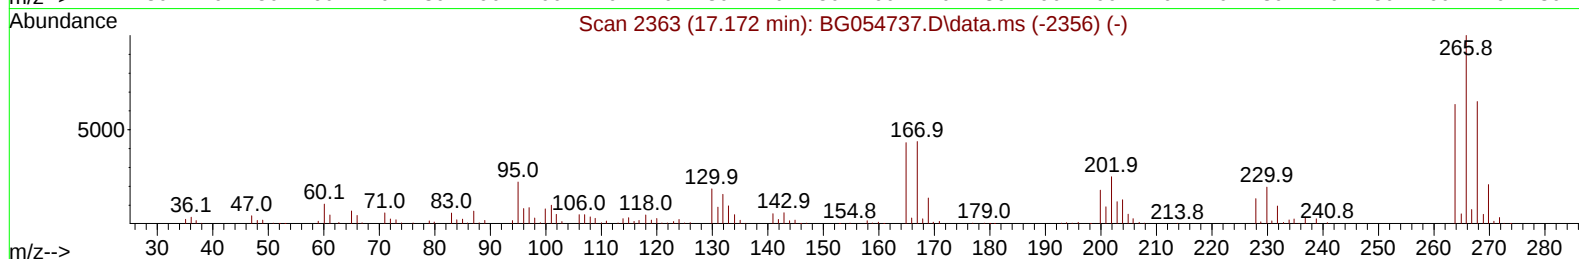
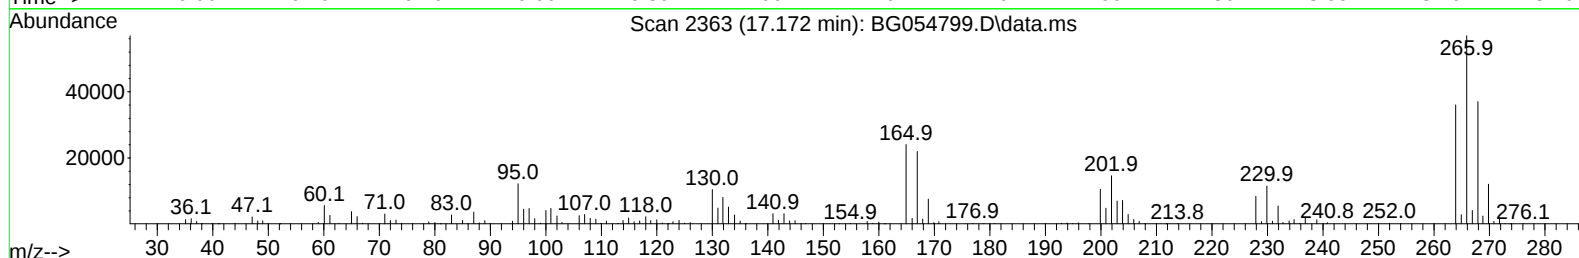


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083122\
Data File : BG054799.D
Acq On : 31 Aug 2022 9:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 06:34:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

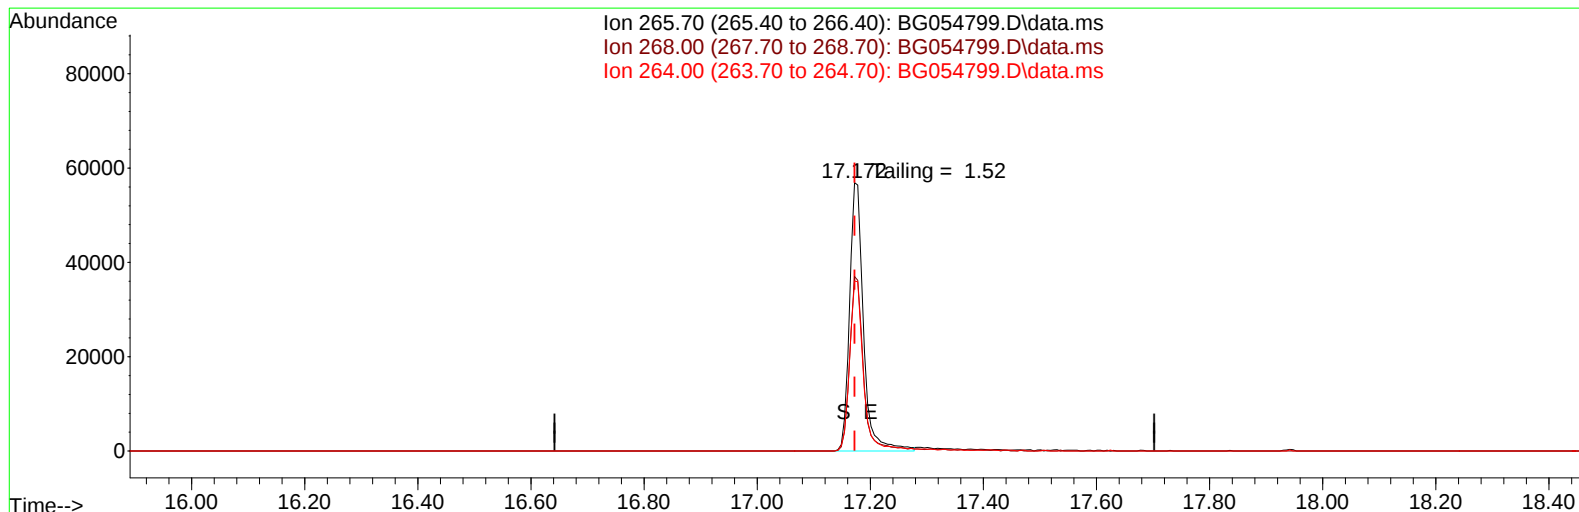

TIC: BG054799.D\data.ms

(70) Pentachlorophenol (C)




17.172min (-0.000) 24988.33 ng

response 97863

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	65.01
264.00	61.70	63.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083122\
Data File : BG054799.D
Acq On : 31 Aug 2022 9:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 06:34:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

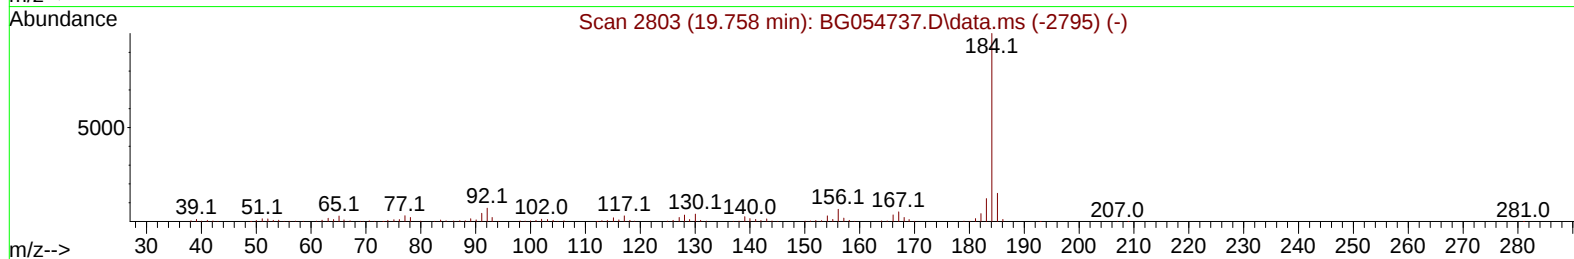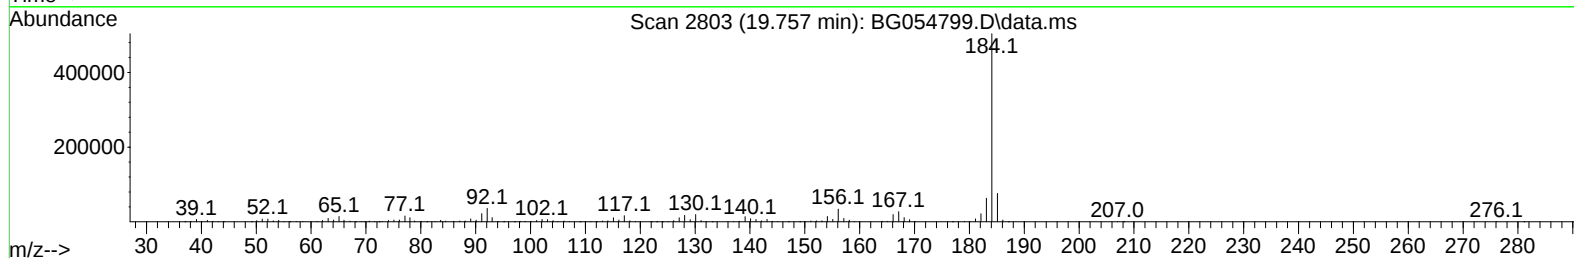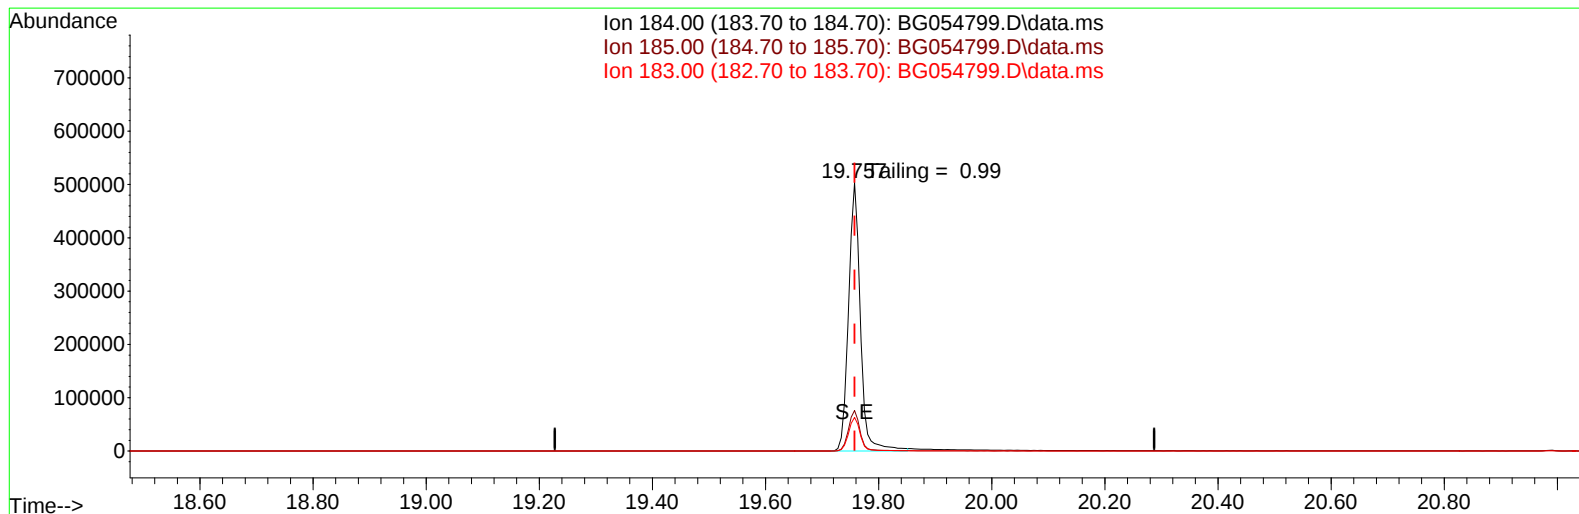

TIC: BG054799.D\data.ms

(77) Benzidine

19.757min (-0.000) 0.00 ng

response 745963

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	15.10
183.00	12.30	12.56
0.00	0.00	0.00