


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083122\
 Data File : BG054799.D
 Acq On : 31 Aug 2022 9:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 25 17:50:55 2022

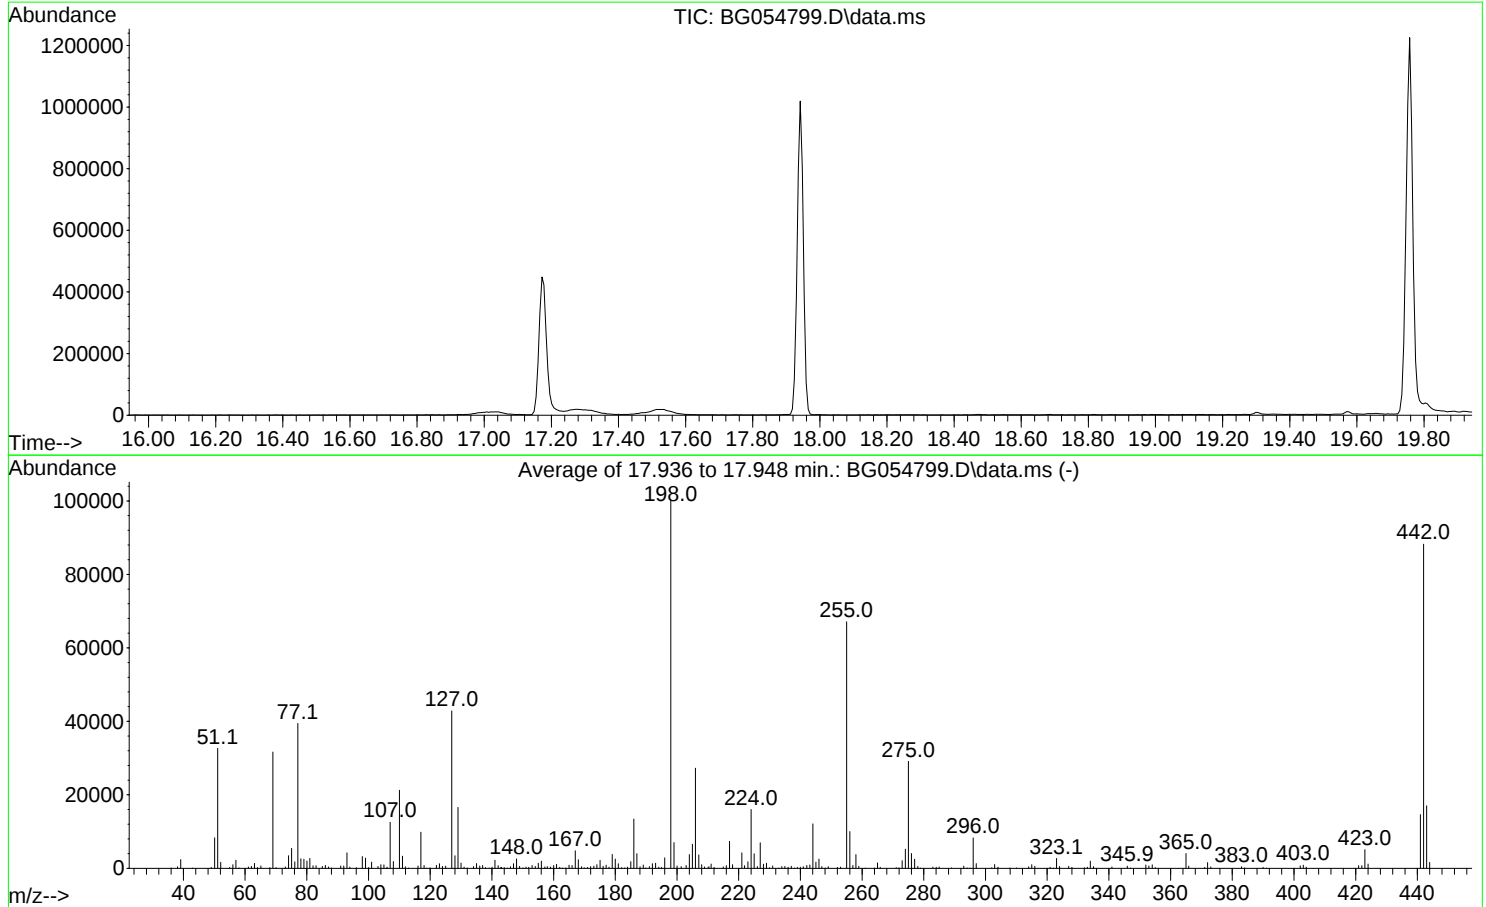




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	32648	PASS
68	69	0.00	2	0.5	164	PASS
69	198	0.00	100	31.6	31632	PASS
70	69	0.00	2	0.7	212	PASS
127	198	10	80	42.8	42824	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	100139	PASS
199	198	5	9	7.0	7010	PASS
275	198	10	60	29.1	29101	PASS
365	198	1	100	4.0	4027	PASS
441	198	0.01	100	14.6	14611	PASS
442	442	50	100	100.0	88243	PASS
443	442	15	24	19.3	17008	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083122\
Data File : BG054799.D
Acq On : 31 Aug 2022 9:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 01 06:34:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

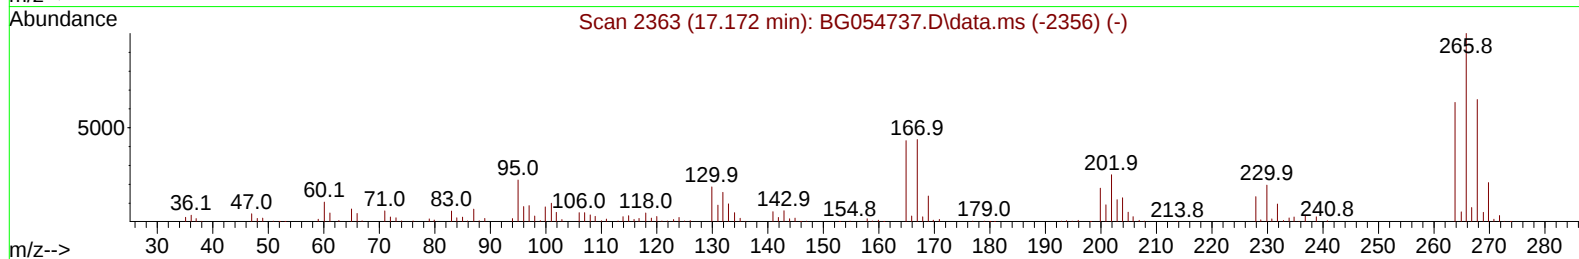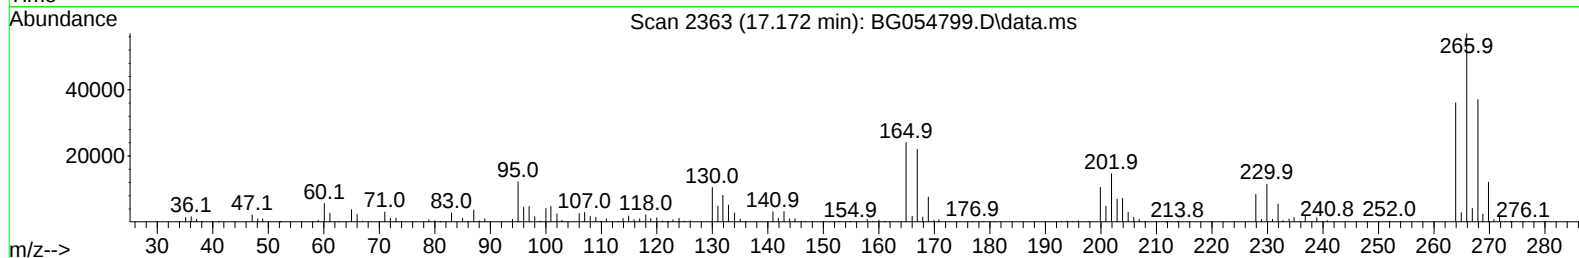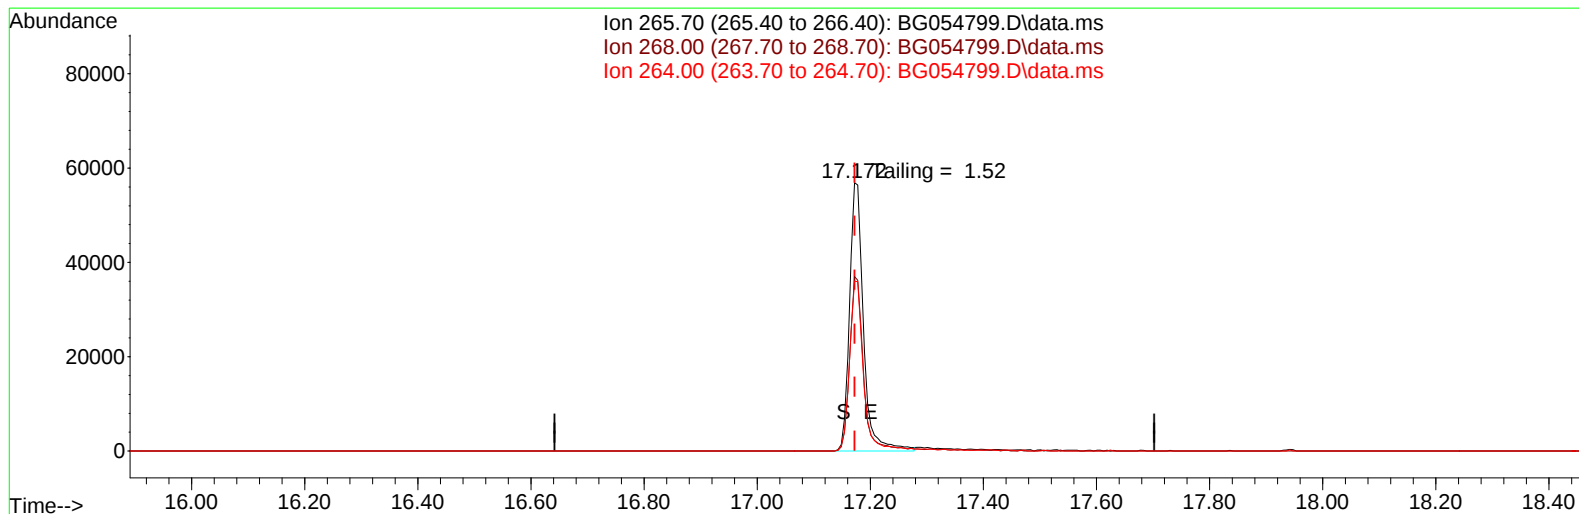

TIC: BG054799.D\data.ms

(70) Pentachlorophenol (C)

17.172min (-0.000) 24988.33 ng




response 97863

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	65.01
264.00	61.70	63.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG083122\
Data File : BG054799.D
Acq On : 31 Aug 2022 9:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 01 06:34:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

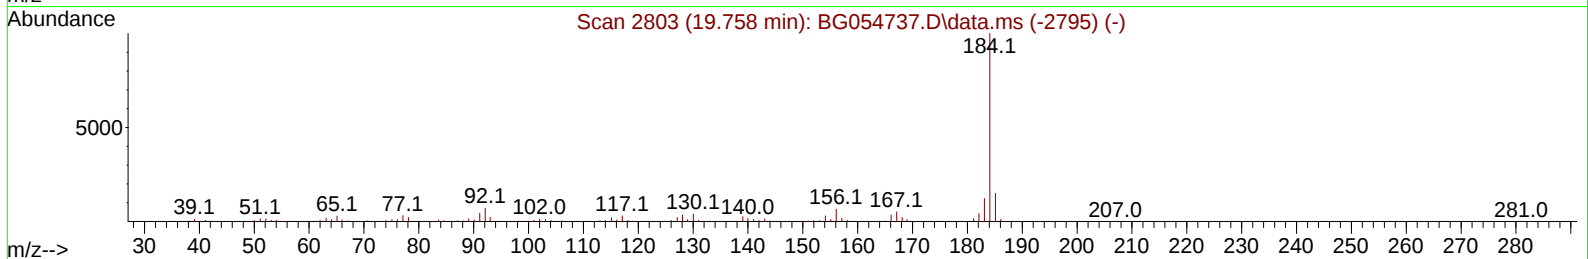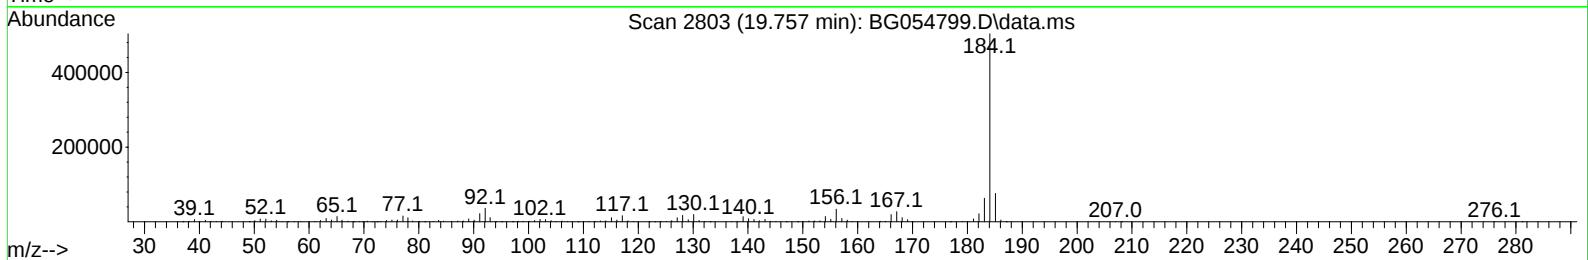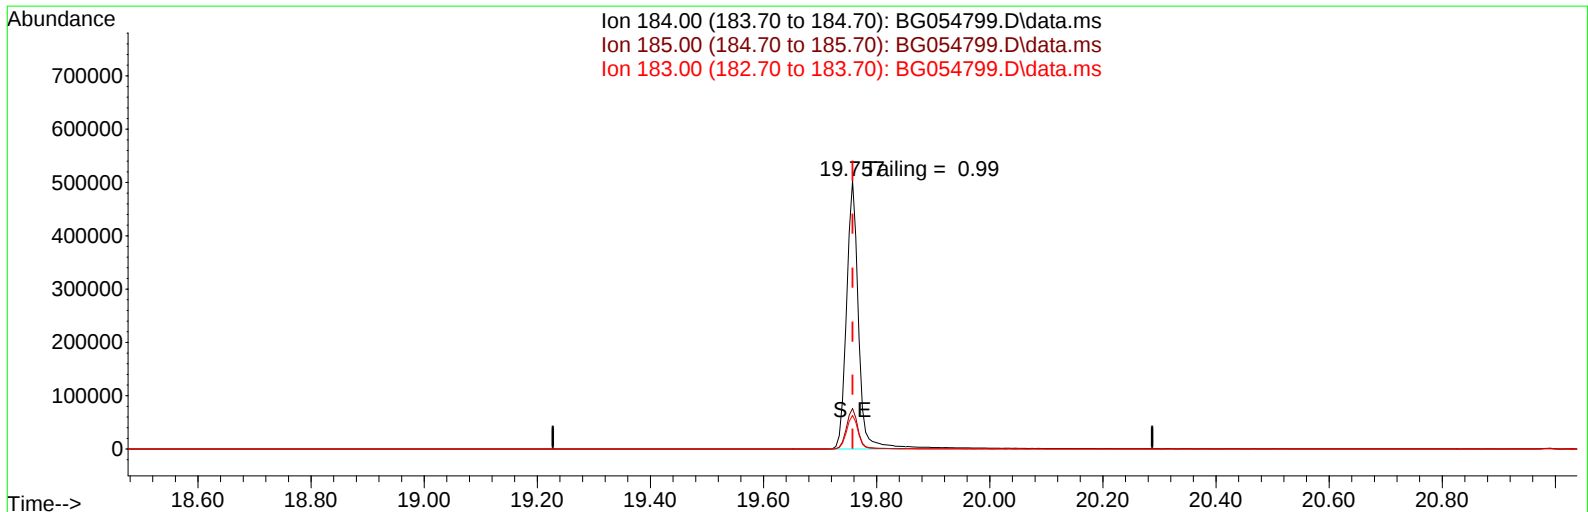

TIC: BG054799.D\data.ms

(77) Benzidine

19.757min (-0.000) 0.00 ng

response 745963

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	15.10
183.00	12.30	12.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/31/2022	BNA_G	BG054799.D
Compound Name	Response	Retention Time
DDT	329896	20.991
DDD	7804	20.539
DDE	720	20.33
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8524	338420	2.52

Instrument :
BNA_G
ClientSampleId :
DFTPP