

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG090115\
 Data File : BG018566.D
 Acq On : 1 Sep 2015 16:56
 Operator : UM/IZ
 Sample : G3478-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF4

Quant Time: Sep 02 02:20:01 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 02 02:18:07 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	96153	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	411321	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	273768	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.38	188	736529	20.00	ng/ul	0.00
78) Chrysene-d12	21.63	240	798895	20.00	ng/ul	-0.01
86) Perylene-d12	24.83	264	793455	20.00	ng/ul	-0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.45	96	8811	4.05	ng/uL	0.00
5) Phenol-d5	7.17	99	185499	21.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	111281	20.58	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	134336	20.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	151936	20.72	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	70599	22.02	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	61676	18.89	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	149692	21.60	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	193807	24.74	ng/ul	0.00
44) Dimethylphthalate-d6	14.04	166	558724	24.26	ng/ul	0.00
47) Acenaphthylene-d8	14.32	160	459666	15.85	ng/ul	0.00
52) 4-Nitrophenol-d4	14.82	143	93876	22.66	ng/ul	0.00
58) Fluorene-d10	15.62	176	282973	14.10	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	51619	14.25	ng/ul	-0.01
71) Anthracene-d10	17.47	188	434445	12.33	ng/ul	0.00
79) Pyrene-d10	19.76	212	384367	9.27	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.60	264	335490	7.96	ng/ul	-0.02


Target Compounds					Qvalue
45) Dimethylphthalate	14.08	163	283249	12.47 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG090115\
Data File : BG018566.D
Acq On : 1 Sep 2015 16:56
Operator : UM/IZ
Sample : G3478-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF4

Quant Time: Sep 02 02:20:01 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 02 02:18:07 2015
Response via : Initial Calibration

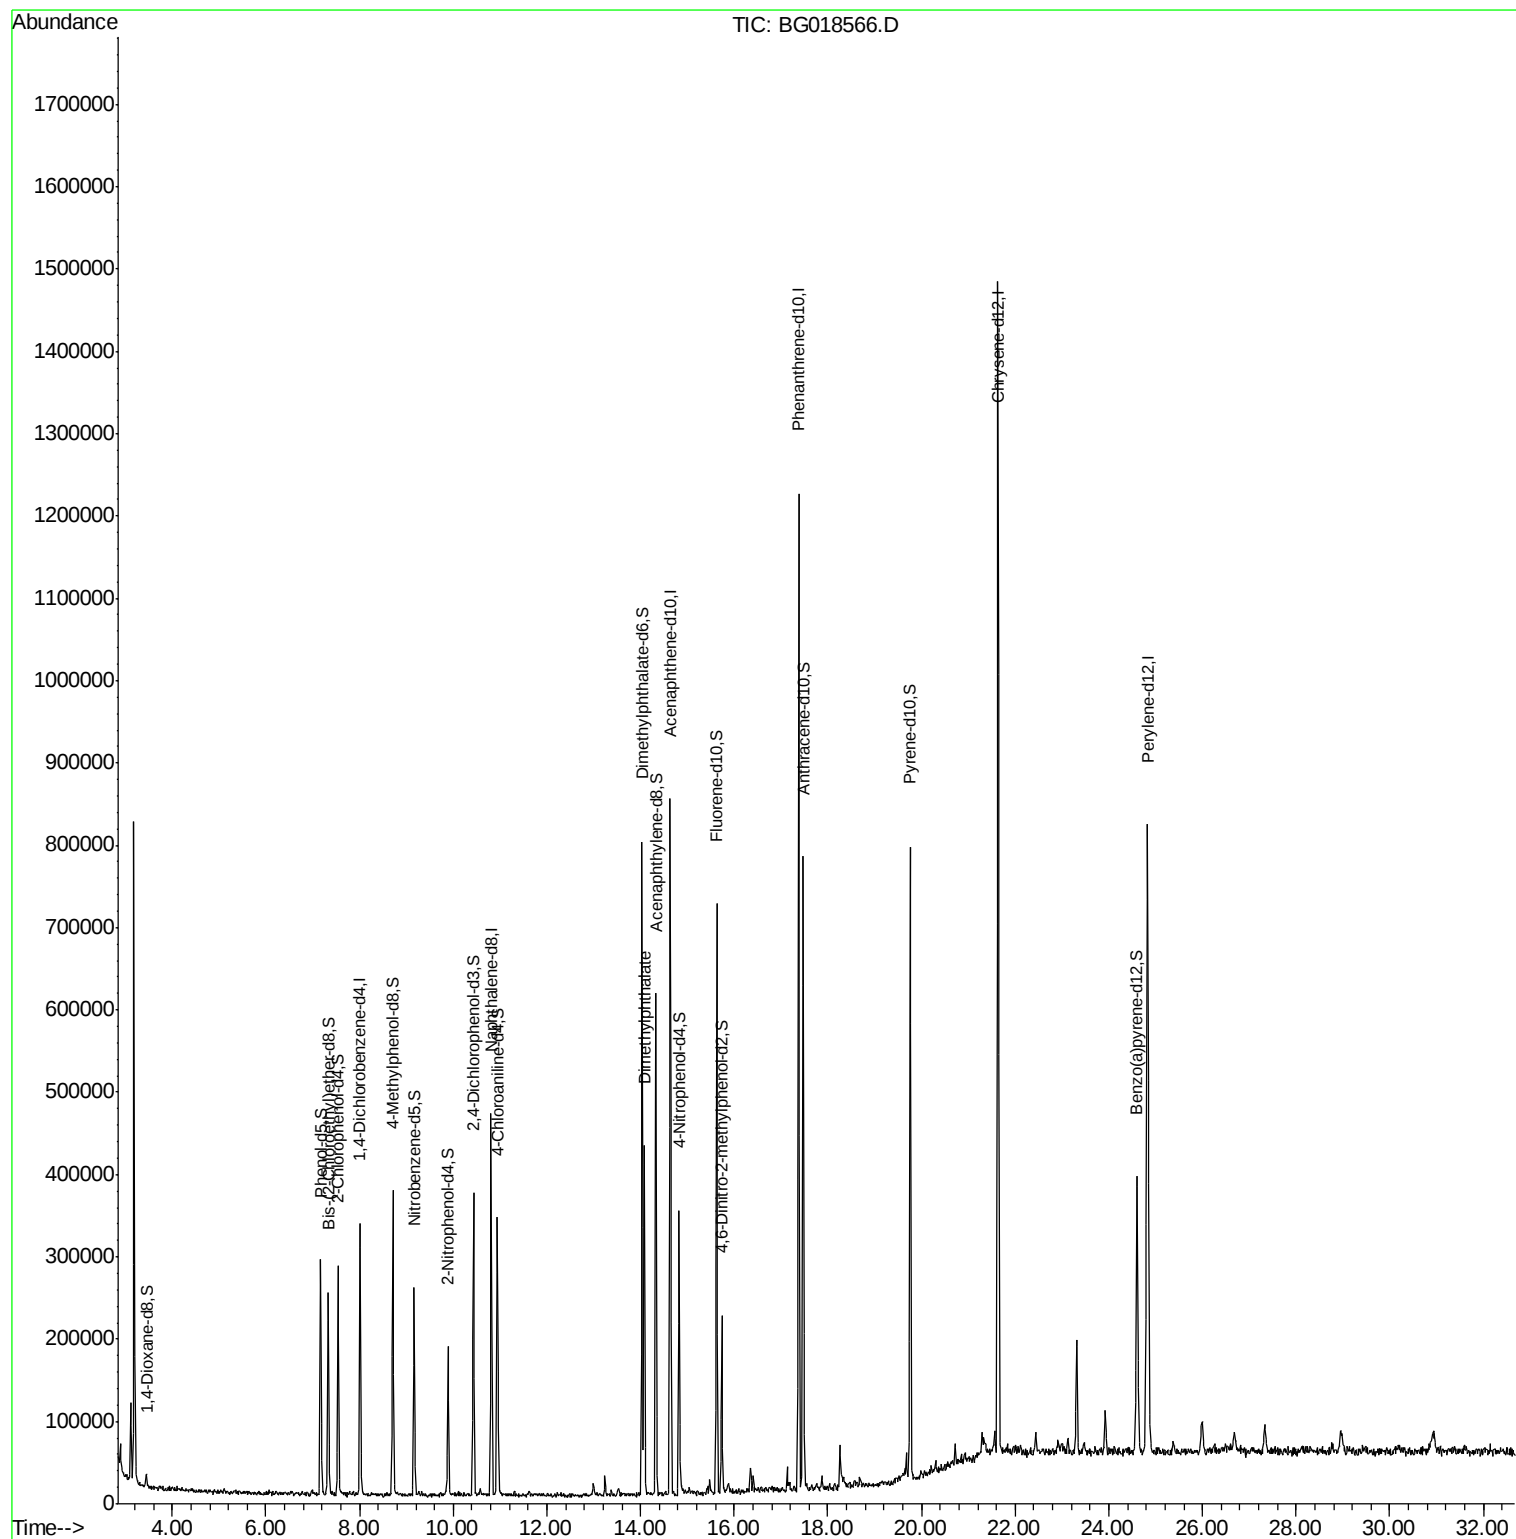

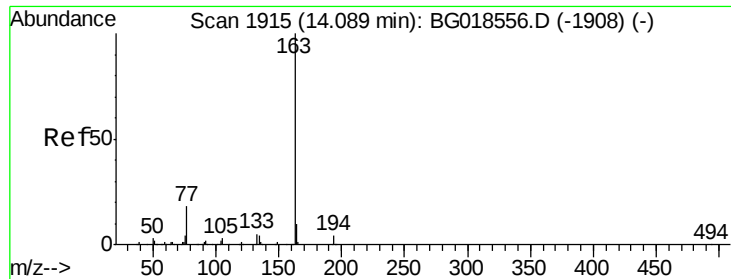

#45
 Dimethylphthalate
 Concen: 12.47 ng/ul
 RT: 14.08 min Scan# 1914
 Delta R.T. -0.01 min
 Lab File: BG018566.D
 Acq: 1 Sep 2015 16:56

Instrument :
 BNA_G
 ClientSampleId :
 C0AF4

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.2	2.9	4.3
164	9.7	7.7	11.5

