

Data Path : Z:\HPCHEM1\BNA G\DATA\BG090115\
 Data File : BG018561.D
 Acq On : 1 Sep 2015 13:44
 Operator : UM/IZ
 Sample : G3478-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE9

Quant Time: Sep 02 02:19:21 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 02 02:18:07 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	92839	20.00	ng/ul	0.00
18) Naphthalene-d8	10.82	136	403845	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	274580	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.38	188	737951	20.00	ng/ul	0.00
78) Chrysene-d12	21.64	240	802326	20.00	ng/ul	0.00
86) Perylene-d12	24.83	264	795022	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.44	96	7315	3.48	ng/uL	0.00
5) Phenol-d5	7.17	99	159264	18.90	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	98018	18.77	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	118251	18.32	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	122045	17.24	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	63823	20.27	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	65558	20.45	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	129115	18.97	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	170478	22.17	ng/ul	0.00
44) Dimethylphthalate-d6	14.04	166	487176	21.09	ng/ul	0.00
47) Acenaphthylene-d8	14.33	160	449340	15.45	ng/ul	0.00
52) 4-Nitrophenol-d4	14.82	143	78152	18.81	ng/ul	0.00
58) Fluorene-d10	15.62	176	288885	14.36	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	52770	14.54	ng/ul	-0.01
71) Anthracene-d10	17.47	188	482583	13.67	ng/ul	0.00
79) Pyrene-d10	19.76	212	440996	10.59	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.61	264	407188	9.65	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.08	163	242782	10.65	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG090115\
Data File : BG018561.D
Acq On : 1 Sep 2015 13:44
Operator : UM/IZ
Sample : G3478-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE9

Quant Time: Sep 02 02:19:21 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 02 02:18:07 2015
Response via : Initial Calibration

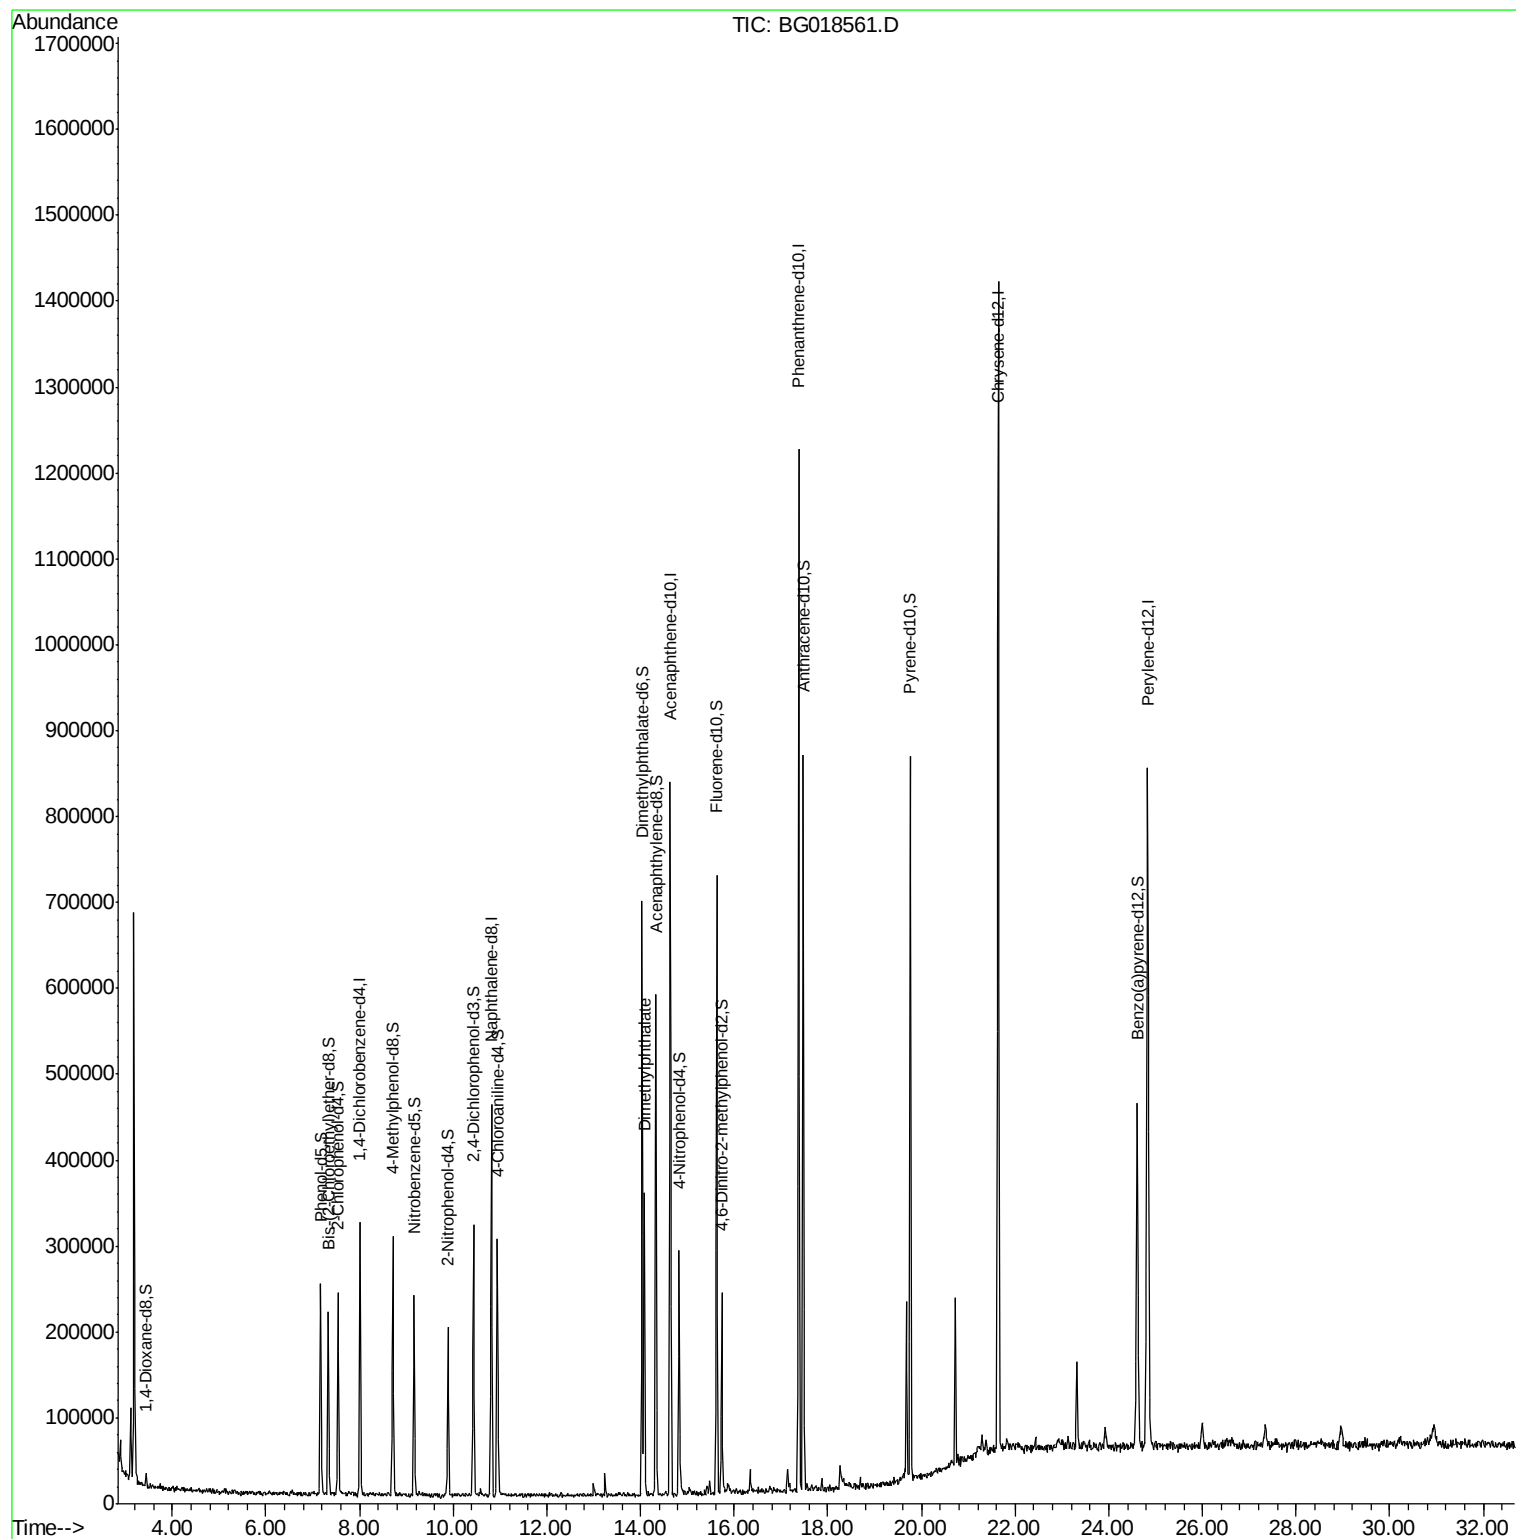

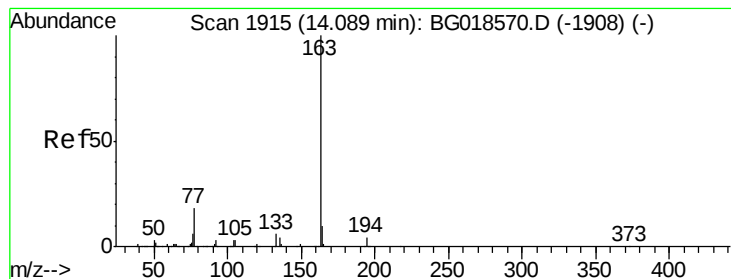

#45

Dimethylphthalate

Concen: 10.65 ng/ul

RT: 14.08 min Scan# 1914

Delta R.T. -0.01 min

Lab File: BG018561.D

Acq: 1 Sep 2015 13:44

Instrument :

BNA_G

ClientSampleId :

C0AE9


Tot Ion:163 Resp: 242782

Ion Ratio Lower Upper

163 100

194 3.6 2.9 4.3

164 9.2 7.7 11.5

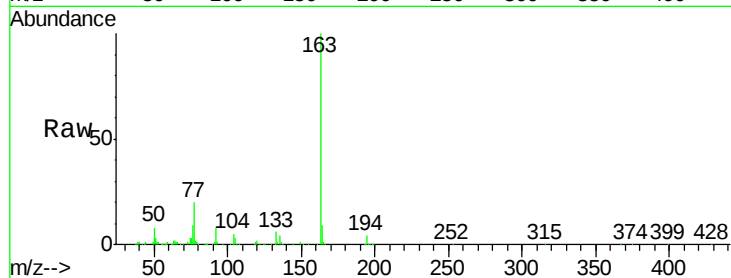

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

