

Data Path : Z:\HPCHEM1\BNA G\DATA\BG090115\
 Data File : BG018562.D
 Acq On : 1 Sep 2015 14:23
 Operator : UM/IZ
 Sample : G3478-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF0

Quant Time: Sep 02 02:19:29 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 02 02:18:07 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	94352	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	401732	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	278918	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.38	188	763228	20.00	ng/ul	0.00
78) Chrysene-d12	21.63	240	829573	20.00	ng/ul	-0.01
86) Perylene-d12	24.83	264	820123	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.45	96	8520	3.99	ng/uL	0.00
5) Phenol-d5	7.17	99	182427	21.30	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	110736	20.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	131994	20.13	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	154852	21.52	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	68682	21.93	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	74020	23.21	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	152613	22.55	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	207279	27.10	ng/ul	0.00
44) Dimethylphthalate-d6	14.04	166	600578	25.59	ng/ul	0.00
47) Acenaphthylene-d8	14.33	160	531637	17.99	ng/ul	0.00
52) 4-Nitrophenol-d4	14.82	143	102221	24.22	ng/ul	0.00
58) Fluorene-d10	15.62	176	350283	17.14	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	64577	17.20	ng/ul	-0.01
71) Anthracene-d10	17.47	188	556350	15.24	ng/ul	0.00
79) Pyrene-d10	19.76	212	523166	12.16	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.61	264	503920	11.57	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.08	163	271658	11.74	ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG090115\
Data File : BG018562.D
Acq On : 1 Sep 2015 14:23
Operator : UM/IZ
Sample : G3478-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF0

Quant Time: Sep 02 02:19:29 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 02 02:18:07 2015
Response via : Initial Calibration

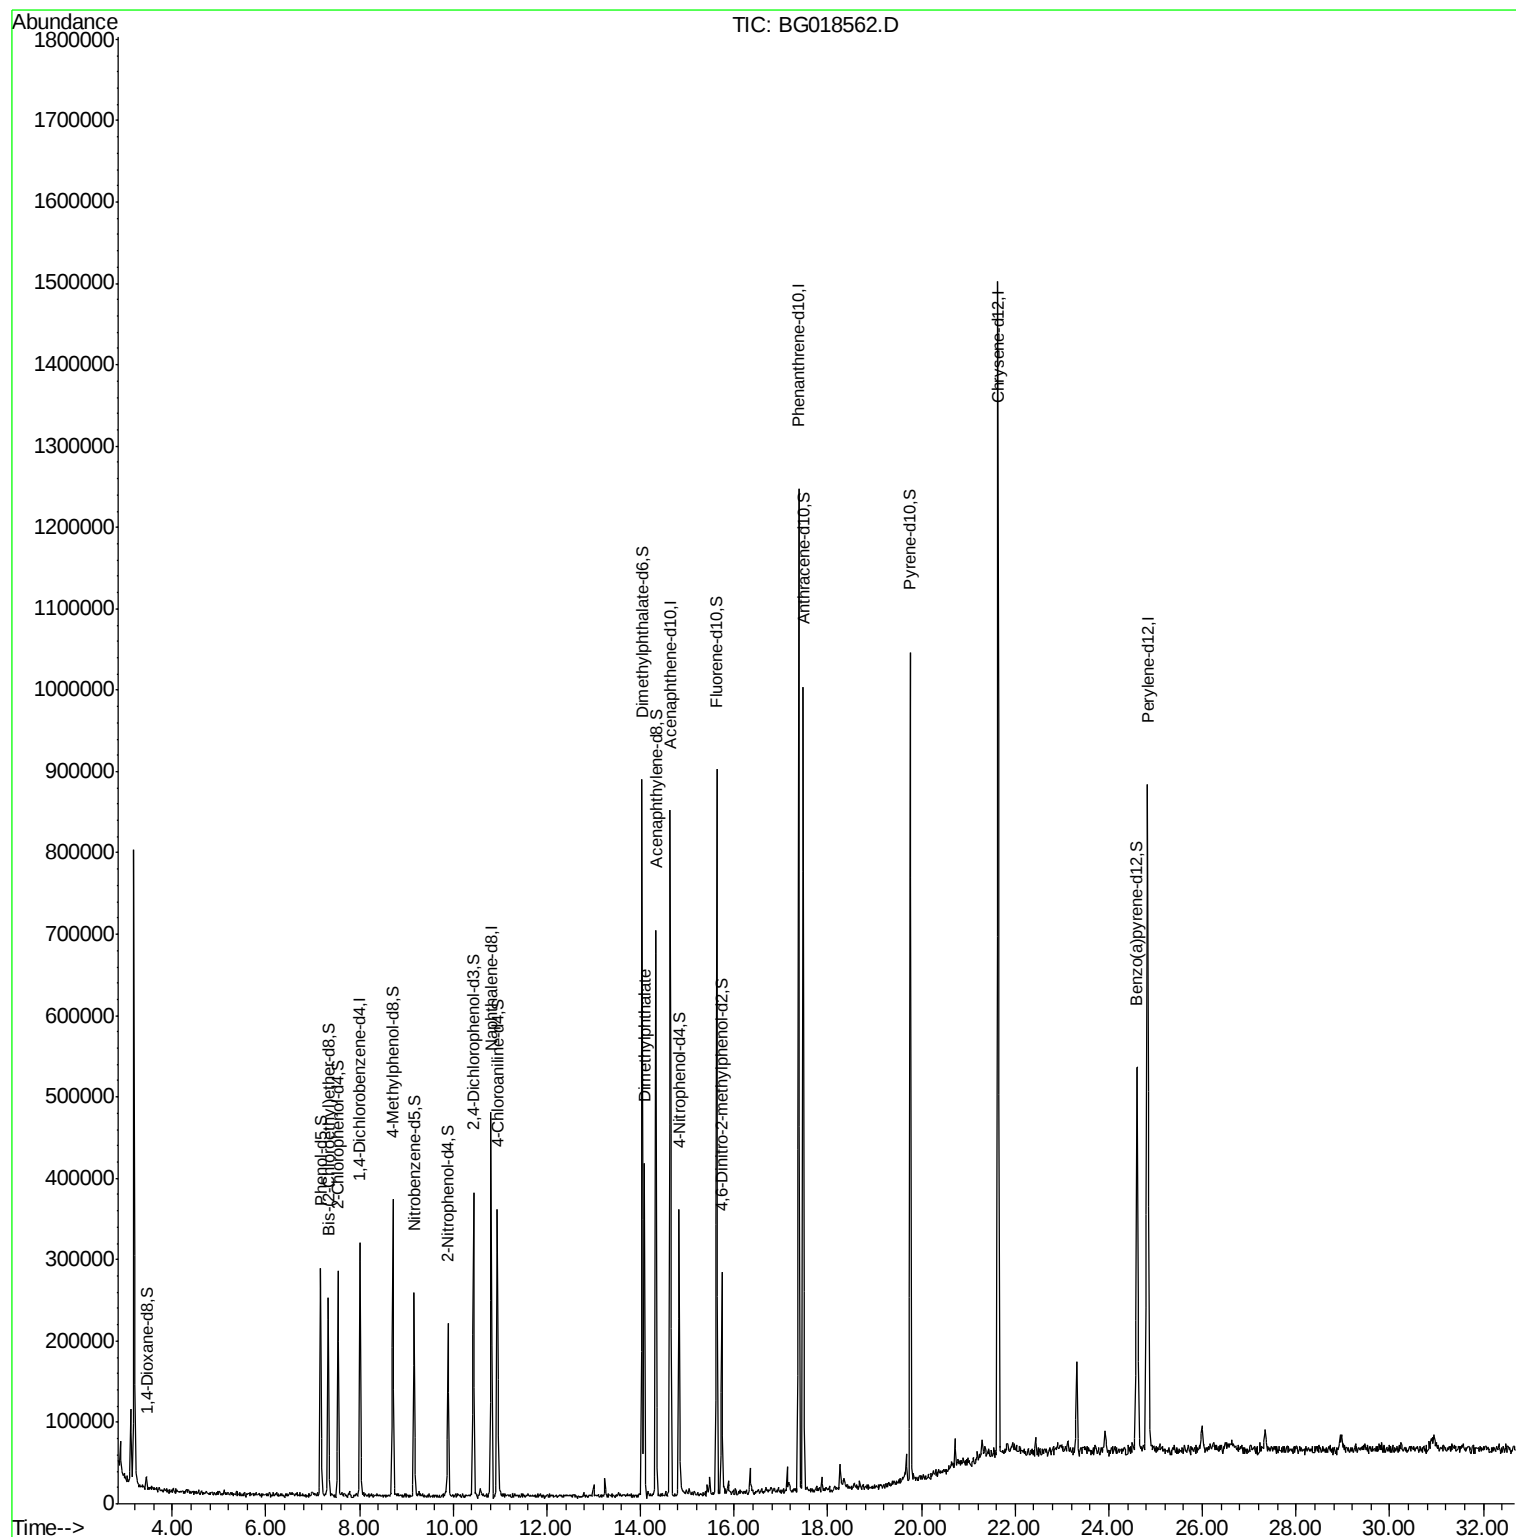

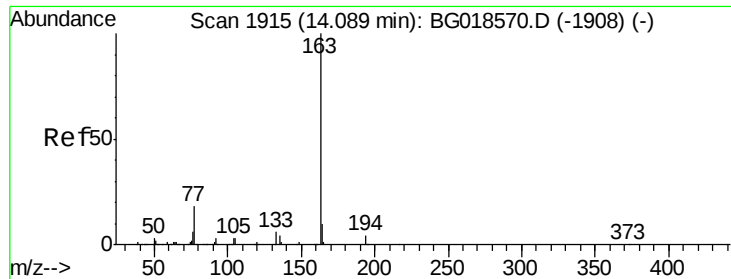

#45
 Dimethylphthalate
 Concen: 11.74 ng/ul
 RT: 14.08 min Scan# 1914
 Delta R.T. -0.01 min
 Lab File: BG018562.D
 Acq: 1 Sep 2015 14:23

Instrument :
 BNA_G
 ClientSampleId :
 C0AF0

Tot Ion:163 Resp: 271658
 Ion Ratio Lower Upper
 163 100
 194 4.5 2.9 4.3#
 164 9.9 7.7 11.5

