

Data Path : Z:\HPCHEM1\BNA G\DATA\BG090115\
 Data File : BG018563.D
 Acq On : 1 Sep 2015 15:01
 Operator : UM/IZ
 Sample : G3478-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF1

Quant Time: Sep 02 02:19:37 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 02 02:18:07 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	95244	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	416449	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	284301	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.38	188	738064	20.00	ng/ul	0.00
78) Chrysene-d12	21.64	240	801936	20.00	ng/ul	0.00
86) Perylene-d12	24.83	264	805402	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.44	96	8572	3.98	ng/uL	0.00
5) Phenol-d5	7.17	99	185654	21.48	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	114067	21.29	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	139087	21.01	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	153532	21.14	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	73091	22.52	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	82157	24.85	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	156637	22.32	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	213509	26.92	ng/ul	0.00
44) Dimethylphthalate-d6	14.04	166	590453	24.68	ng/ul	0.00
47) Acenaphthylene-d8	14.33	160	637298	21.16	ng/ul	0.00
52) 4-Nitrophenol-d4	14.82	143	106672	24.79	ng/ul	0.00
58) Fluorene-d10	15.62	176	450917	21.64	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	74113	20.41	ng/ul	-0.01
71) Anthracene-d10	17.47	188	764363	21.65	ng/ul	0.00
79) Pyrene-d10	19.76	212	807058	19.40	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.61	264	817781	19.13	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.08	163	284317	12.05	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG090115\
Data File : BG018563.D
Acq On : 1 Sep 2015 15:01
Operator : UM/IZ
Sample : G3478-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF1

Quant Time: Sep 02 02:19:37 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 02 02:18:07 2015
Response via : Initial Calibration

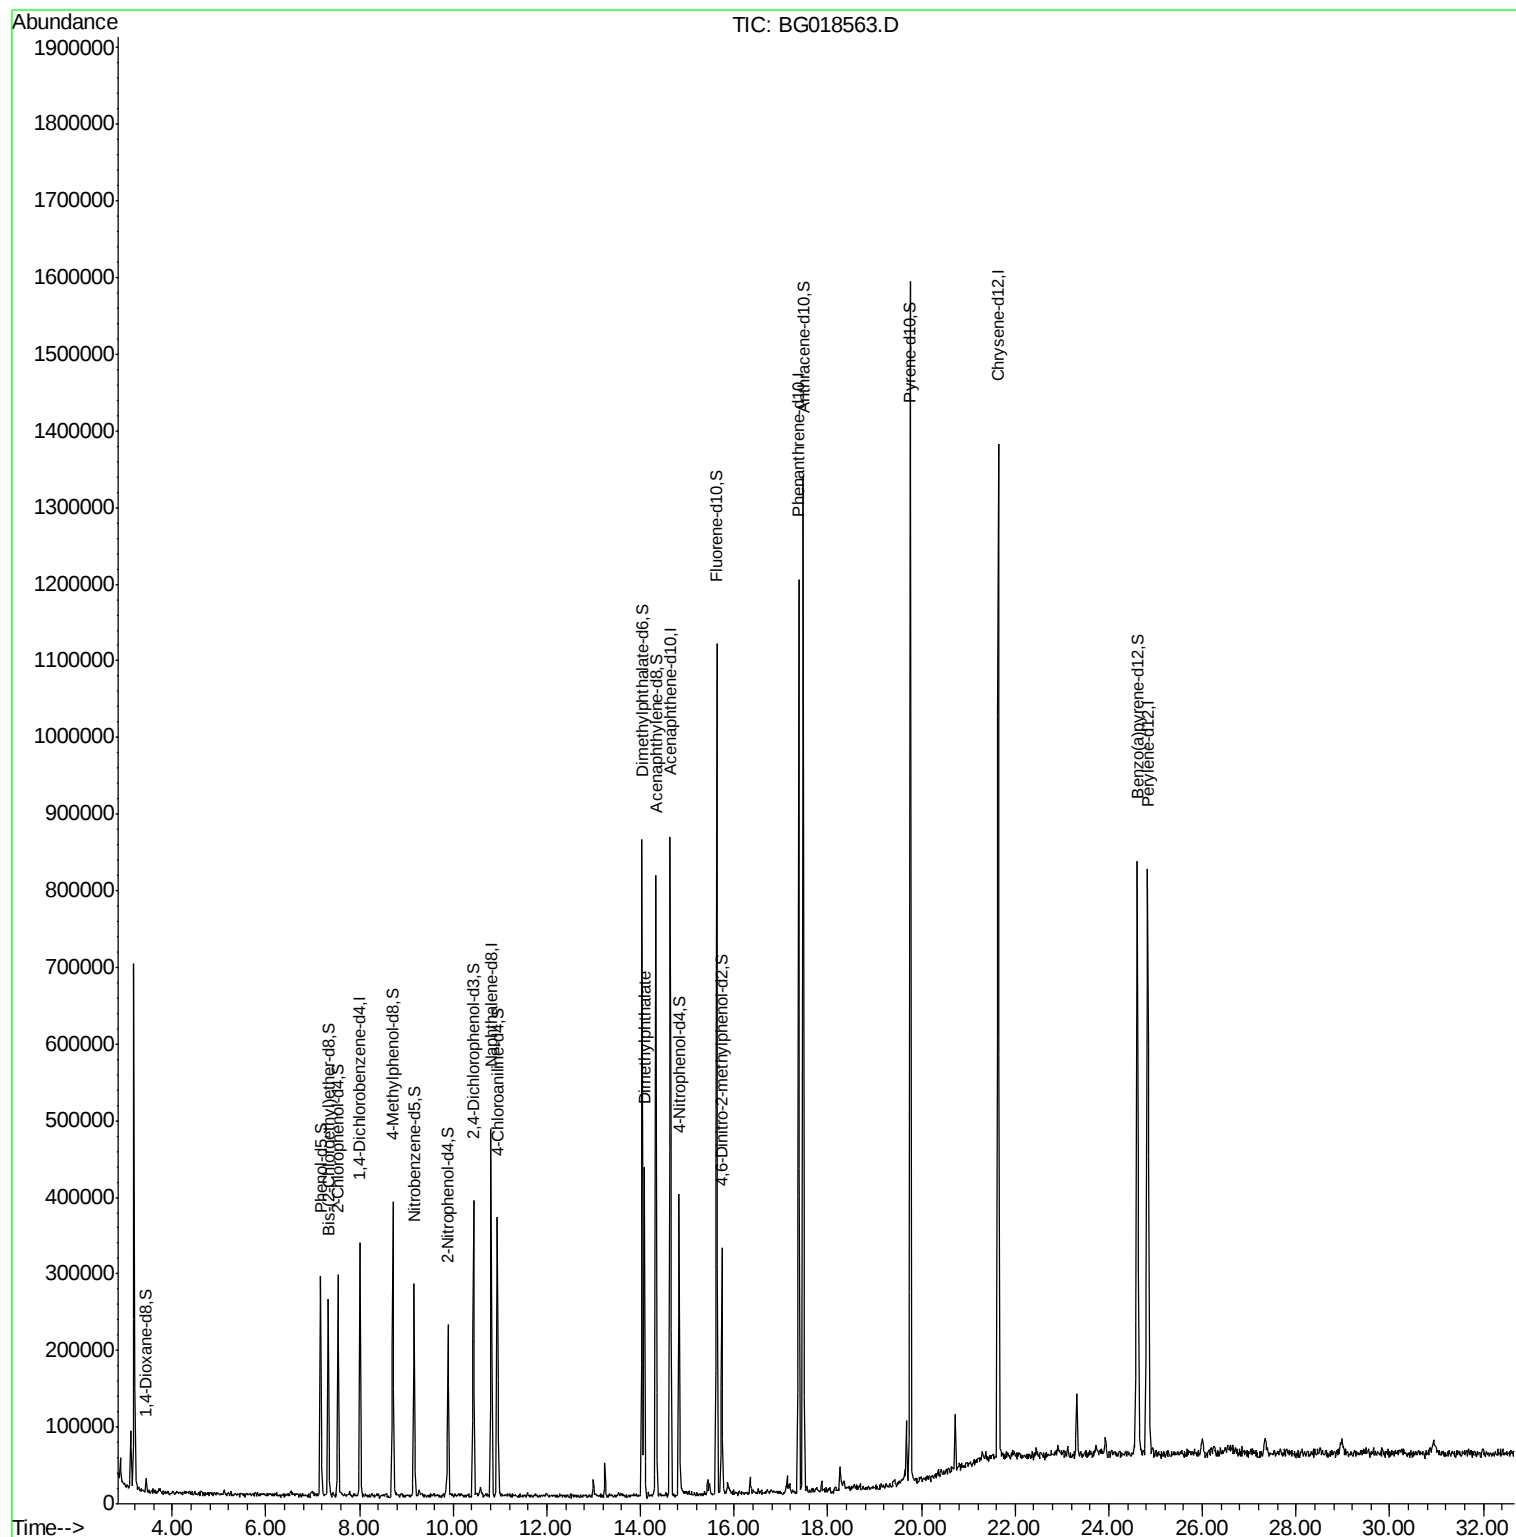


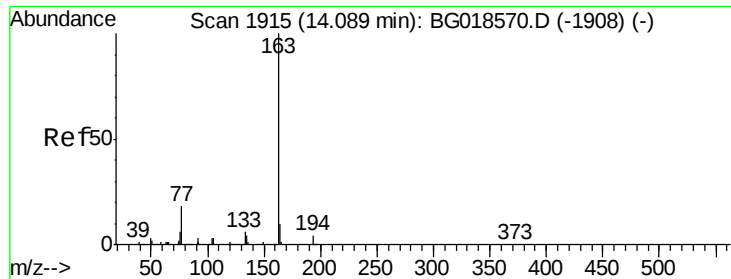

#45
 Dimethylphthalate
 Concen: 12.05 ng/ul
 RT: 14.08 min Scan# 1914
 Delta R.T. -0.01 min
 Lab File: BG018563.D
 Acq: 1 Sep 2015 15:01

Instrument :
 BNA_G
 ClientSampleId :
 C0AF1

Tot Ion:163 Resp: 284317
 Ion Ratio Lower Upper
 163 100
 194 4.0 2.9 4.3
 164 11.1 7.7 11.5

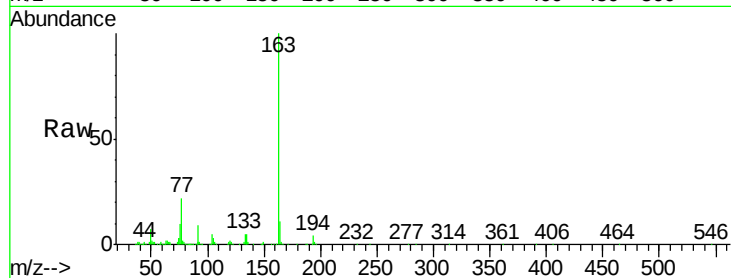

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

