

Data Path : Z:\HPCHEM1\BNA G\DATA\BG090115\
 Data File : BG018565.D
 Acq On : 1 Sep 2015 16:17
 Operator : UM/IZ
 Sample : G3478-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF3

Quant Time: Sep 02 02:19:53 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 02 02:18:07 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	95155	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	415273	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	282280	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.37	188	761491	20.00	ng/ul	0.00
78) Chrysene-d12	21.64	240	798480	20.00	ng/ul	0.00
86) Perylene-d12	24.83	264	791423	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.45	96	7700	3.58	ng/uL	0.00
5) Phenol-d5	7.17	99	161258	18.67	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	98872	18.47	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	124999	18.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	124596	17.17	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	64700	19.99	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	69848	21.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	133075	19.02	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	187381	23.70	ng/ul	0.00
44) Dimethylphthalate-d6	14.04	166	516139	21.73	ng/ul	0.00
47) Acenaphthylene-d8	14.32	160	534773	17.88	ng/ul	0.00
52) 4-Nitrophenol-d4	14.82	143	89700	21.00	ng/ul	0.00
58) Fluorene-d10	15.62	176	376481	18.20	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.74	200	64834	17.31	ng/ul	0.00
71) Anthracene-d10	17.47	188	635725	17.46	ng/ul	0.00
79) Pyrene-d10	19.76	212	639896	15.45	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.61	264	601847	14.32	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.08	163	242023	10.33	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG090115\
Data File : BG018565.D
Acq On : 1 Sep 2015 16:17
Operator : UM/IZ
Sample : G3478-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF3

Quant Time: Sep 02 02:19:53 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 02 02:18:07 2015
Response via : Initial Calibration

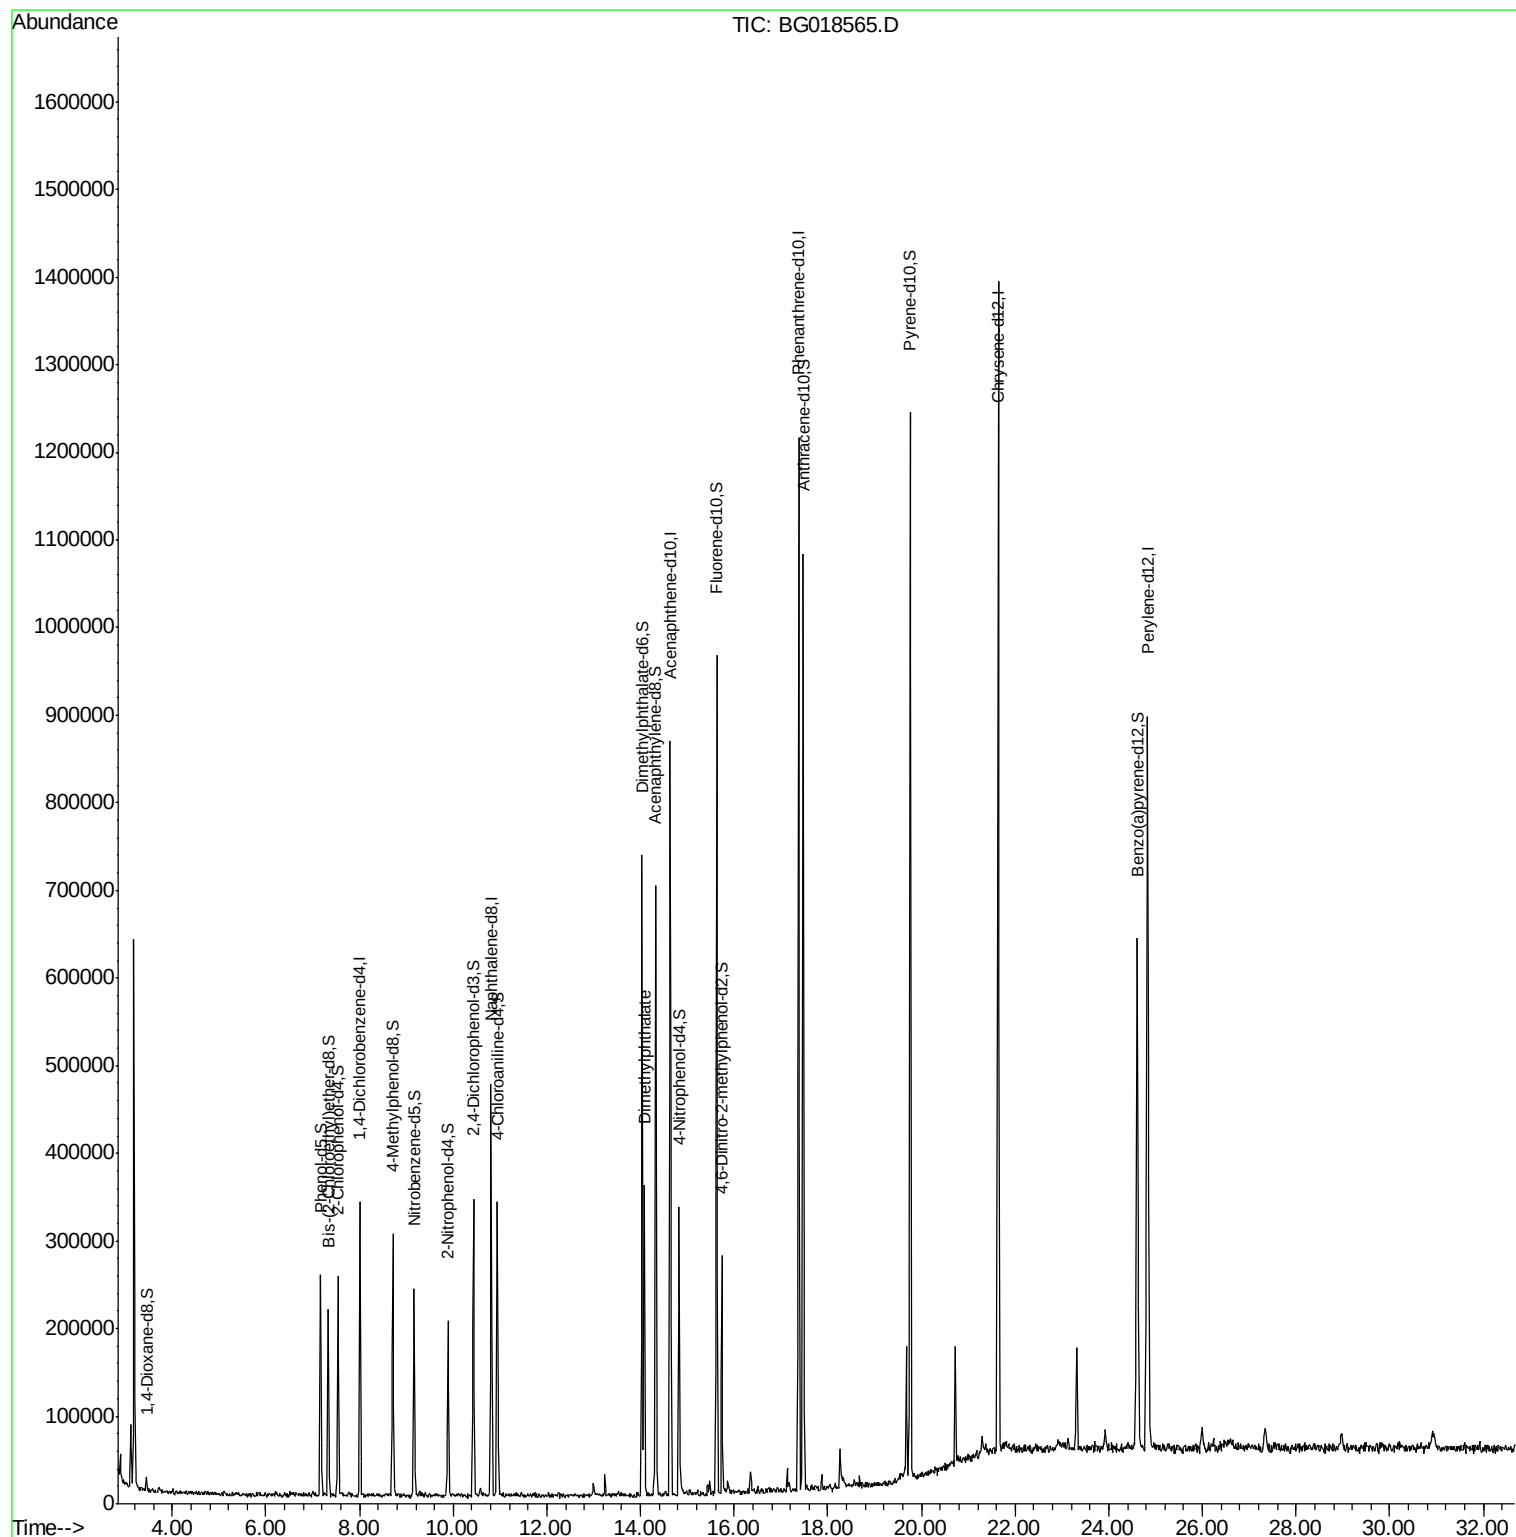

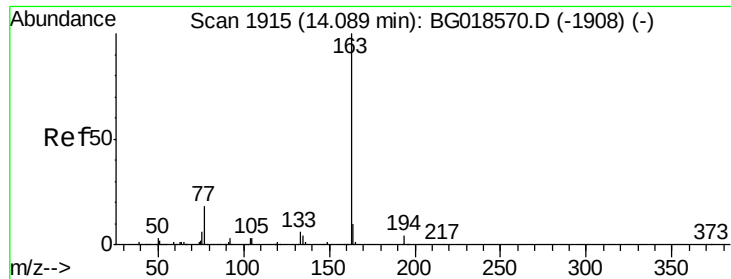

#45
 Dimethylphthalate
 Concen: 10.33 ng/ul
 RT: 14.08 min Scan# 1914
 Delta R.T. -0.01 min
 Lab File: BG018565.D
 Acq: 1 Sep 2015 16:17

Instrument :
 BNA_G
 ClientSampleId :
 C0AF3

Tot Ion	Ratio	Lower	Upper
163	100		
194	3.8	2.9	4.3
164	10.2	7.7	11.5

