
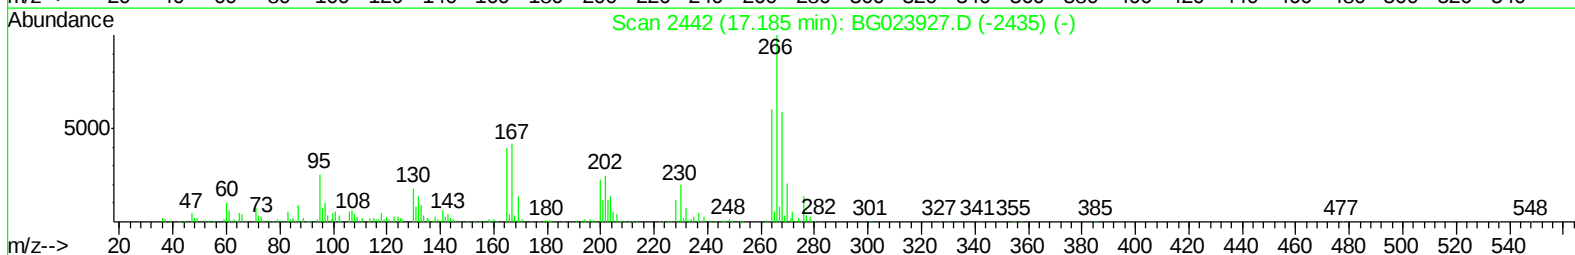
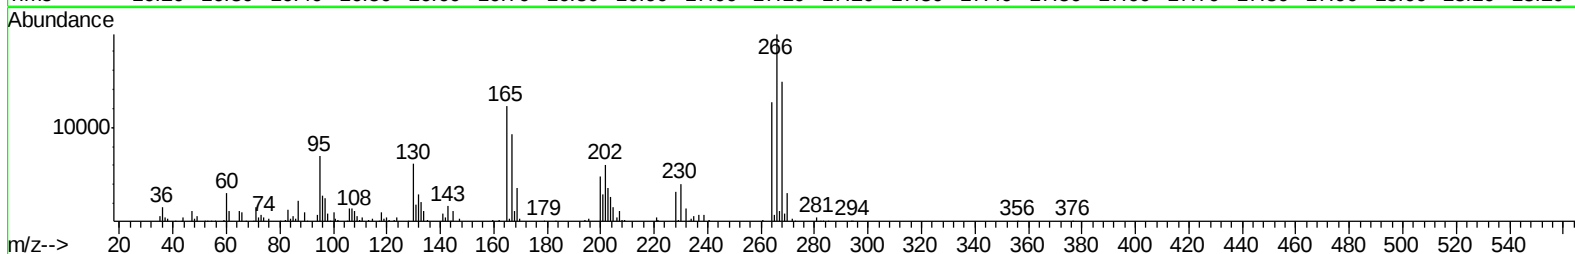


Data Path : Z:\HPCHEM1\BNA_G\Data\BG090116\
Data File : BG023936.D
Acq On : 1 Sep 2016 17:20
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 05:52:46 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 20:05:47 2016
Response via : Initial Calibration

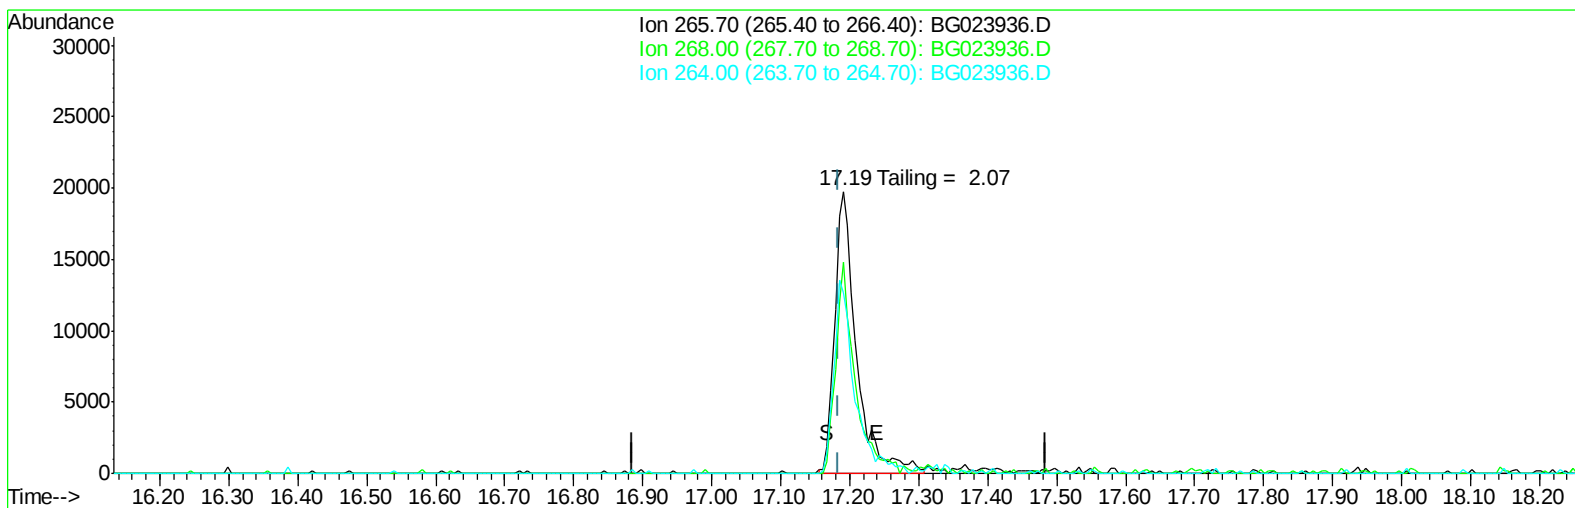

TIC: BG023936.D

(69) Pentachlorophenol (C)




17.191min (+0.006) 0.00ng

response 41485

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	74.93
264.00	63.20	64.19
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG090116\
Data File : BG023936.D
Acq On : 1 Sep 2016 17:20
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 05:52:46 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 20:05:47 2016
Response via : Initial Calibration

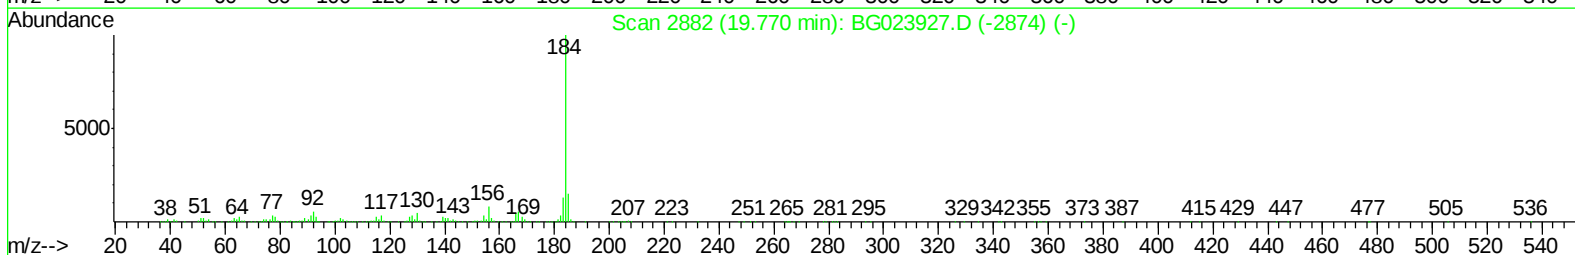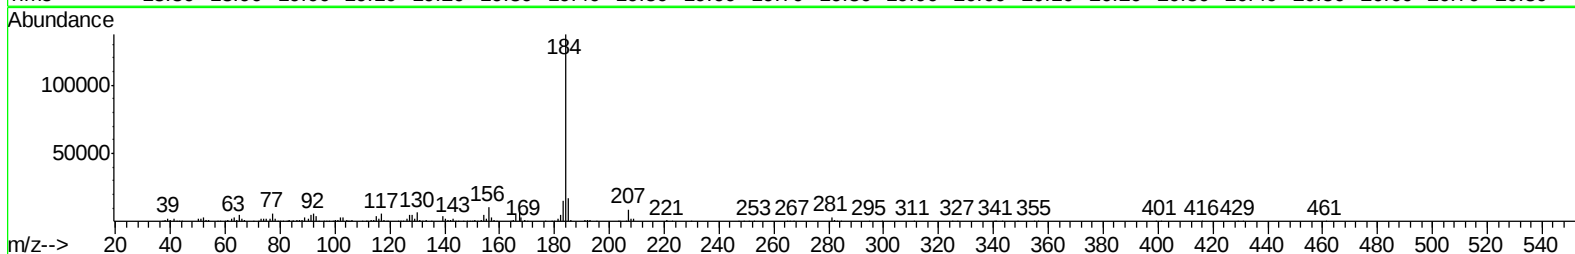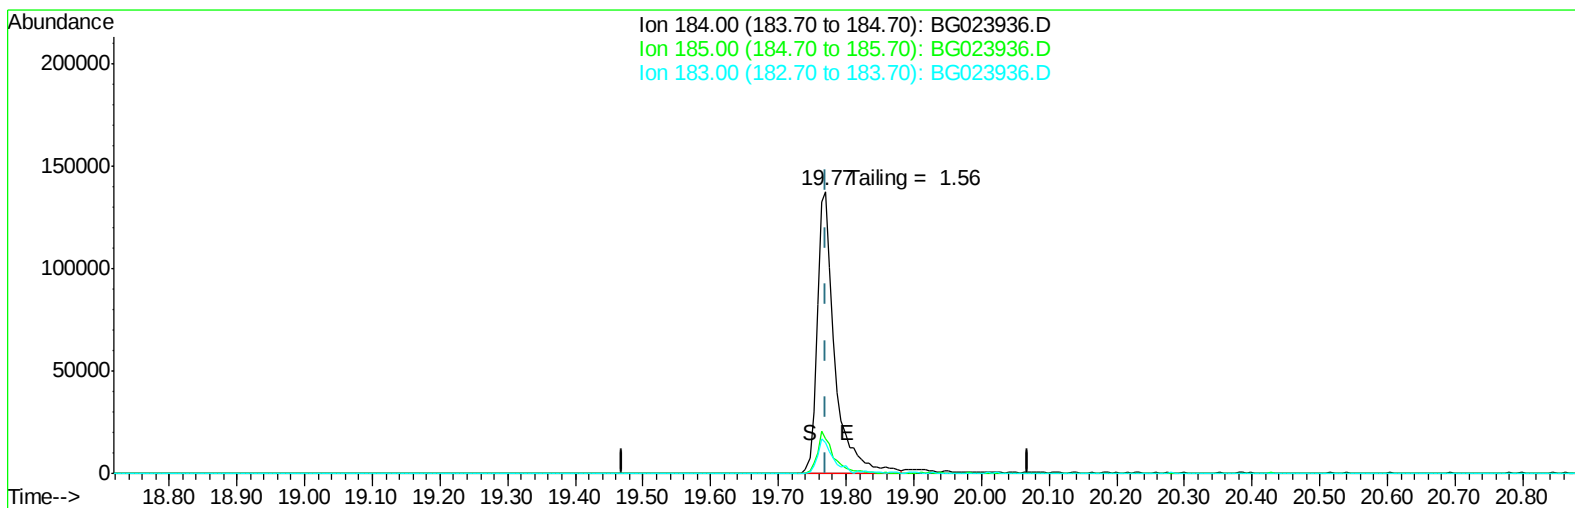

TIC: BG023936.D

(76) Benzidine

19.770min (-0.000) 8684.03ng

response 251160

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	12.14#
183.00	13.40	11.00
0.00	0.00	0.00