


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG090116\
 Data File : BG023936.D
 Acq On : 1 Sep 2016 17:20
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG083116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 31 20:05:47 2016

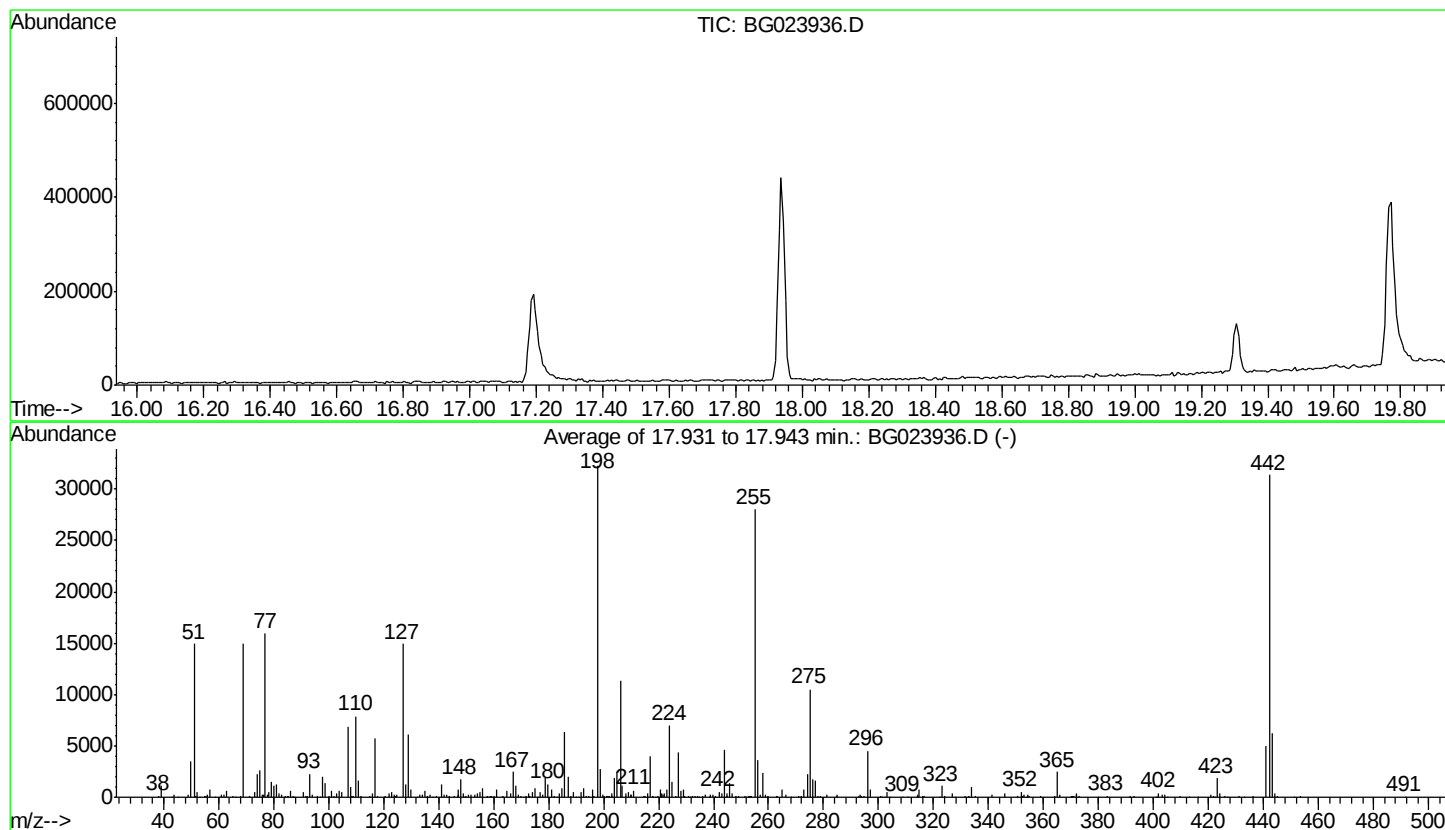

AutoFind: Scans 2569, 2570, 2571; Background Corrected with Scan 2563

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.2	14910	PASS
68	69	0.00	2	0.5	79	PASS
69	198	0.00	100	46.4	14982	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.2	14927	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	32277	PASS
199	198	5	9	8.3	2694	PASS
275	198	10	60	32.5	10490	PASS
365	198	1	100	7.7	2483	PASS
441	442	0.01	24	16.0	5034	PASS
442	198	50	100	97.2	31376	PASS
443	442	15	24	20.0	6272	PASS