
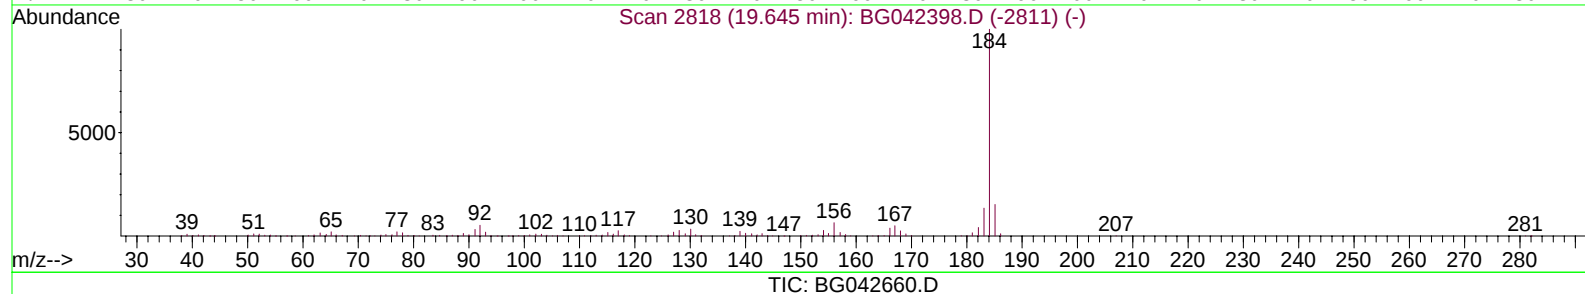
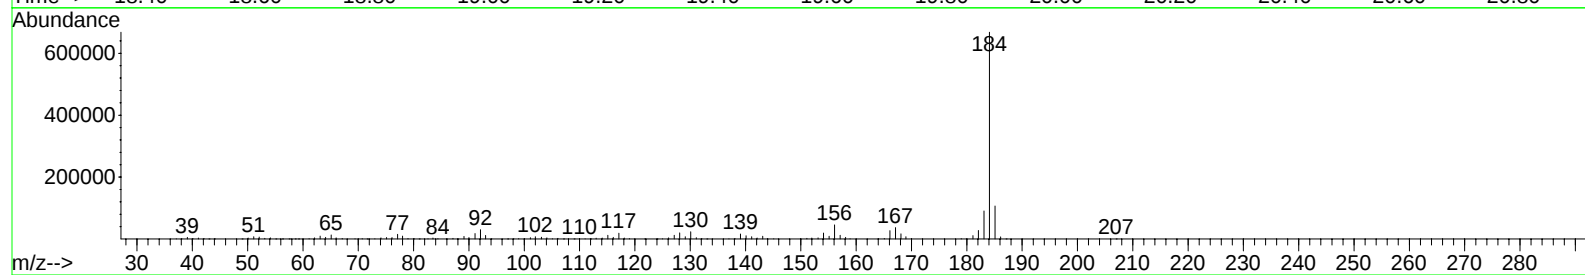


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090119\
Data File : BG042660.D
Acq On : 1 Sep 2019 11:09
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 12:13:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 14:29:15 2019
Response via : Initial Calibration

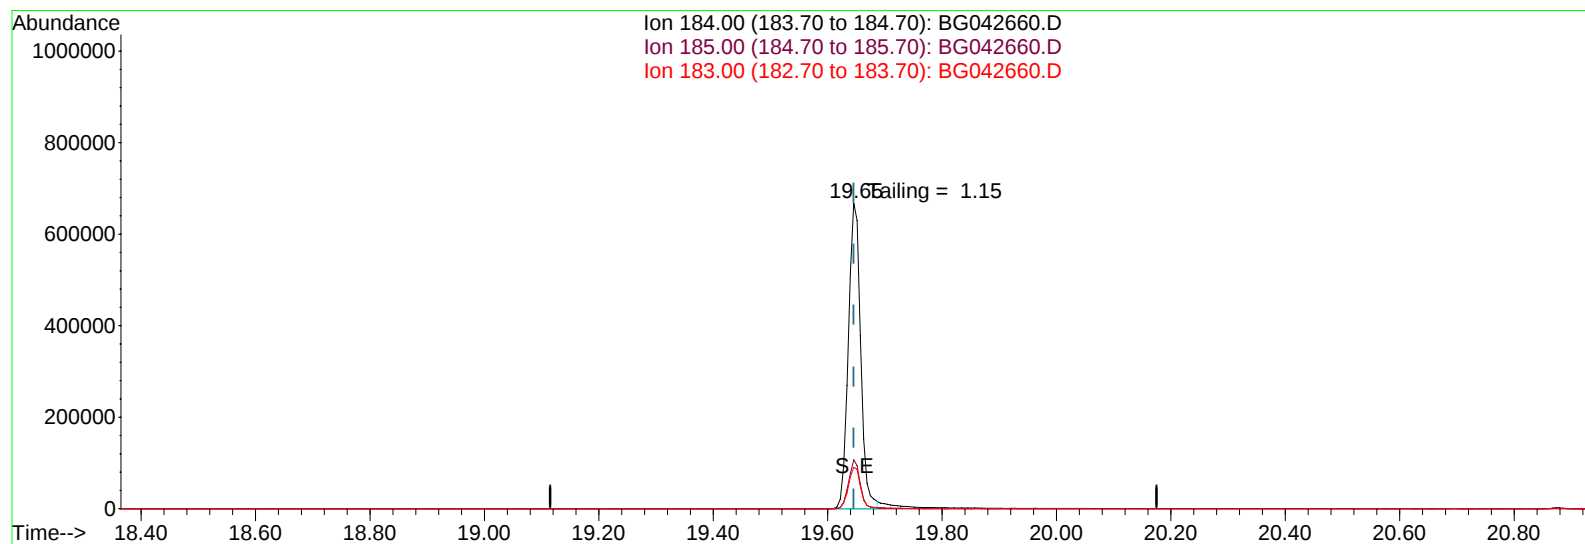

(77) Benzidine




19.645min (+0.000) 17333.53ng

response 1044609

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	15.99
183.00	13.50	13.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090119\
Data File : BG042660.D
Acq On : 1 Sep 2019 11:09
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 12:13:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 14:29:15 2019
Response via : Initial Calibration

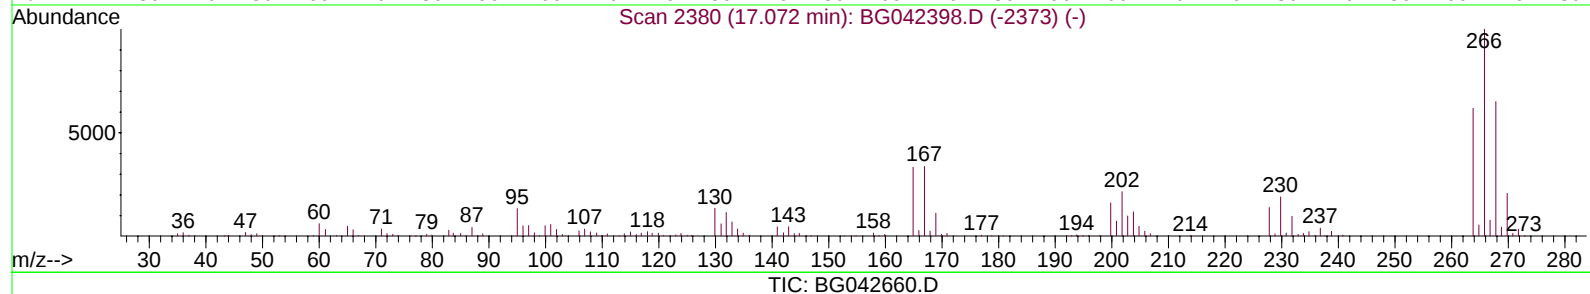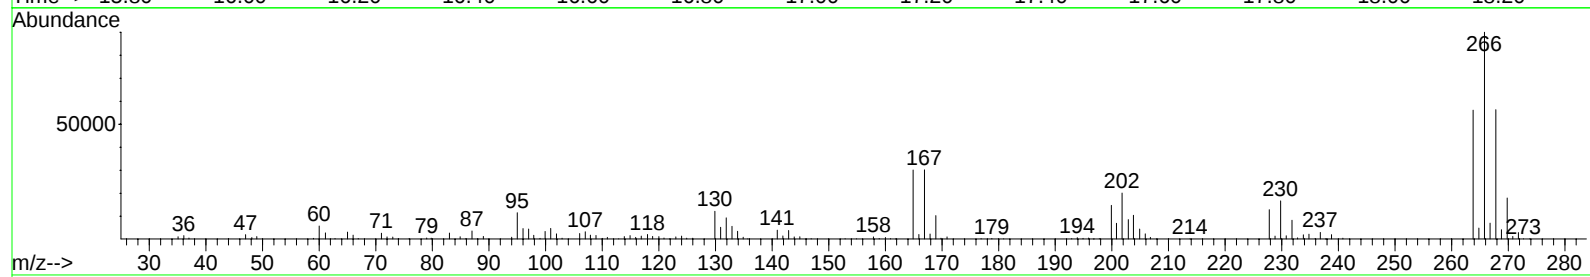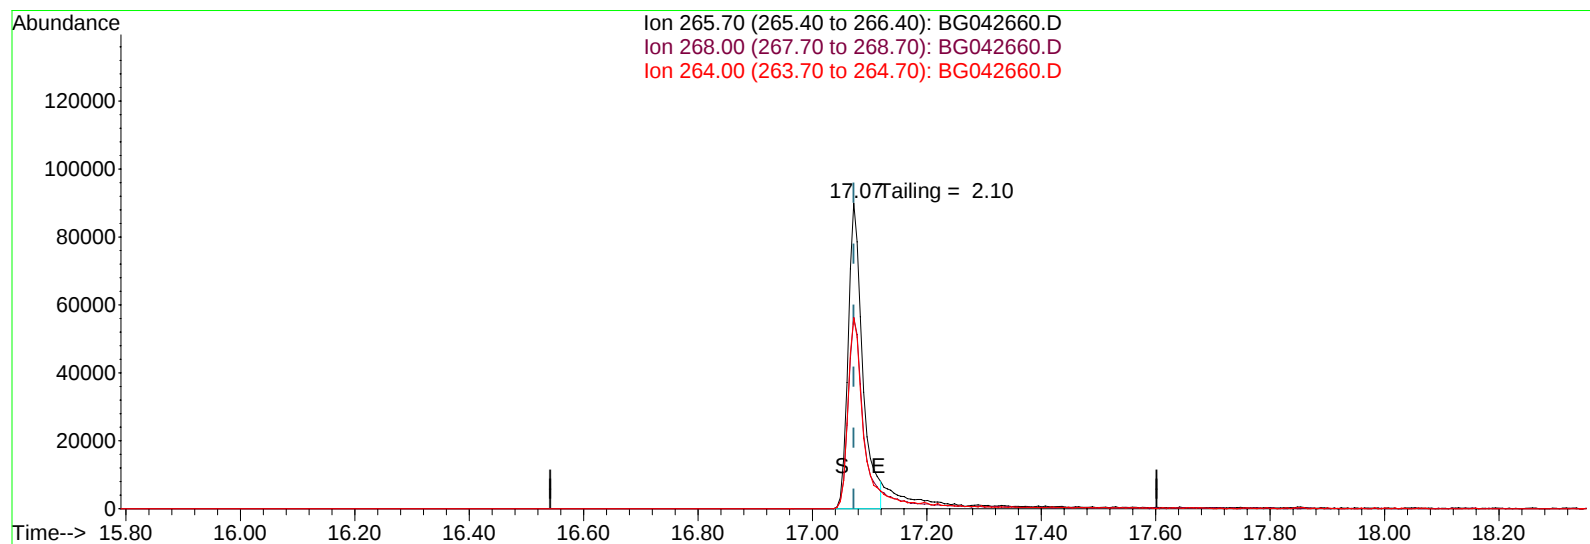

(70) Pentachlorophenol (C)

17.072min (+0.000) 17160.60ng

response 183067

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	62.61
264.00	61.80	62.36
0.00	0.00	0.00