
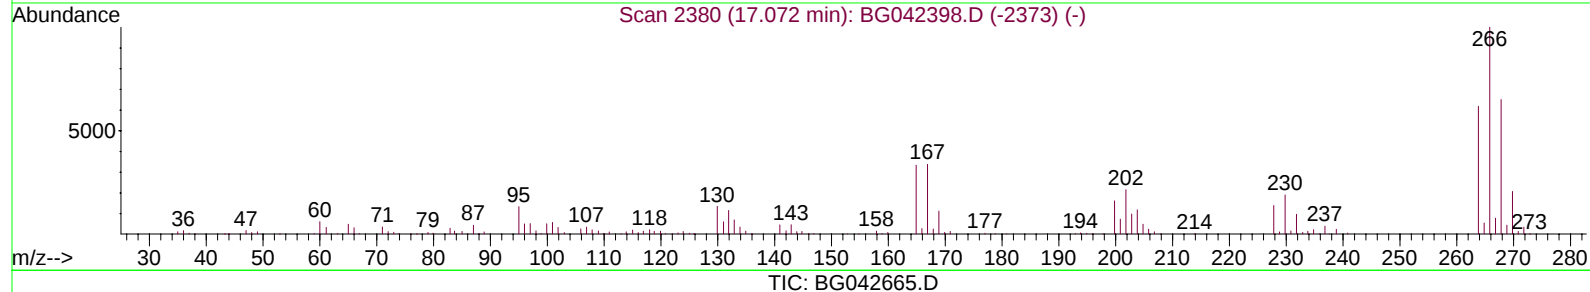
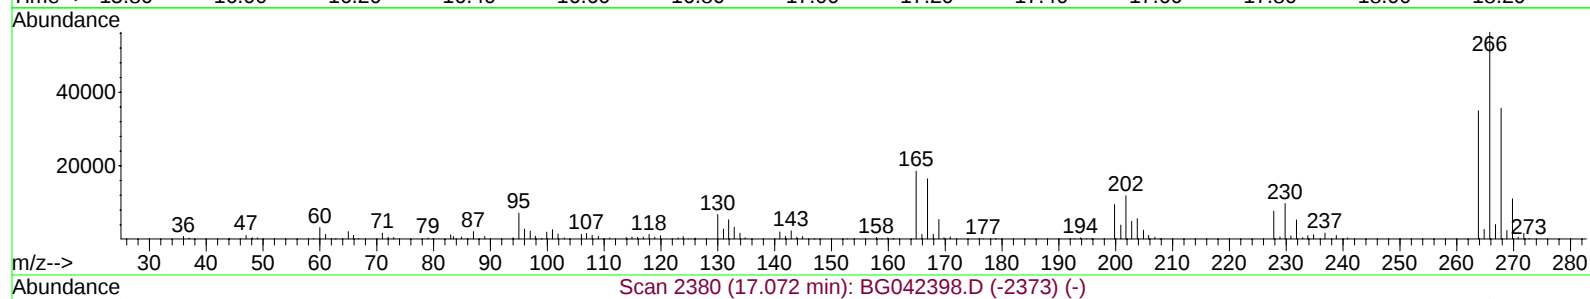


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090119\
Data File : BG042665.D
Acq On : 1 Sep 2019 16:03
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 12:16:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 14:29:15 2019
Response via : Initial Calibration

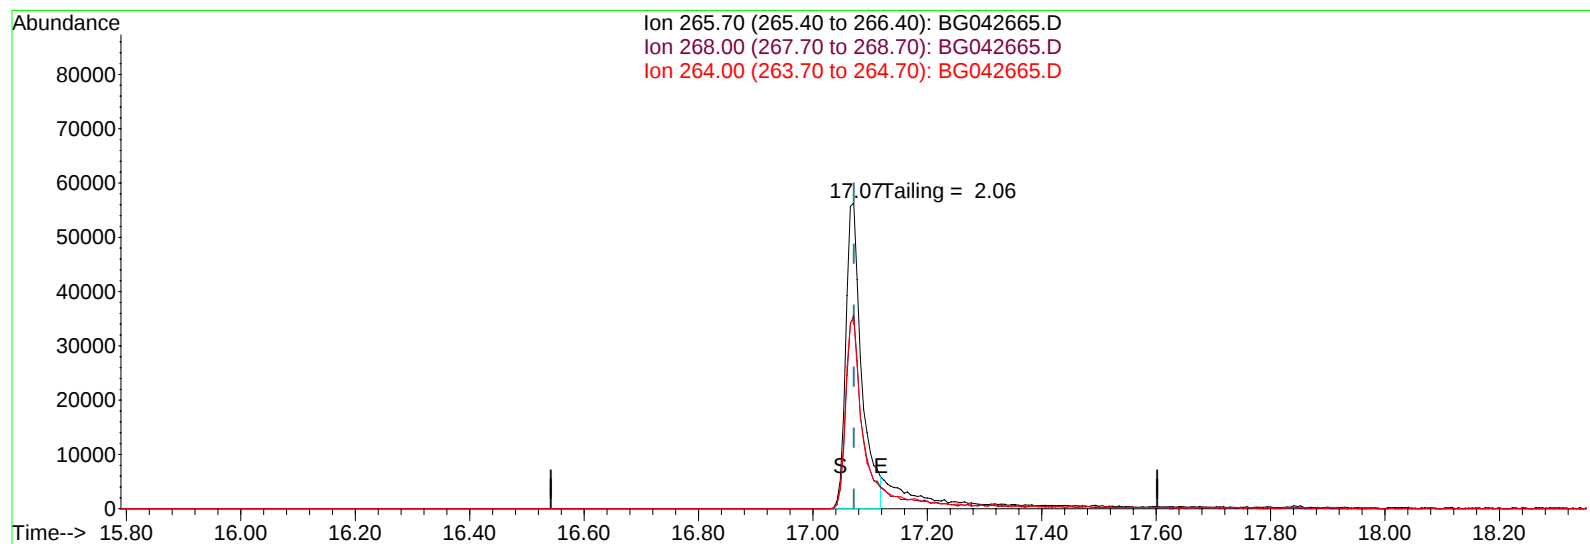

(70) Pentachlorophenol (C)




17.071min (-0.001) 82747.27ng

response 128646

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	63.34
264.00	61.80	62.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG090119\
 Data File : BG042665.D
 Acq On : 1 Sep 2019 16:03
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 12:16:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 22 14:29:15 2019
 Response via : Initial Calibration

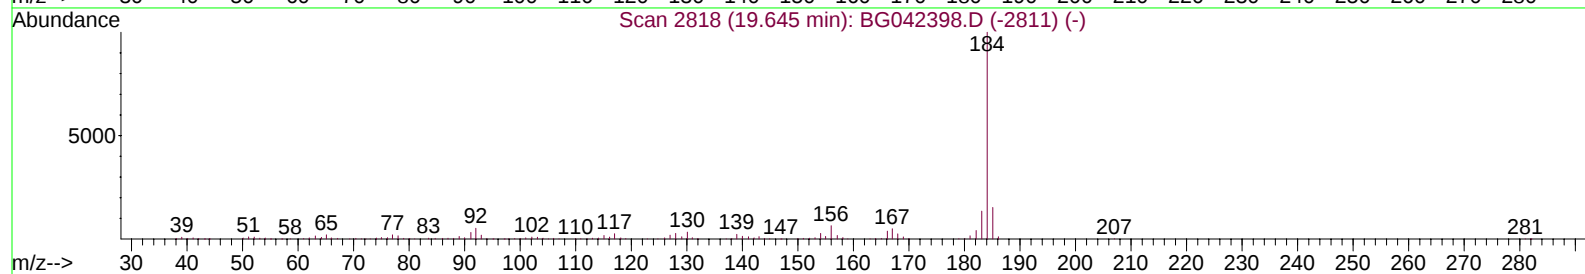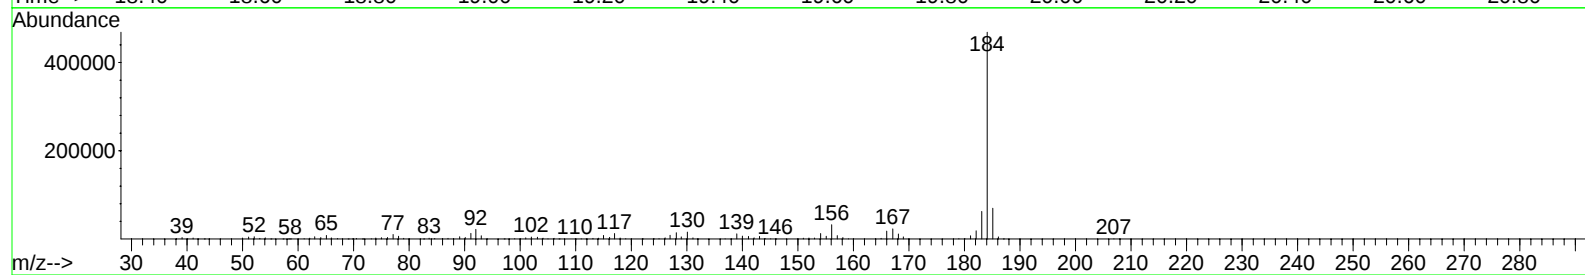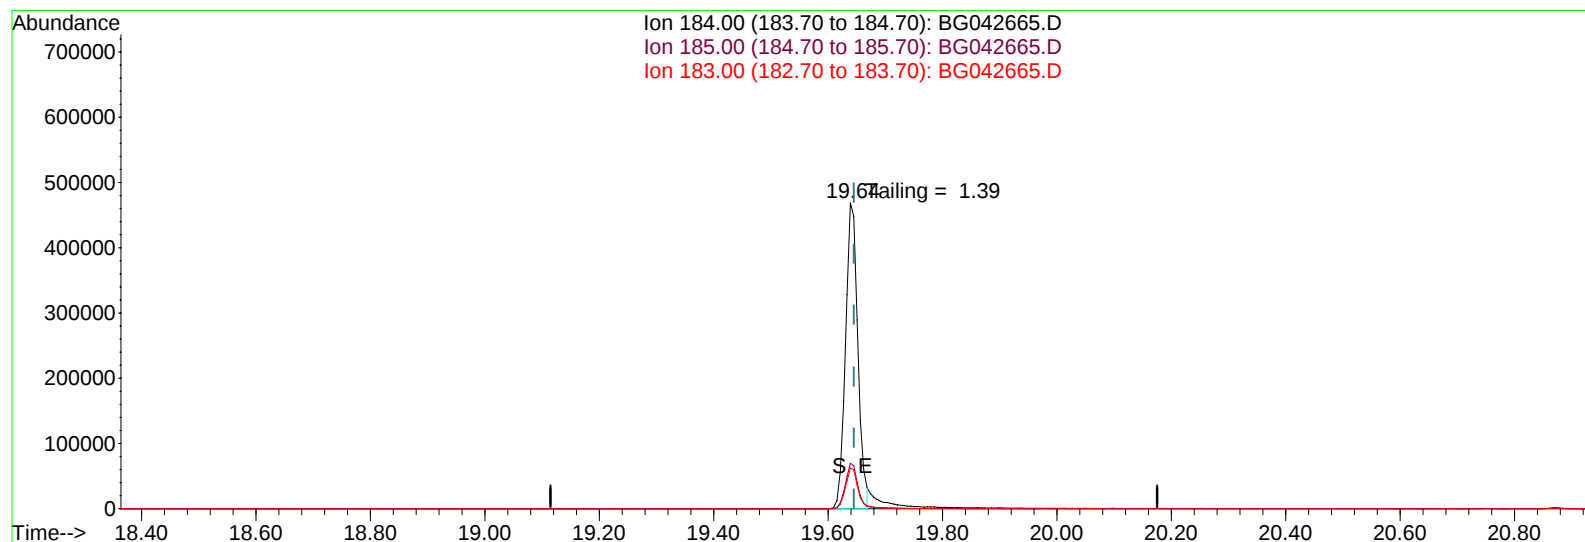

TIC: BG042665.D

(77) Benzidine

19.639min (-0.006) 49941.90ng

response 753156

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.88
183.00	13.50	13.32
0.00	0.00	0.00