

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090119\
 Data File : BG042672.D
 Acq On : 1 Sep 2019 21:49
 Operator : HP/JU
 Sample : K4554-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-15-(13-15)

Quant Time: Sep 02 08:15:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 22 14:29:15 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.99	152	29834	20.00	ng	-0.01
21) Naphthalene-d8	10.82	136	113207	20.00	ng	0.00
39) Acenaphthene-d10	14.66	164	88511	20.00	ng	0.00
64) Phenanthrene-d10	17.41	188	223252	20.00	ng	-0.01
76) Chrysene-d12	21.68	240	254244	20.00	ng	-0.01
87) Perylene-d12	24.93	264	297937	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.55	112	175601	119.21	ng	0.00
7) Phenol-d6	7.16	99	235284	118.25	ng	-0.01
23) Nitrobenzene-d5	9.16	82	136030	83.04	ng	-0.01
42) 2,4,6-Tribromophenol	16.15	330	173881	138.22	ng	-0.01
45) 2-Fluorobiphenyl	13.28	172	486276	92.92	ng	0.00
79) Terphenyl-d14	20.02	244	1038527	88.31	ng	0.00
Target Compounds						
10) Phenol	7.19	94	21711	10.732	ng	92
50) Dimethylphthalate	14.11	163	43428	6.800	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090119\
Data File : BG042672.D
Acq On : 1 Sep 2019 21:49
Operator : HP/JU
Sample : K4554-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-15-(13-15)

Quant Time: Sep 02 08:15:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 14:29:15 2019
Response via : Initial Calibration

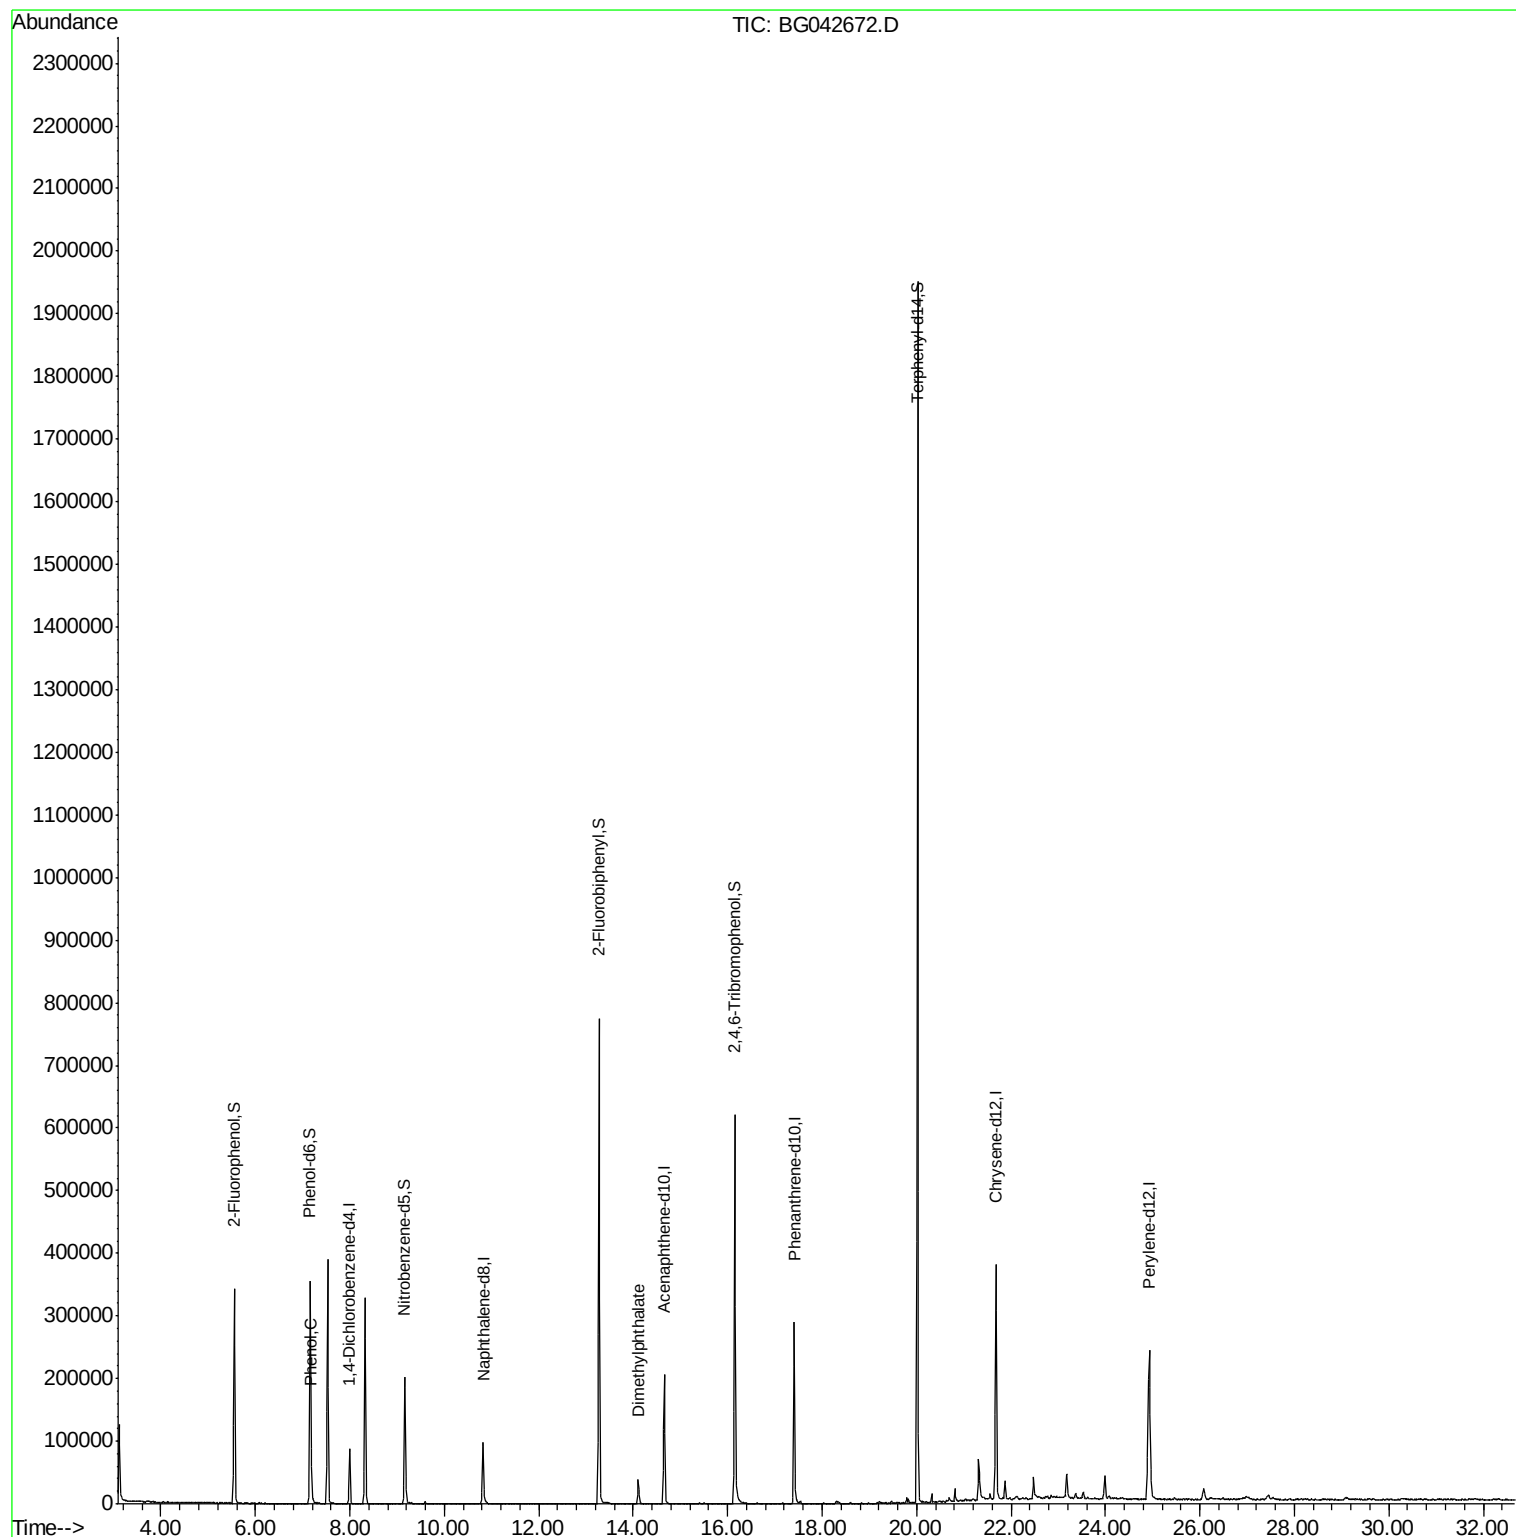

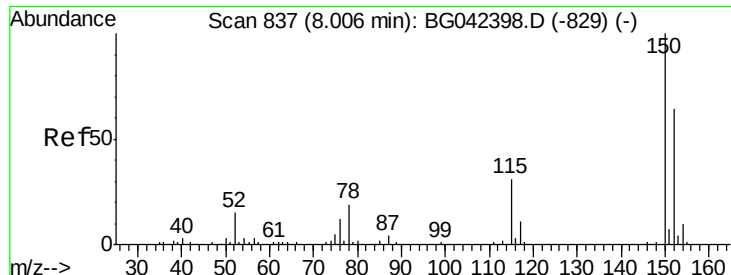


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.99 min Scan# 835
Delta R.T. -0.01 min
Lab File: BG042672.D
Acq: 1 Sep 2019 21:49

Instrument :
BNA_G
ClientSampleId :
SB-15-(13-15)

Tot Ion:152 Resp: 29834
Ion Ratio Lower Upper
152 100
150 155.7 125.4 188.0
115 53.5 38.5 57.7

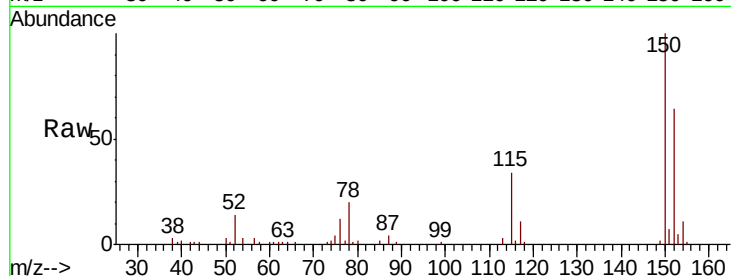


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

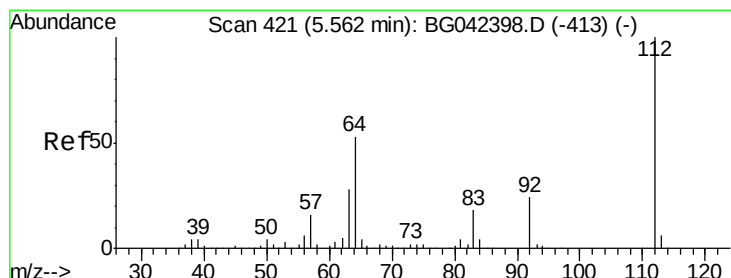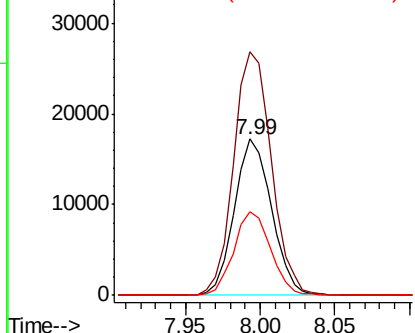



#5


2-Fluorophenol
Concen: 119.207 ng
RT: 5.55 min Scan# 420
Delta R.T. -0.01 min
Lab File: BG042672.D
Acq: 1 Sep 2019 21:49

Tgt Ion:112 Resp: 175601
Ion Ratio Lower Upper
112 100
64 52.8 42.8 64.2
63 28.1 22.7 34.1

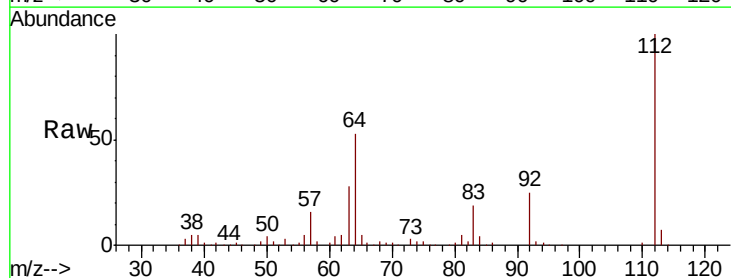

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

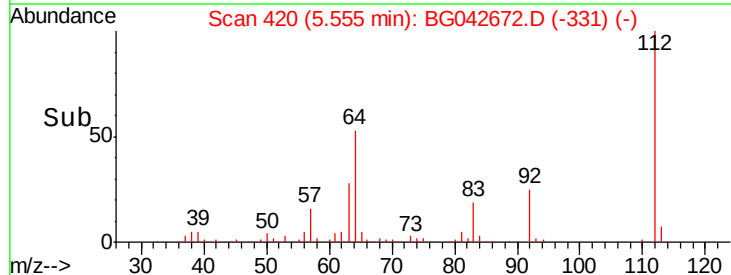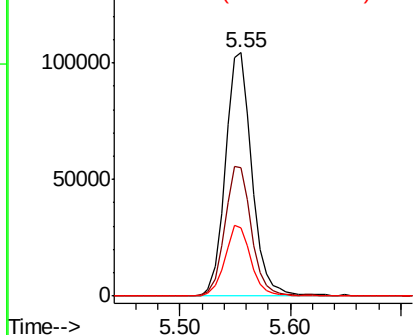

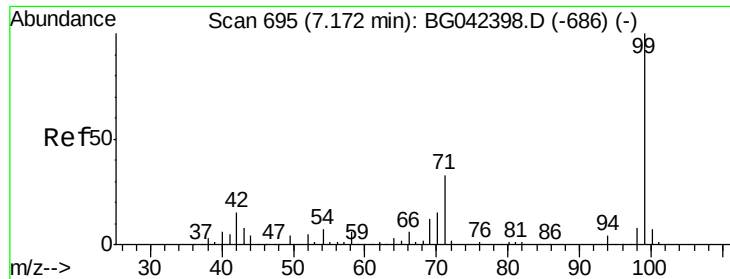

#7

Phenol-d6

Concen: 118.246 ng

RT: 7.16 min Scan# 693

Delta R.T. -0.01 min

Lab File: BG042672.D

Acq: 1 Sep 2019 21:49

Instrument :

BNA_G

ClientSampleId :

SB-15-(13-15)


Tot Ion: 99 Resp: 235284

Ion Ratio Lower Upper




99 100

42 15.4 12.0 18.0

71 37.2 26.3 39.5

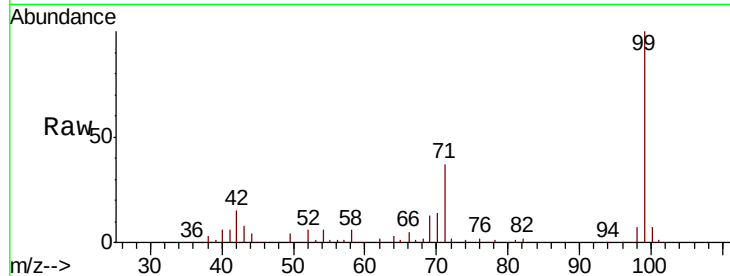

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

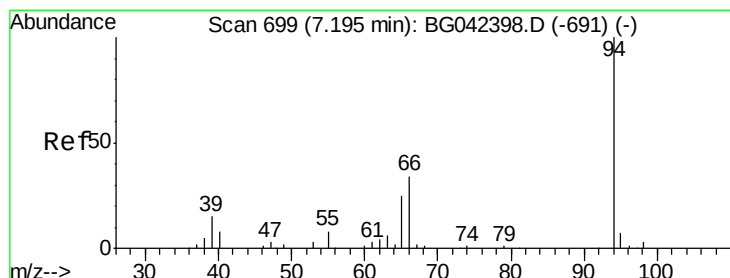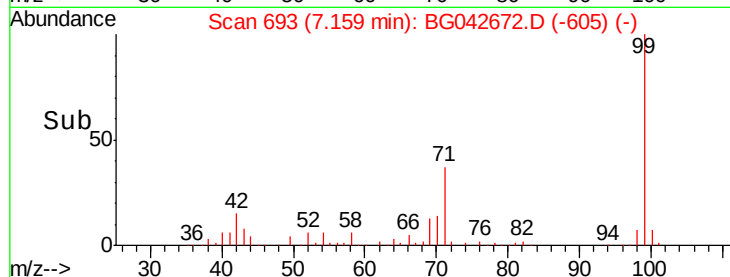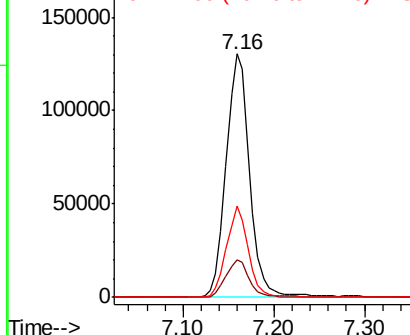

#10

Phenol

Concen: 10.732 ng

RT: 7.19 min Scan# 698

Delta R.T. -0.01 min

Lab File: BG042672.D

Acq: 1 Sep 2019 21:49


Tgt Ion: 94 Resp: 21711

Ion Ratio Lower Upper



94 100


65 29.8 5.6 45.6

66 40.5 16.0 56.0

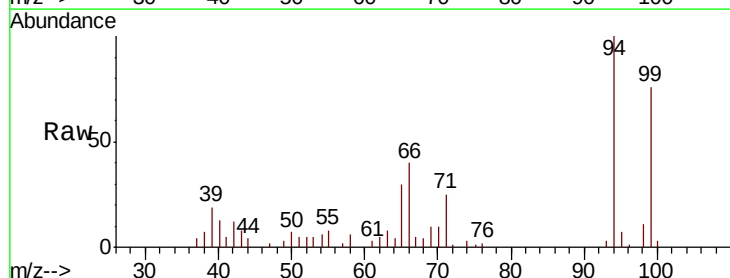

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

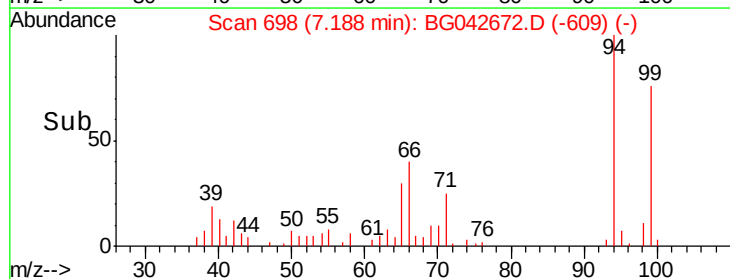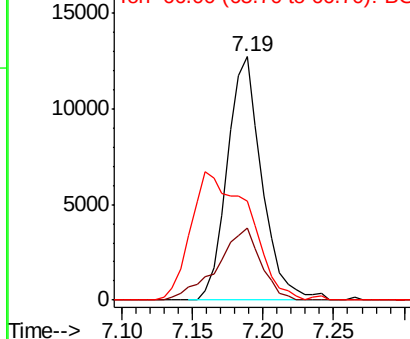



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.82 min Scan# 1316

Delta R.T. -0.01 min

Lab File: BG042672.D

Acq: 1 Sep 2019 21:49

Instrument :

BNA_G

ClientSampleId :

SB-15-(13-15)

Tot Ion:136 Resp: 113207



Ion Ratio Lower Upper

136 100

137 11.8 8.7 13.1

54 6.0 4.9 7.3

68 3.0 3.6 5.4#


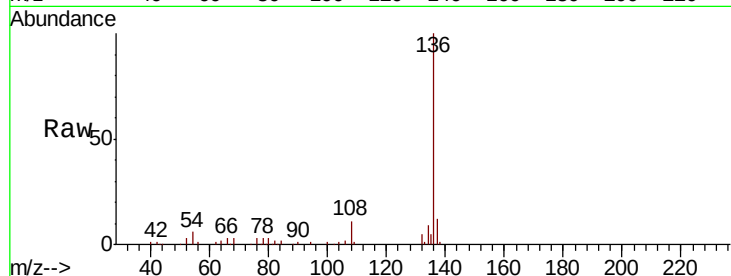


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC

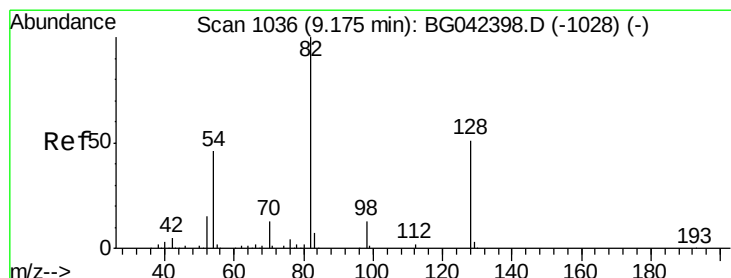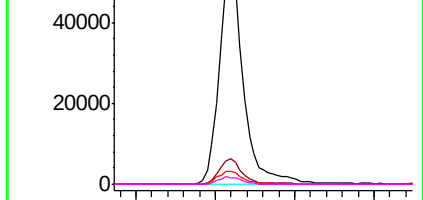

#23

Nitrobenzene-d5

Concen: 83.036 ng

RT: 9.16 min Scan# 1034

Delta R.T. -0.01 min

Lab File: BG042672.D

Acq: 1 Sep 2019 21:49



Tgt Ion: 82 Resp: 136030

Ion Ratio Lower Upper

82 100

128 52.2 40.7 61.1


54 48.2 36.3 54.5

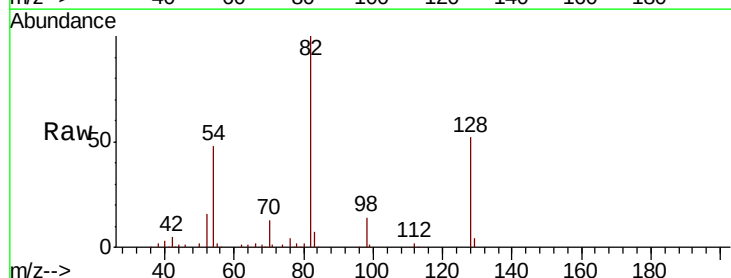


Abundance Ion 82.00 (81.70 to 82.70): BGC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BGC

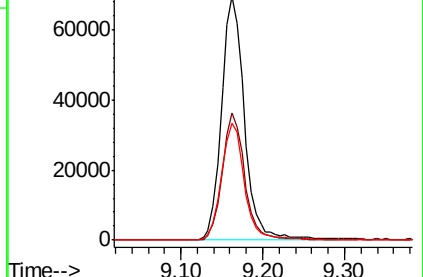

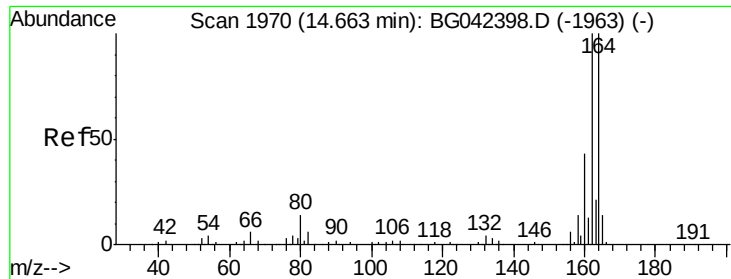

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.66 min Scan# 1969

Delta R.T. -0.01 min

Lab File: BG042672.D

Acq: 1 Sep 2019 21:49

Instrument :


BNA_G

ClientSampleId :

SB-15-(13-15)

Tot Ion:164 Resp: 88511

Ion	Ratio	Lower	Upper
164	100		
162	100.0	79.9	119.9
160	43.6	34.3	51.5



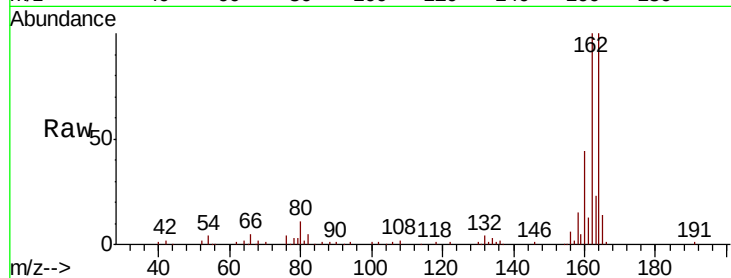


Abundance

Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

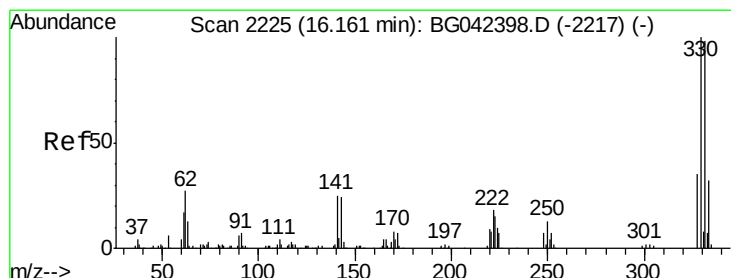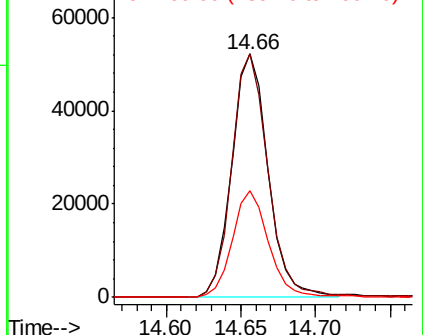

#42

2,4,6-Tribromophenol

Concen: 138.216 ng

RT: 16.15 min Scan# 2223


Delta R.T. -0.01 min

Lab File: BG042672.D

Acq: 1 Sep 2019 21:49

Tgt Ion:330 Resp: 173881

Ion	Ratio	Lower	Upper
330	100		
332	94.5	77.4	116.0
141	25.8	21.4	32.0


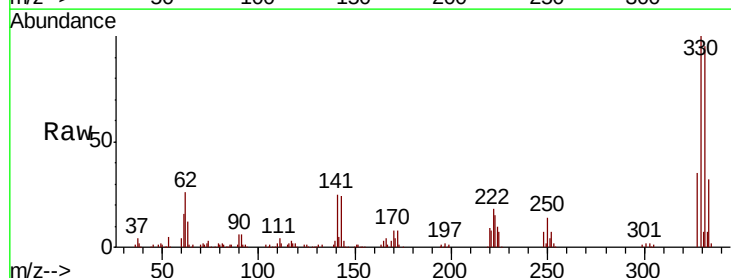



Abundance

Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E




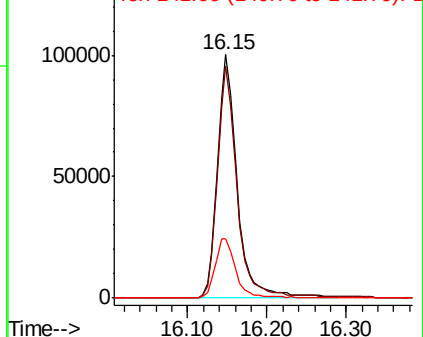




#45
2-Fluorobiphenyl
Concen: 92.919 ng
RT: 13.28 min Scan# 1734
Delta R.T. -0.01 min
Lab File: BG042672.D
Acq: 1 Sep 2019 21:49




Instrument :
BNA_G
ClientSampleId :
SB-15-(13-15)


Tot Ion:172 Resp: 486276
Ion Ratio Lower Upper
172 100
171 36.9 30.5 45.7
170 24.3 20.2 30.2

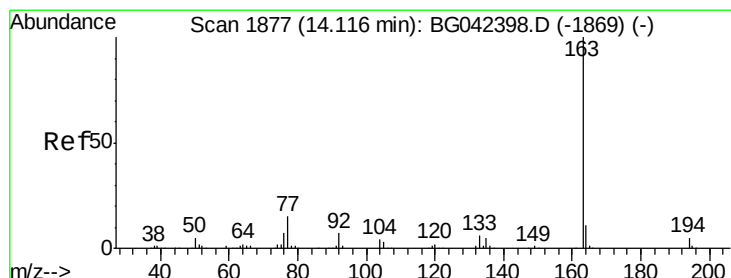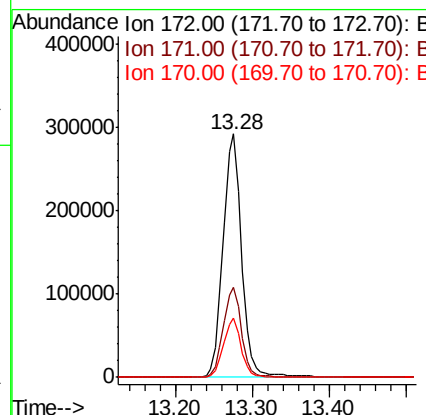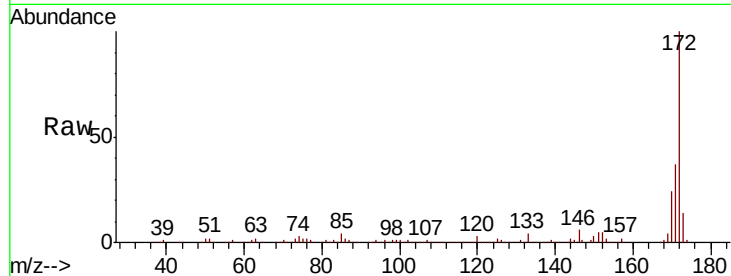

#50
Dimethylphthalate
Concen: 6.800 ng
RT: 14.11 min Scan# 1876
Delta R.T. -0.01 min
Lab File: BG042672.D
Acq: 1 Sep 2019 21:49

Tgt Ion:163 Resp: 43428
Ion Ratio Lower Upper
163 100
194 4.8 4.2 6.2
164 10.4 8.8 13.2



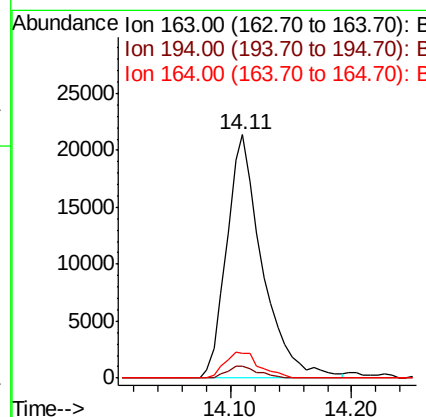
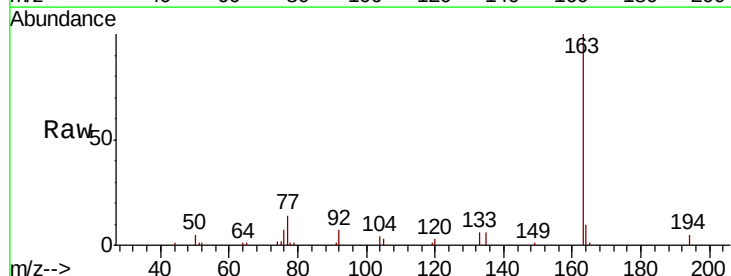


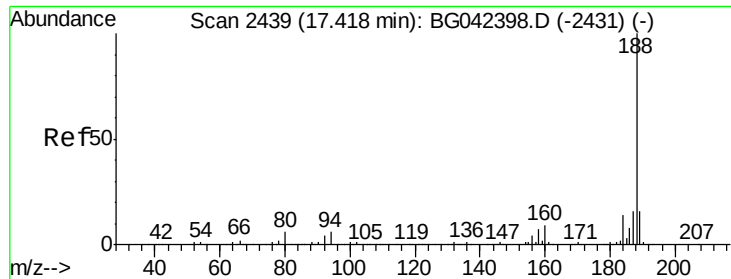

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.41 min Scan# 2437
Delta R.T. -0.01 min
Lab File: BG042672.D
Acq: 1 Sep 2019 21:49




Instrument :
BNA_G
ClientSampleId :
SB-15-(13-15)


Tot Ion:188 Resp: 223252
Ion Ratio Lower Upper
188 100
94 5.1 4.5 6.7
80 5.0 4.9 7.3

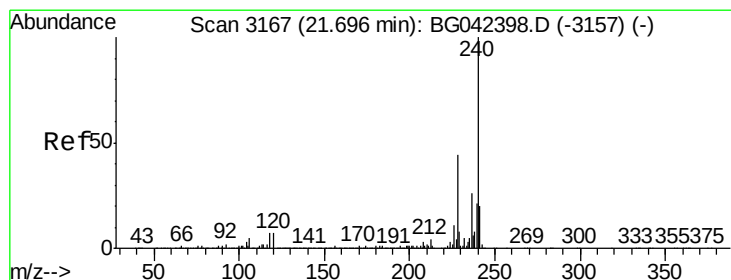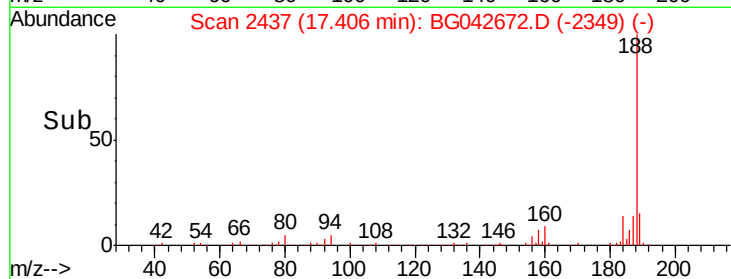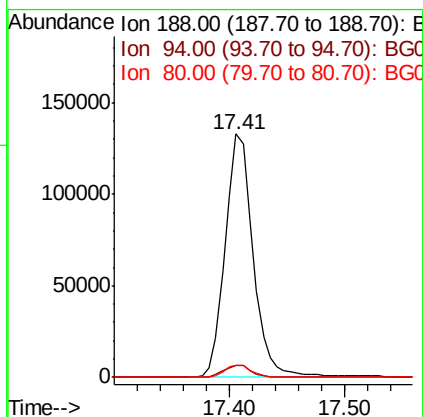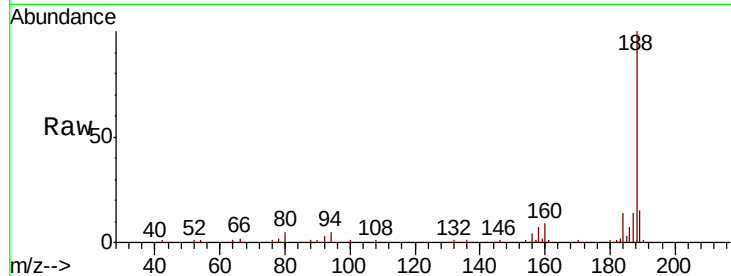

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.68 min Scan# 3165
Delta R.T. -0.01 min
Lab File: BG042672.D
Acq: 1 Sep 2019 21:49

Tgt Ion:240 Resp: 254244
Ion Ratio Lower Upper
240 100
120 5.7 5.7 8.5#
236 25.1 21.0 31.4

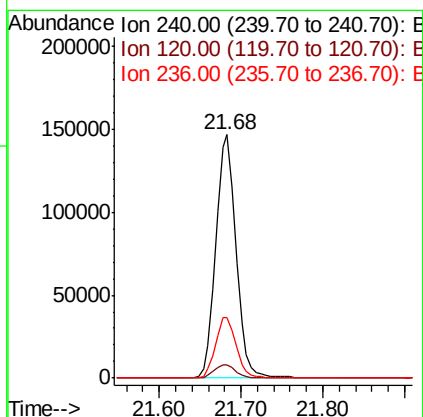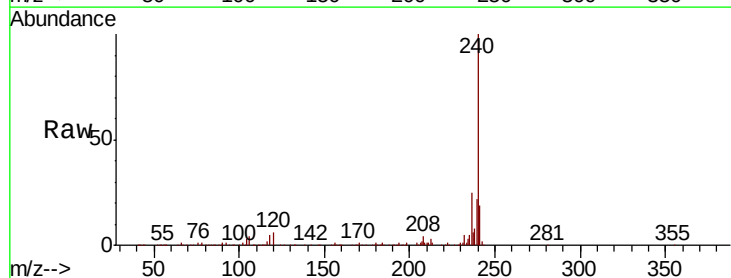

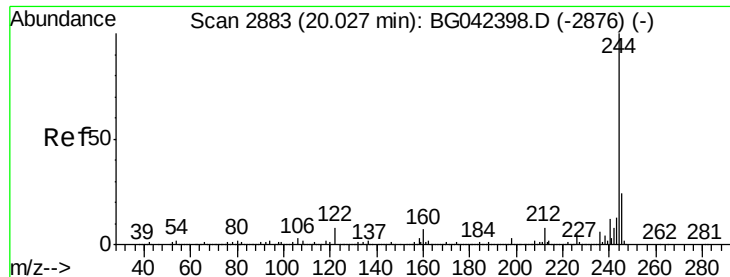

#79

Terphenyl-d14

Concen: 88.309 ng

RT: 20.02 min Scan# 2882

Delta R.T. -0.01 min

Lab File: BG042672.D

Acq: 1 Sep 2019 21:49

Instrument :

BNA_G

ClientSampleId :

SB-15-(13-15)


Tot Ion:244 Resp: 1038527

Ion Ratio Lower Upper

244 100

212 7.0 6.0 9.0

122 6.3 6.7 10.1#



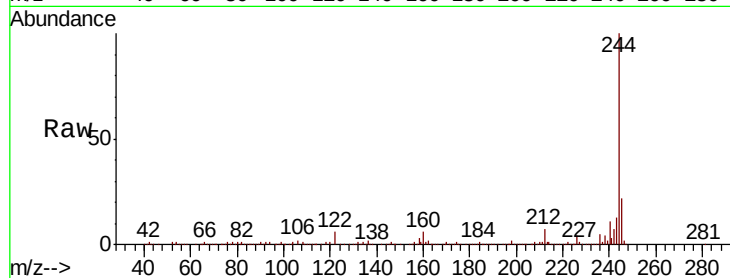


Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

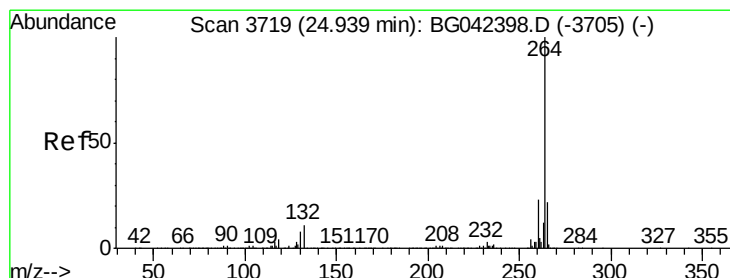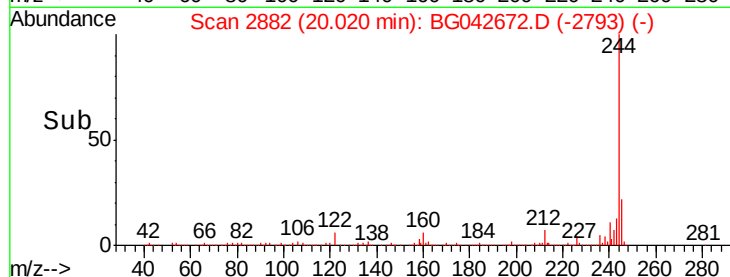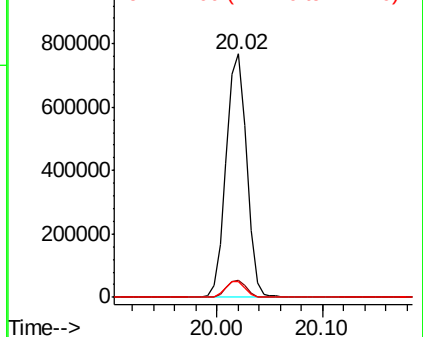

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.93 min Scan# 3717

Delta R.T. -0.01 min

Lab File: BG042672.D

Acq: 1 Sep 2019 21:49


Tgt Ion:264 Resp: 297937

Ion Ratio Lower Upper

264 100

260 22.5 18.5 27.7

265 22.1 17.6 26.4

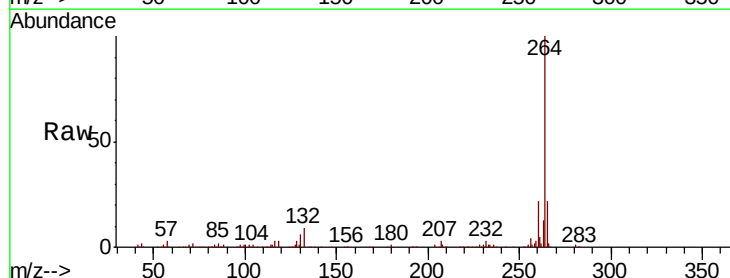

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

