


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG090119\
 Data File : BG042665.D
 Acq On : 1 Sep 2019 16:03
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 22 14:29:15 2019

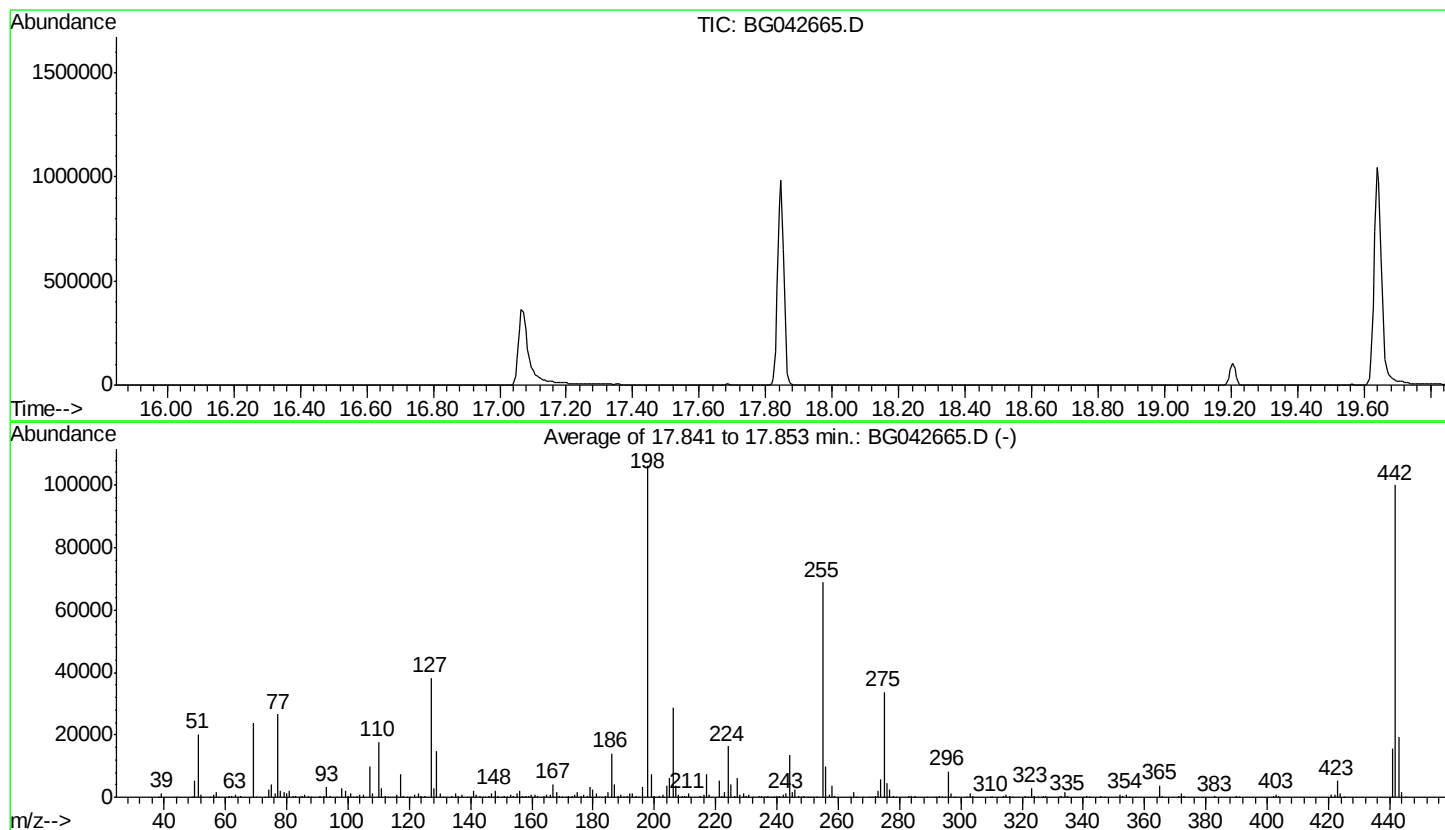

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.1	20273	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	22.4	23755	PASS
70	69	0.00	2	0.3	73	PASS
127	198	10	80	36.1	38346	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	106248	PASS
199	198	5	9	7.2	7597	PASS
275	198	10	60	31.8	33770	PASS
365	198	1	100	3.6	3868	PASS
441	198	0.01	100	14.8	15695	PASS
442	198	50	100	94.2	100056	PASS
443	442	15	24	19.1	19098	PASS