
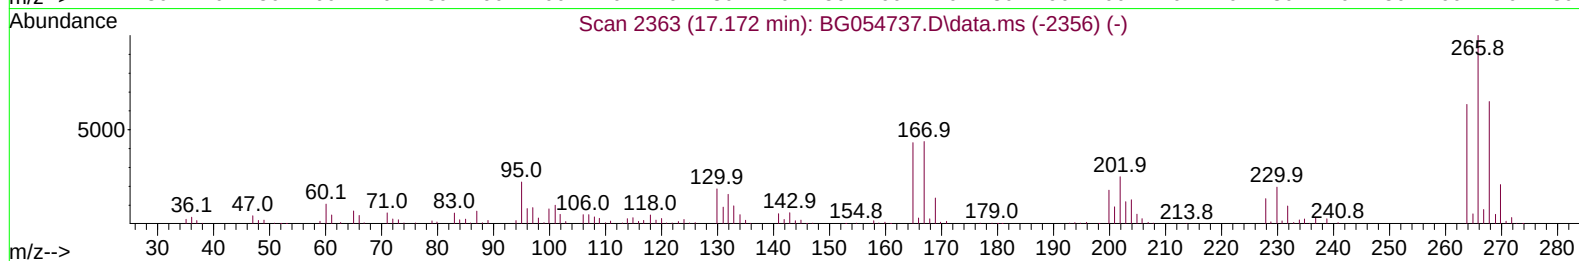
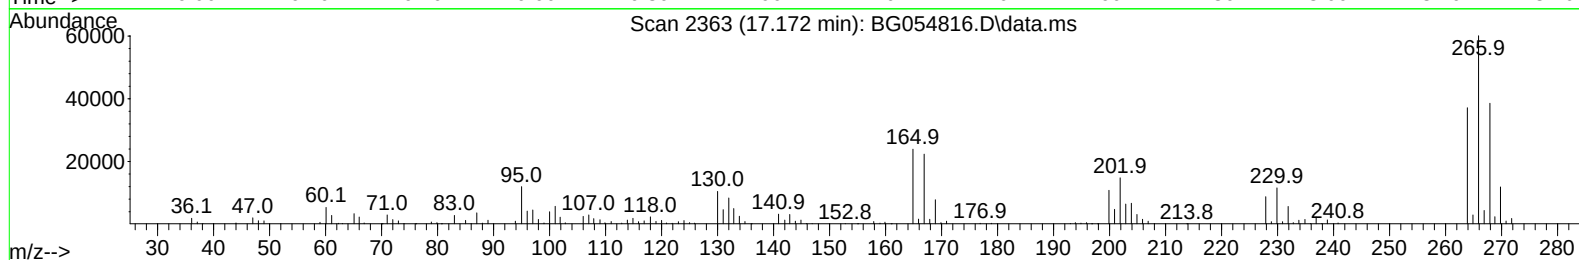


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG090122\  
Data File : BG054816.D  
Acq On : 1 Sep 2022 10:35  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 17:29:44 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG082522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Aug 25 17:50:55 2022  
Response via : Initial Calibration

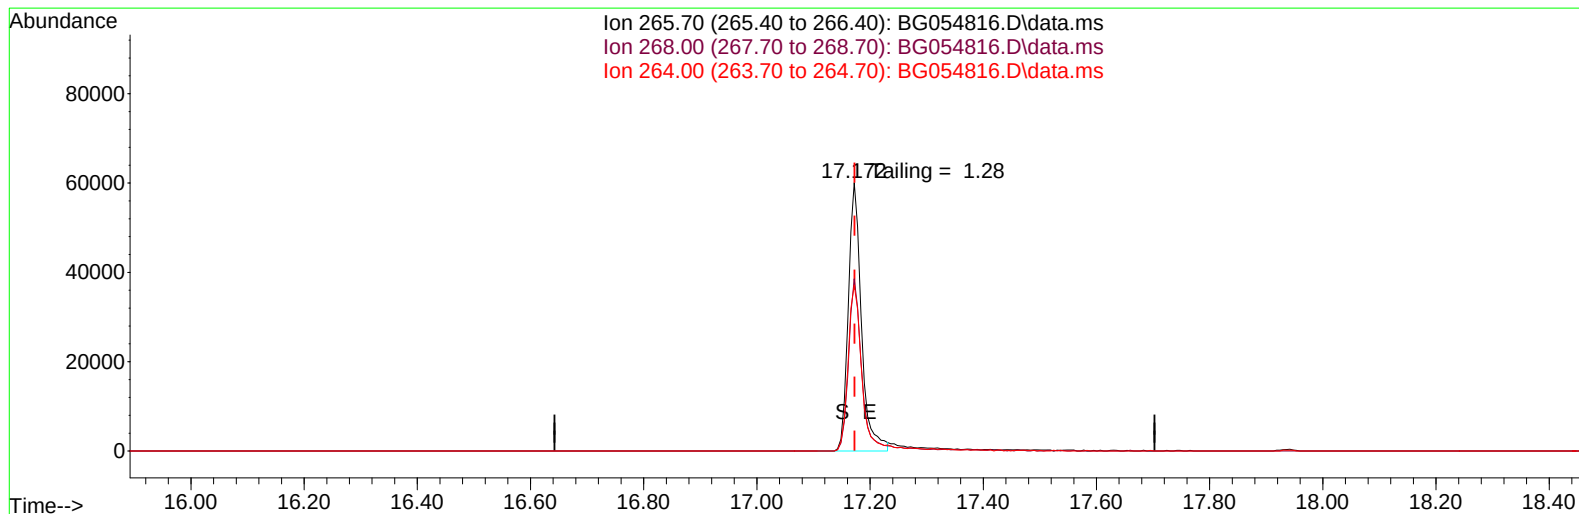

TIC: BG054816.D\data.ms

**(70) Pentachlorophenol (C)**




17.172min (-0.000) 282120.93 ng

response 100272

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.00  | 64.18  |
| 264.00 | 61.70  | 61.82  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG090122\  
Data File : BG054816.D  
Acq On : 1 Sep 2022 10:35  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 17:29:44 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG082522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Aug 25 17:50:55 2022  
Response via : Initial Calibration

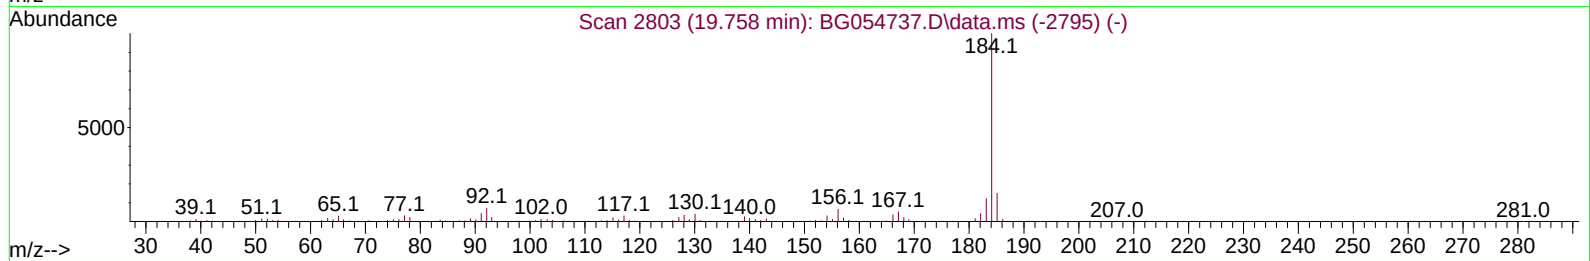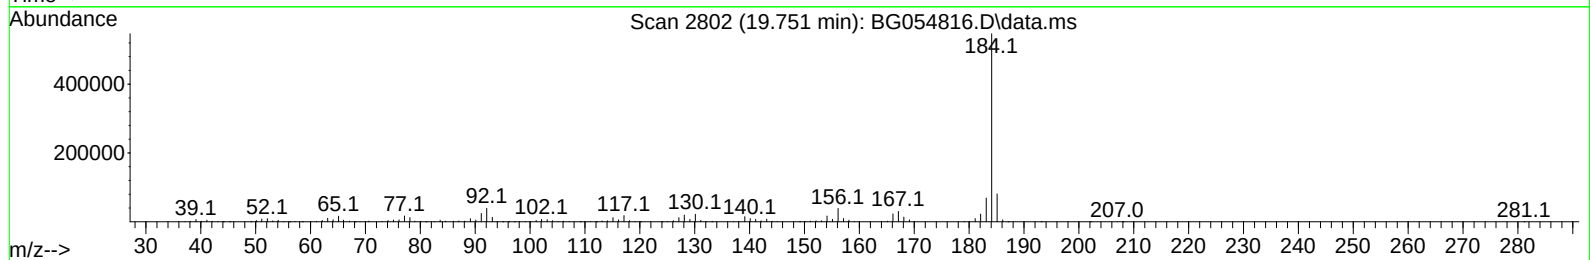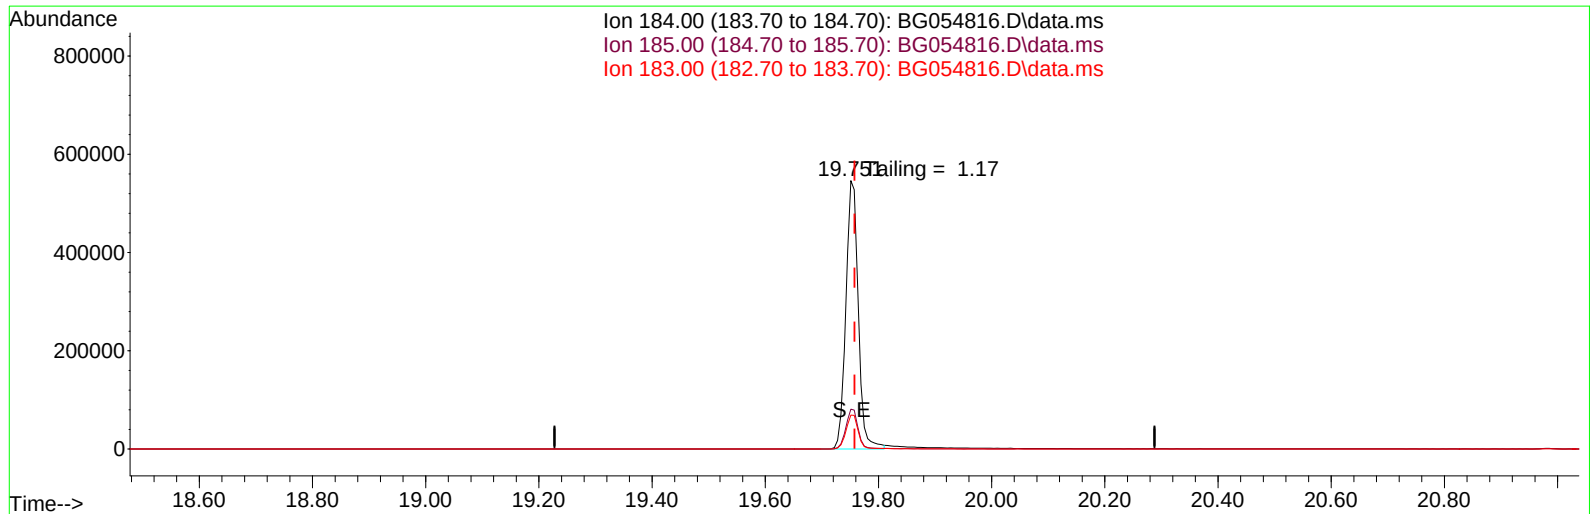

TIC: BG054816.D\data.ms

**(77) Benzidine**

19.751min (-0.006) 42835.85 ng

response 864708

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.20  | 14.85  |
| 183.00 | 12.30  | 12.66  |
| 0.00   | 0.00   | 0.00   |