


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090122\
 Data File : BG054816.D
 Acq On : 1 Sep 2022 10:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 25 17:50:55 2022

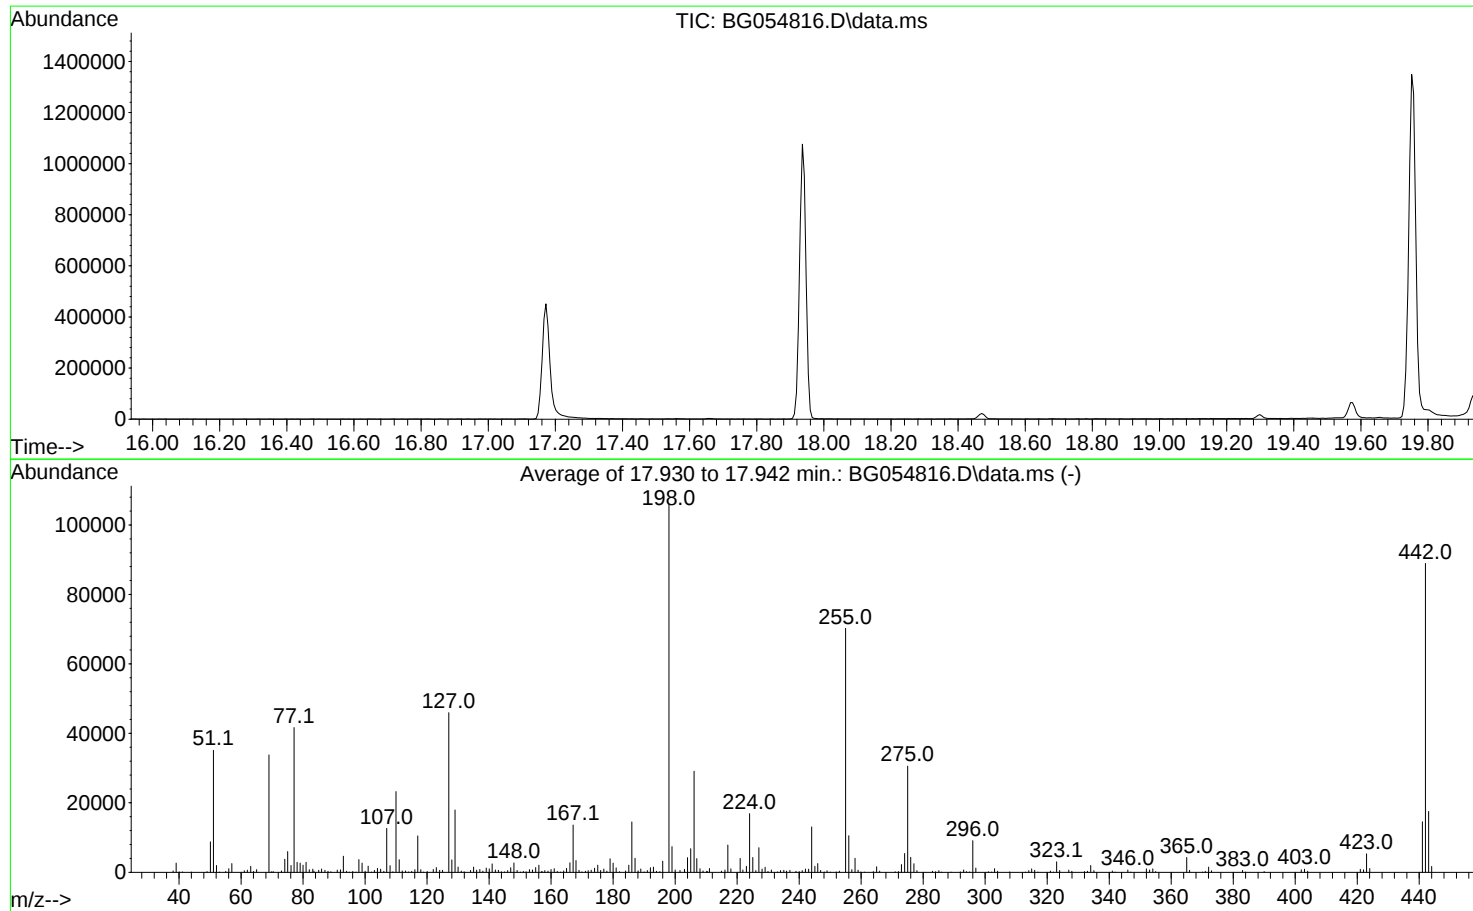




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	35149	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.9	33811	PASS
70	69	0.00	2	0.5	175	PASS
127	198	10	80	43.4	45944	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	105917	PASS
199	198	5	9	7.0	7416	PASS
275	198	10	60	28.8	30555	PASS
365	198	1	100	4.0	4278	PASS
441	198	0.01	100	13.7	14549	PASS
442	442	50	100	100.0	88944	PASS
443	442	15	24	19.7	17522	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090122\
Data File : BG054816.D
Acq On : 1 Sep 2022 10:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 01 17:29:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

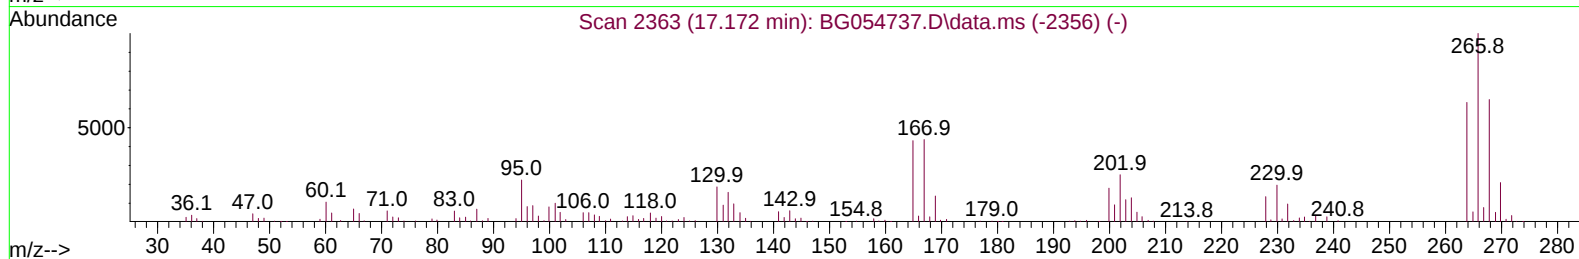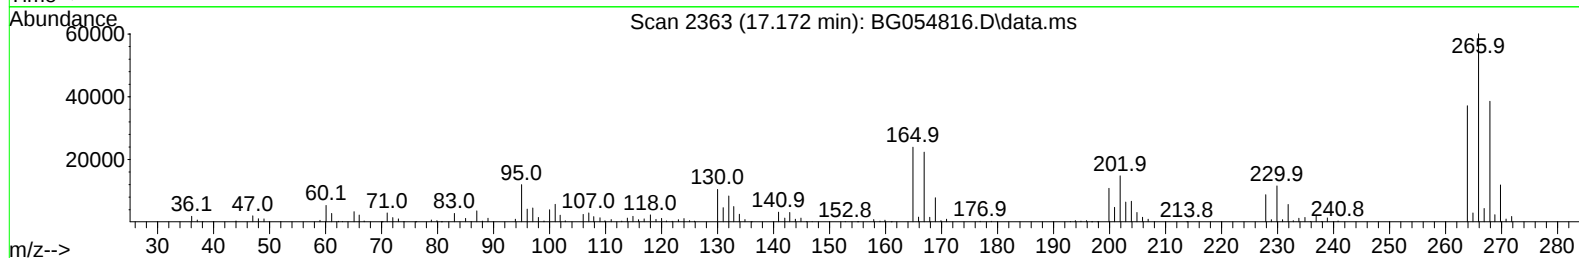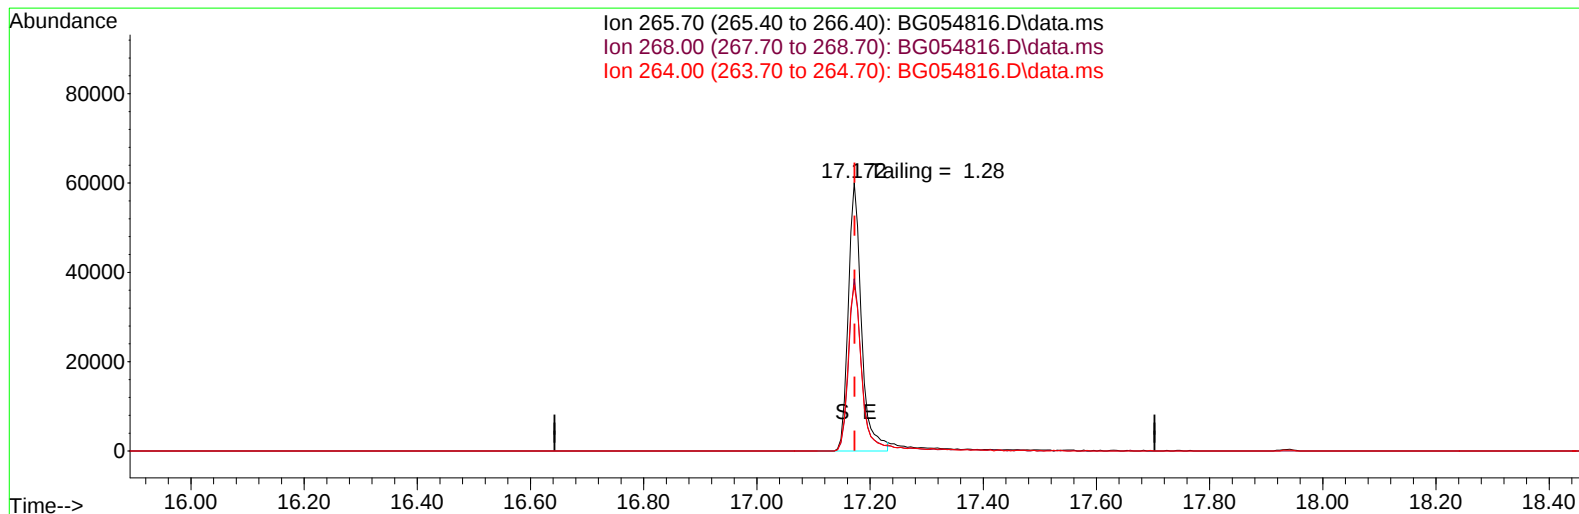

TIC: BG054816.D\data.ms

(70) Pentachlorophenol (C)

17.172min (-0.000) 282120.93 ng




response 100272

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	64.18
264.00	61.70	61.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090122\
Data File : BG054816.D
Acq On : 1 Sep 2022 10:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 01 17:29:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 17:50:55 2022
Response via : Initial Calibration

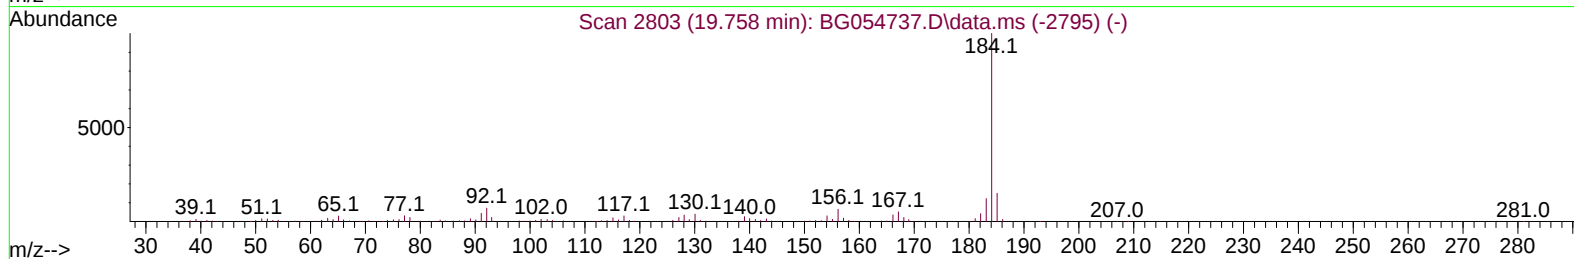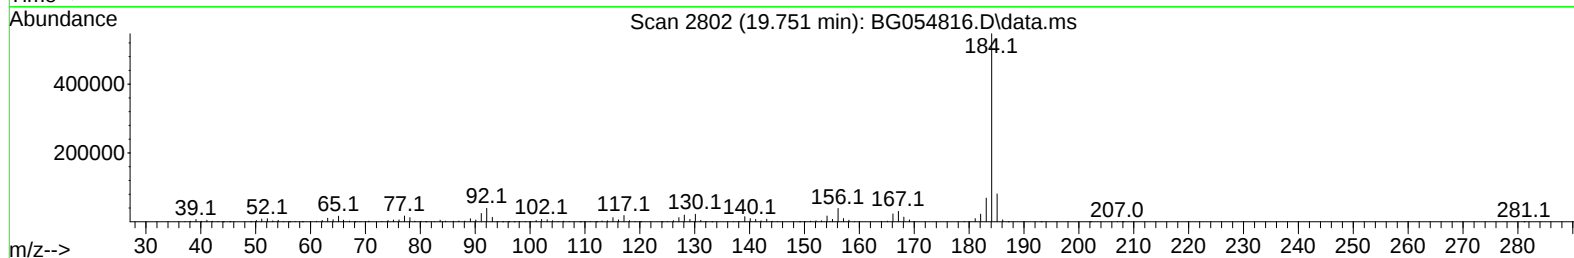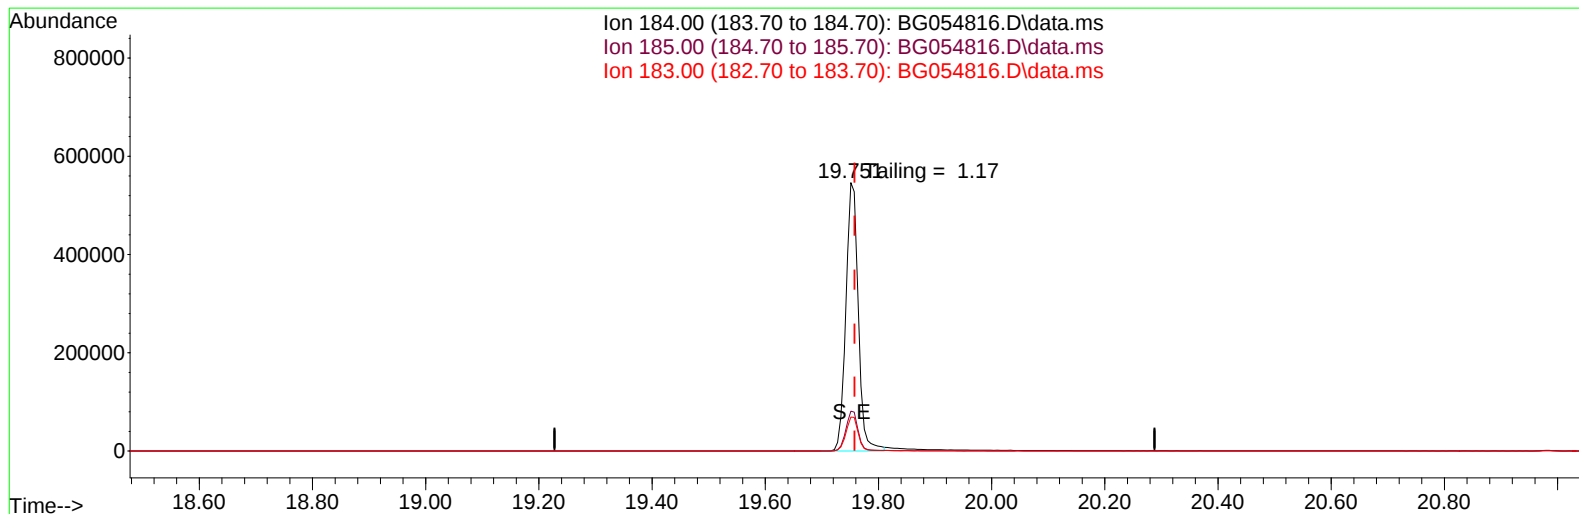

TIC: BG054816.D\data.ms

(77) Benzidine

19.751min (-0.006) 42835.85 ng

response 864708

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.85
183.00	12.30	12.66
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/1/2022	BNA_G	BG054816.D
Compound Name	Response	Retention Time
DDT	395695	20.98
DDD	8451	20.53
DDE	519	20.02
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8970	404665	2.22

Instrument :
BNA_G
ClientSampleId :
DFTPP