
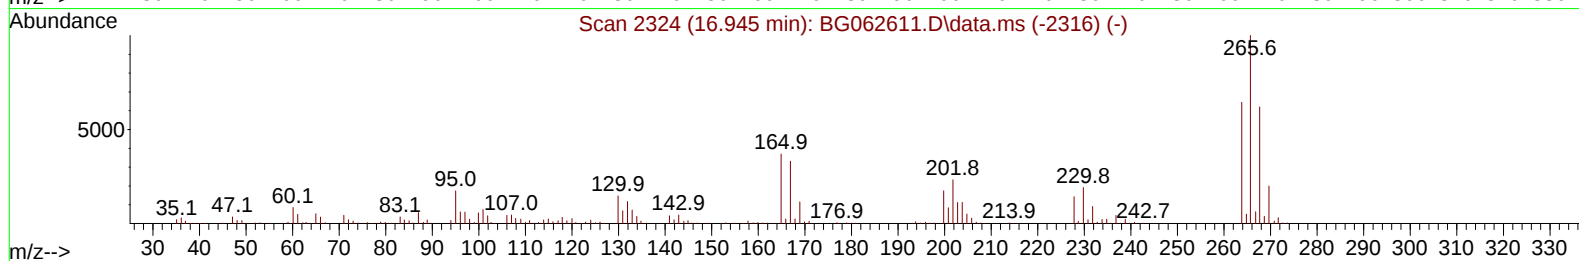
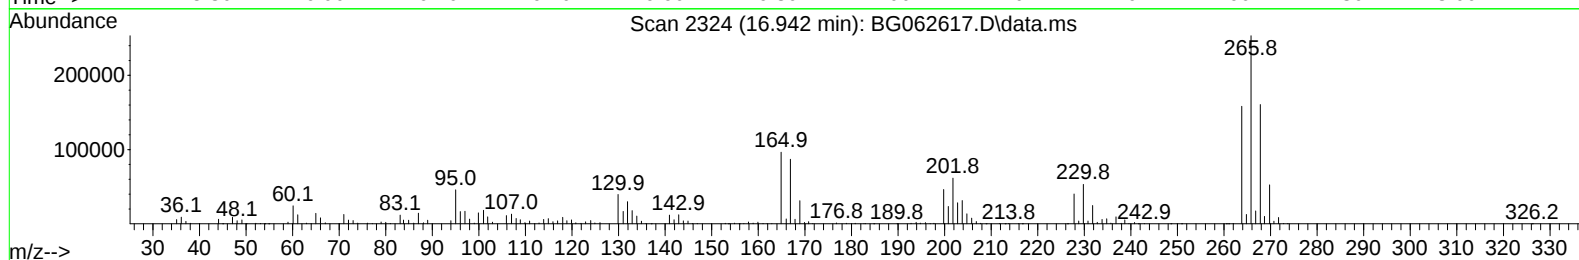


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090324\
Data File : BG062617.D
Acq On : 3 Sep 2024 8:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 12:16:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 02:36:01 2024
Response via : Initial Calibration

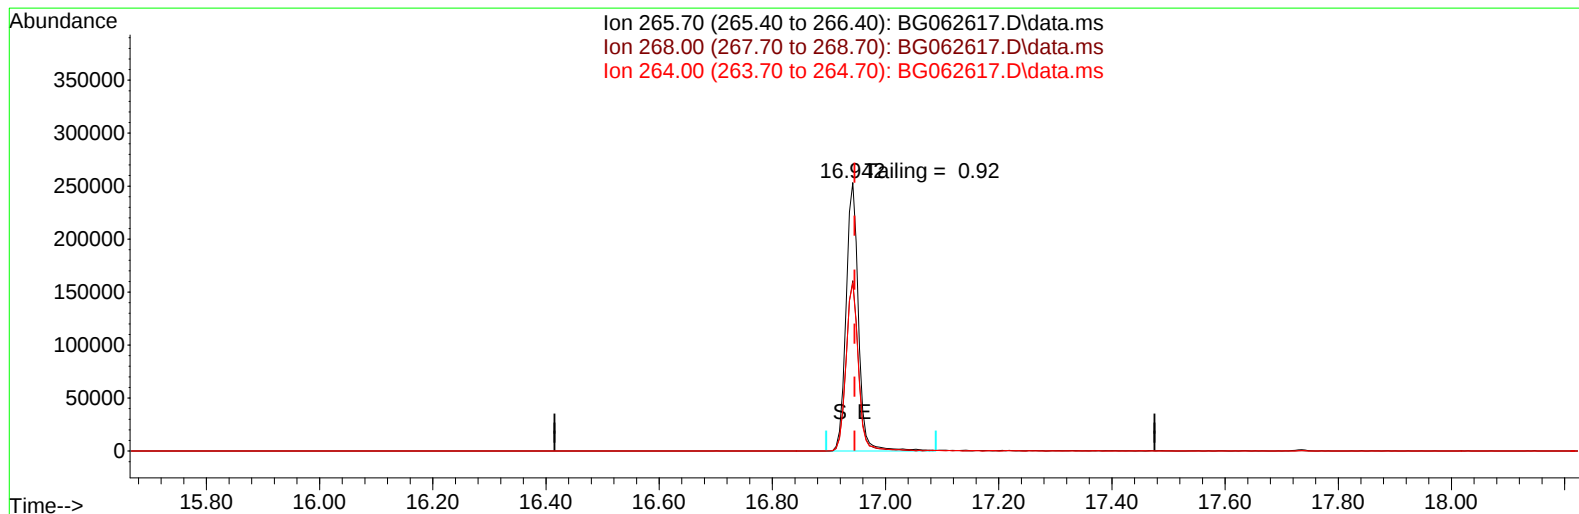

TIC: BG062617.D\data.ms

(70) Pentachlorophenol (C)




16.942min (-0.003) 49388.52 ng

response 386250

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	67.48
264.00	64.50	62.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090324\
Data File : BG062617.D
Acq On : 3 Sep 2024 8:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 12:16:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 02:36:01 2024
Response via : Initial Calibration

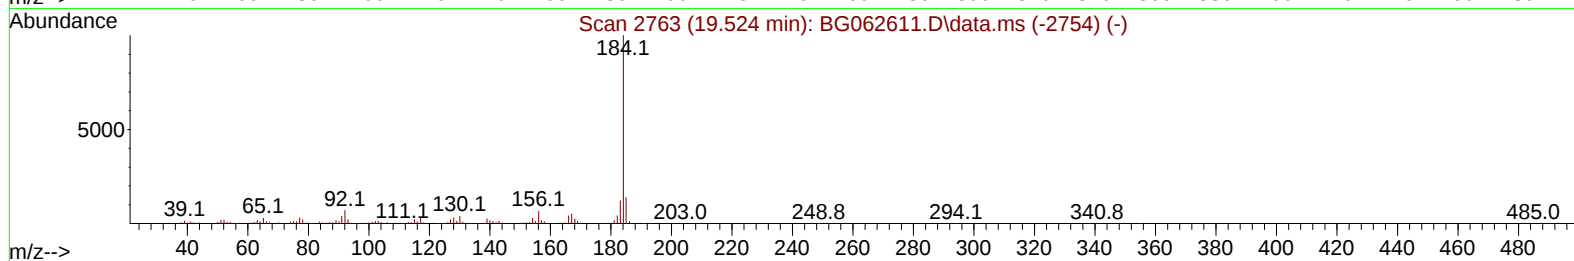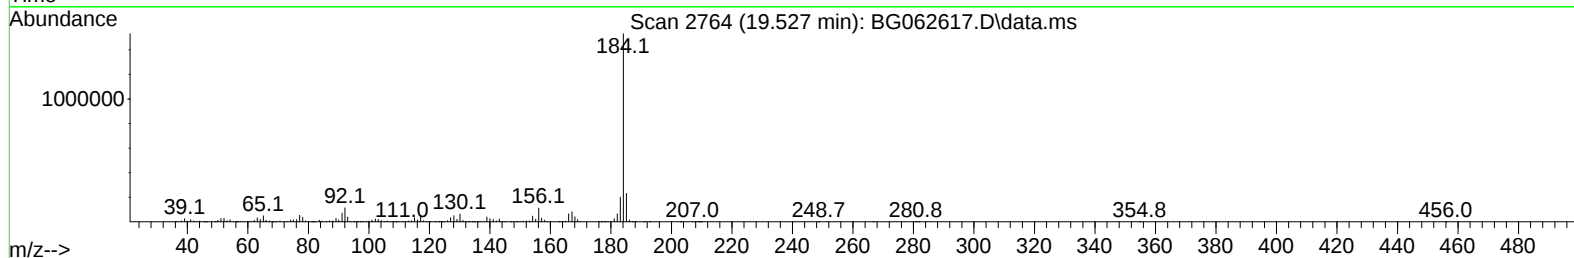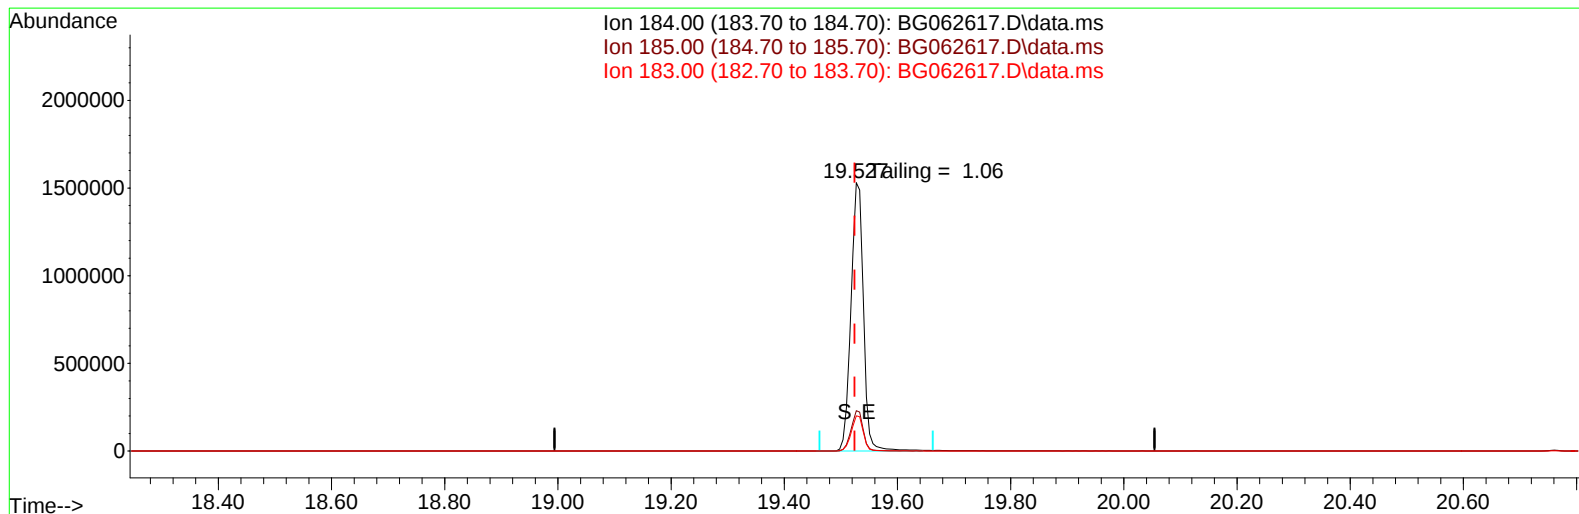

TIC: BG062617.D\data.ms

(77) Benzidine**19.527min (+ 0.003) 80011.47 ng****response 2334791**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	15.07
183.00	12.10	13.11
0.00	0.00	0.00