


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090324\
Data File : BG062617.D
Acq On : 3 Sep 2024 8:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Aug 31 02:36:01 2024

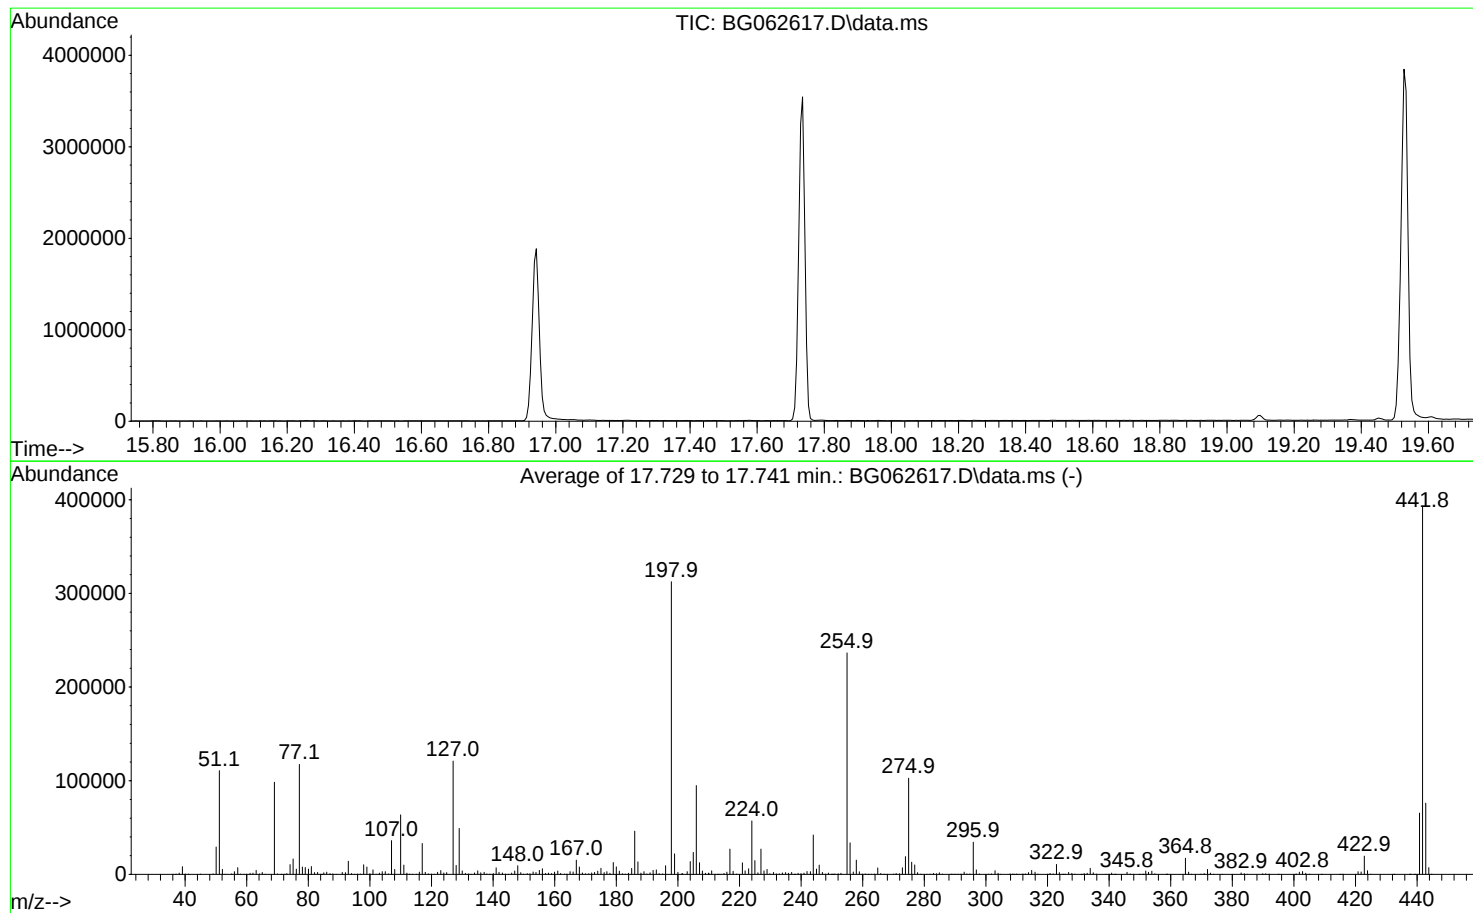




AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	110693	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.5	98373	PASS
70	69	0.00	2	0.6	599	PASS
127	198	10	80	38.7	121005	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	312469	PASS
199	198	5	9	7.0	21860	PASS
275	198	10	60	32.9	102760	PASS
365	198	1	100	5.6	17347	PASS
441	198	0.01	100	20.9	65400	PASS
442	442	50	100	100.0	392768	PASS
443	442	15	24	19.4	76067	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090324\
Data File : BG062617.D
Acq On : 3 Sep 2024 8:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 03 12:16:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 02:36:01 2024
Response via : Initial Calibration

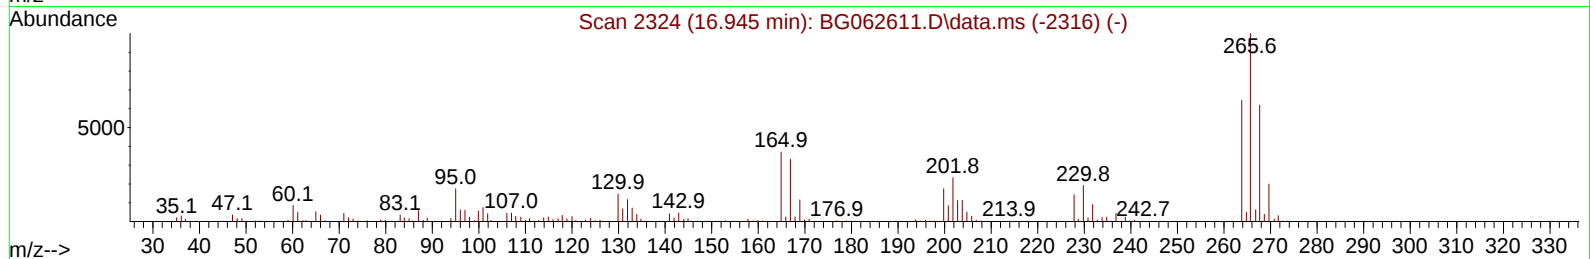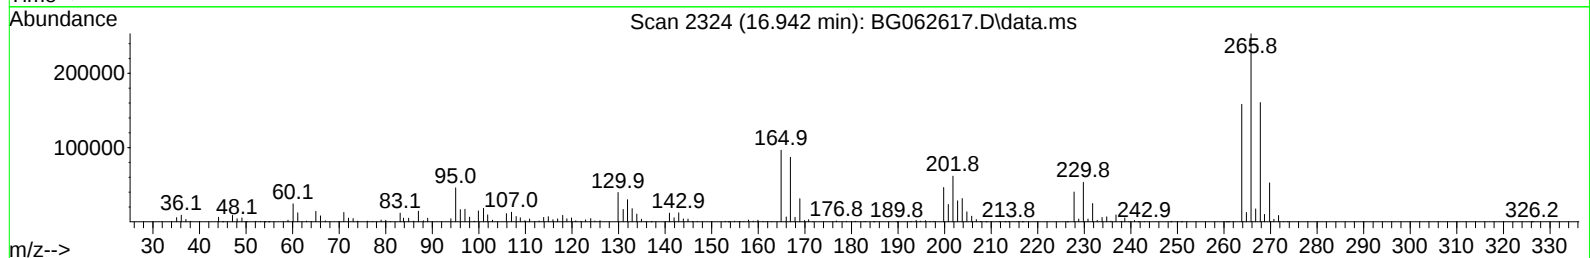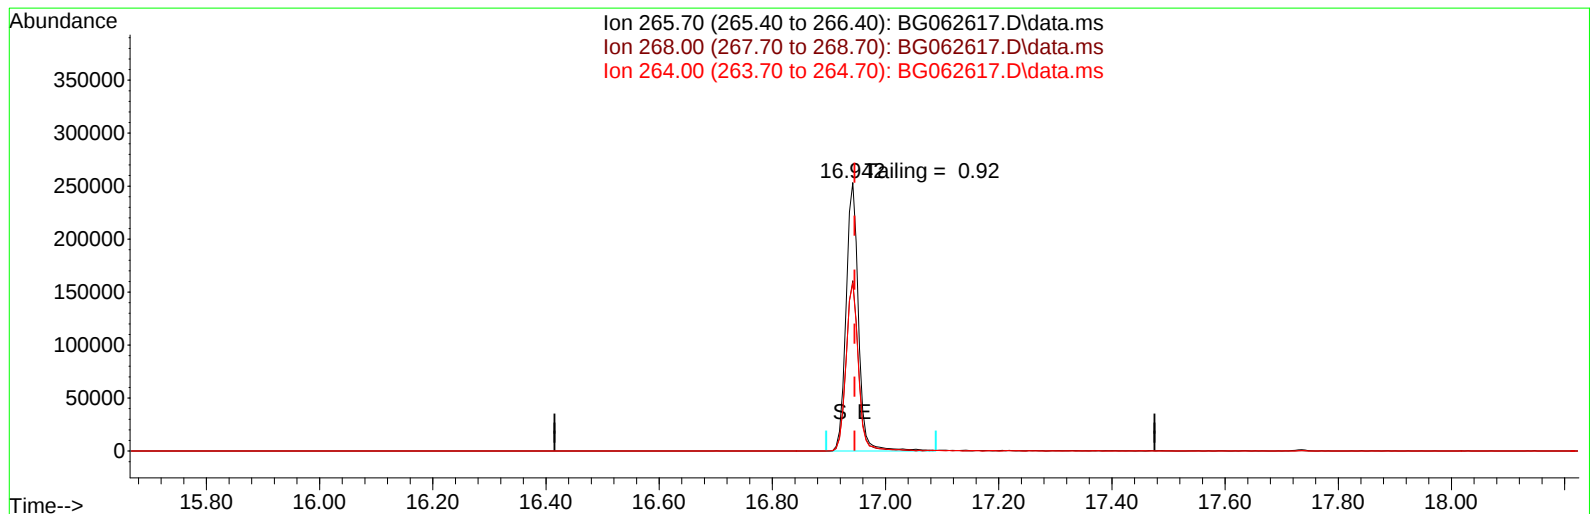

TIC: BG062617.D\data.ms

(70) Pentachlorophenol (C)

16.942min (-0.003) 49388.52 ng




response 386250

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	67.48
264.00	64.50	62.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090324\
Data File : BG062617.D
Acq On : 3 Sep 2024 8:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 03 12:16:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG083024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 02:36:01 2024
Response via : Initial Calibration

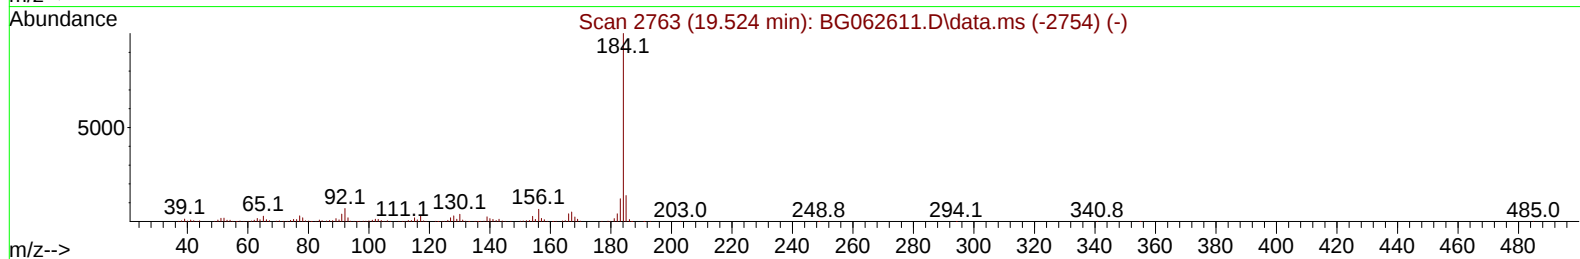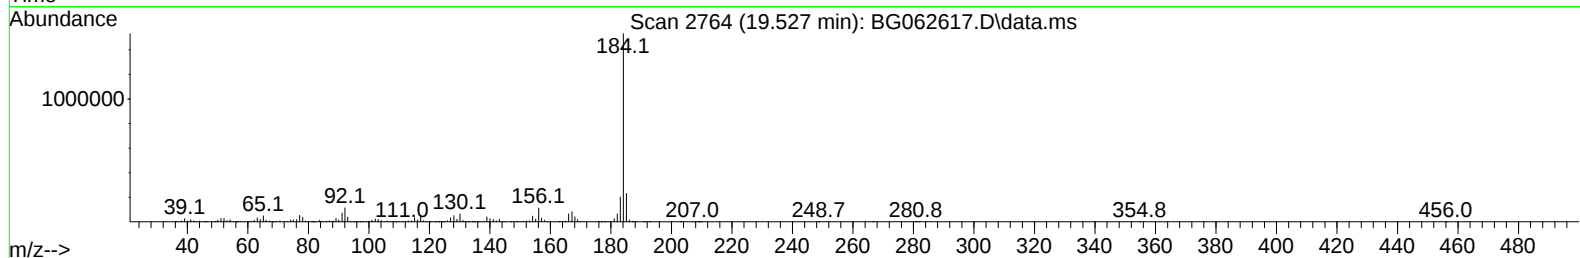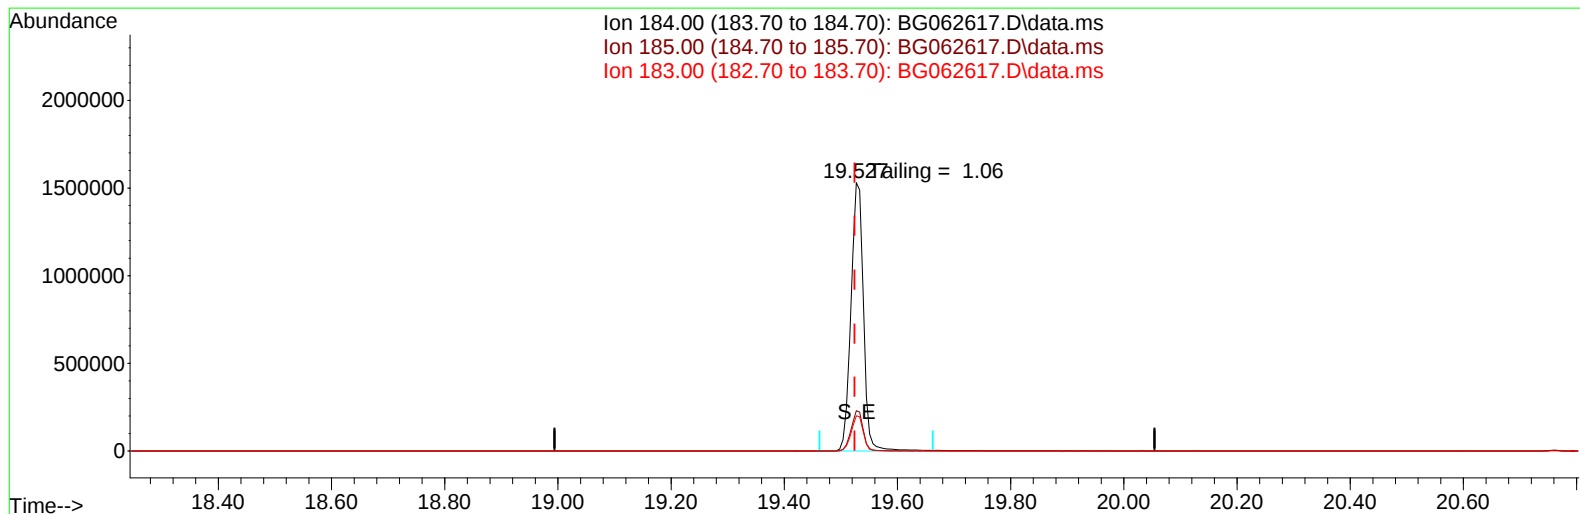

TIC: BG062617.D\data.ms

(77) Benzidine

19.527min (+ 0.003) 80011.47 ng

response 2334791

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	15.07
183.00	12.10	13.11
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/3/2024	BNA_G	<u>BG062617.D</u>
Compound Name	Response	Retention Time
DDT	961965	20.761
DDD	19513	20.32
DDE	811	19.815
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20324	982289	2.07

Instrument :
BNA_G
ClientSampleId :
DFTPP