
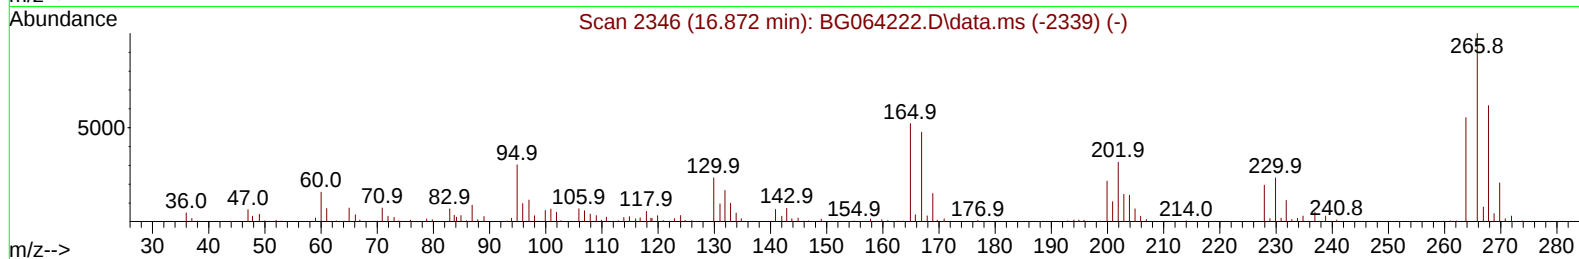
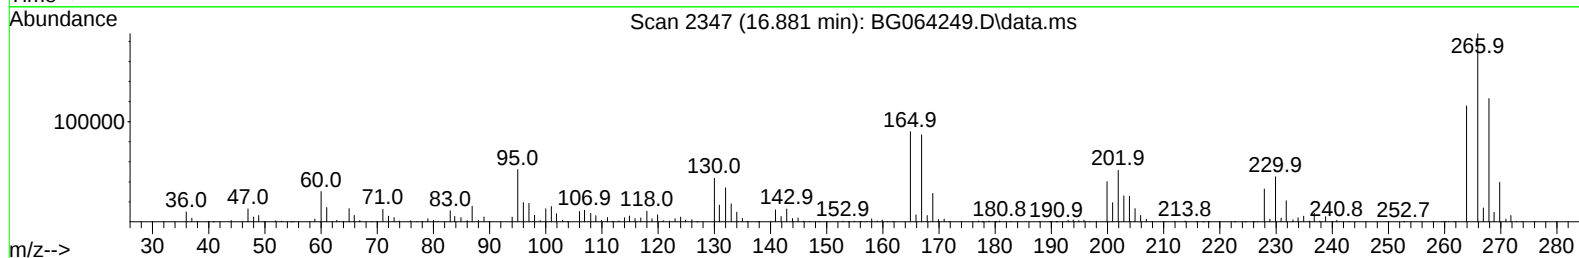


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090325\
Data File : BG064249.D
Acq On : 3 Sep 2025 11:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 12:45:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

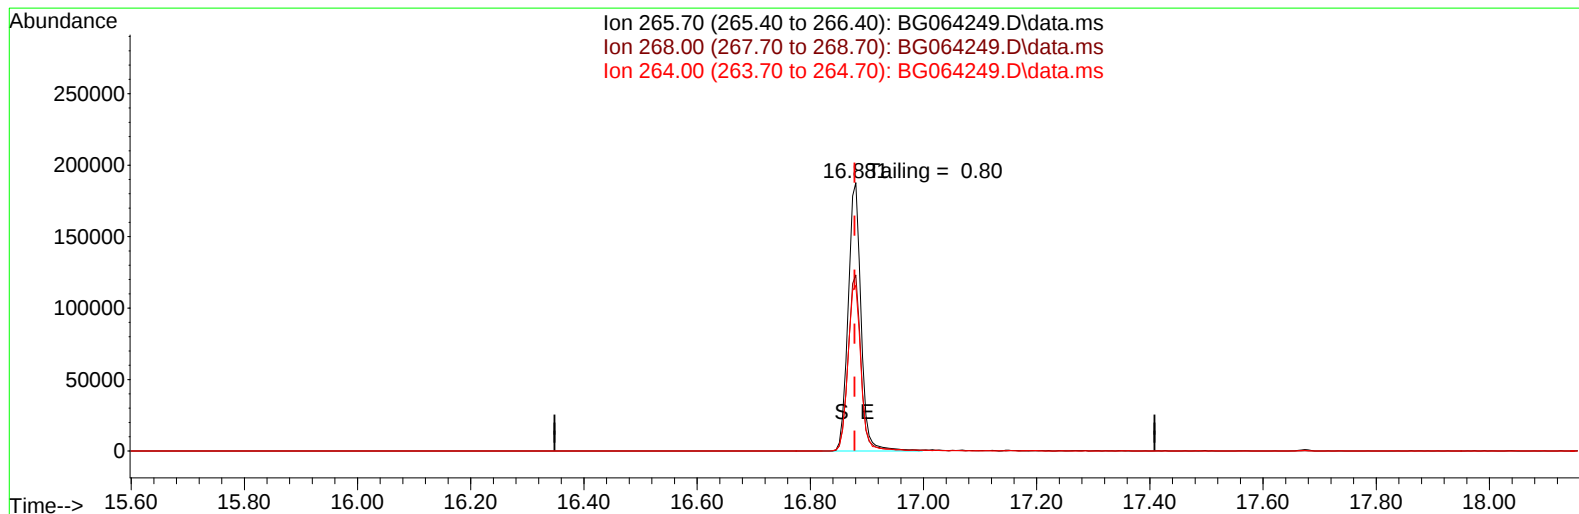

TIC: BG064249.D\data.ms

(70) Pentachlorophenol (C)




16.881min (+ 0.003) 612423.57 ng

response 297829

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	65.60
264.00	55.40	61.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090325\
Data File : BG064249.D
Acq On : 3 Sep 2025 11:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 12:45:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

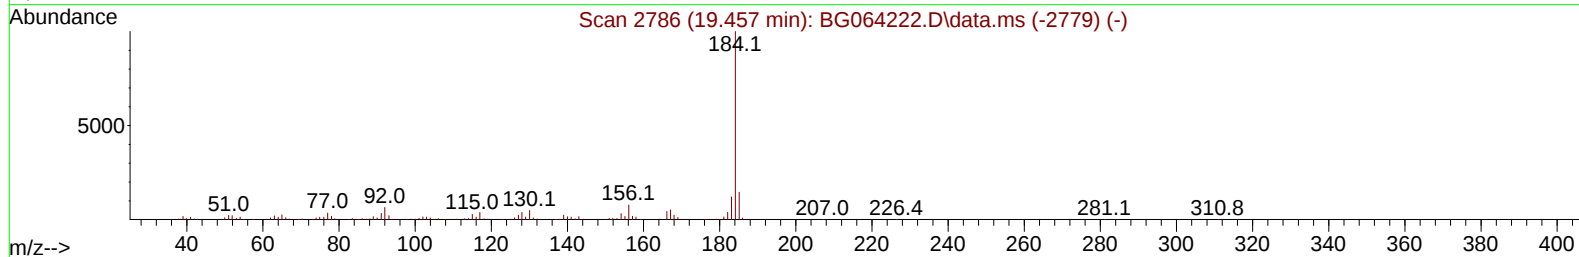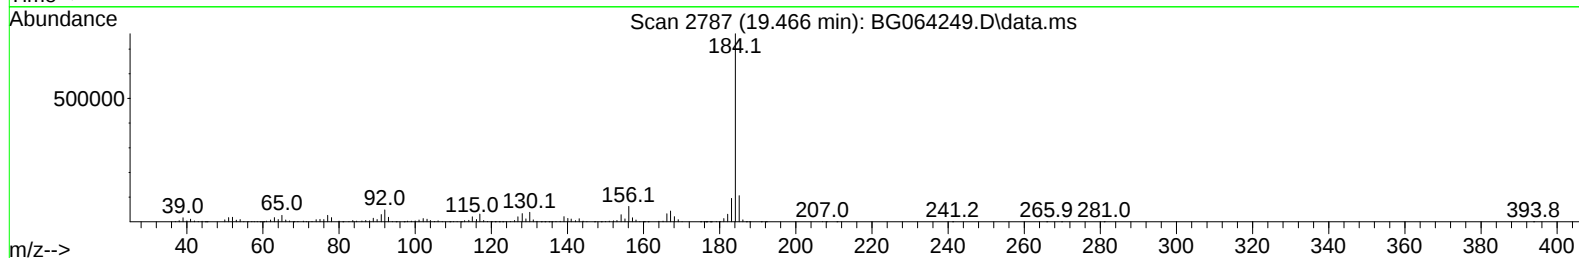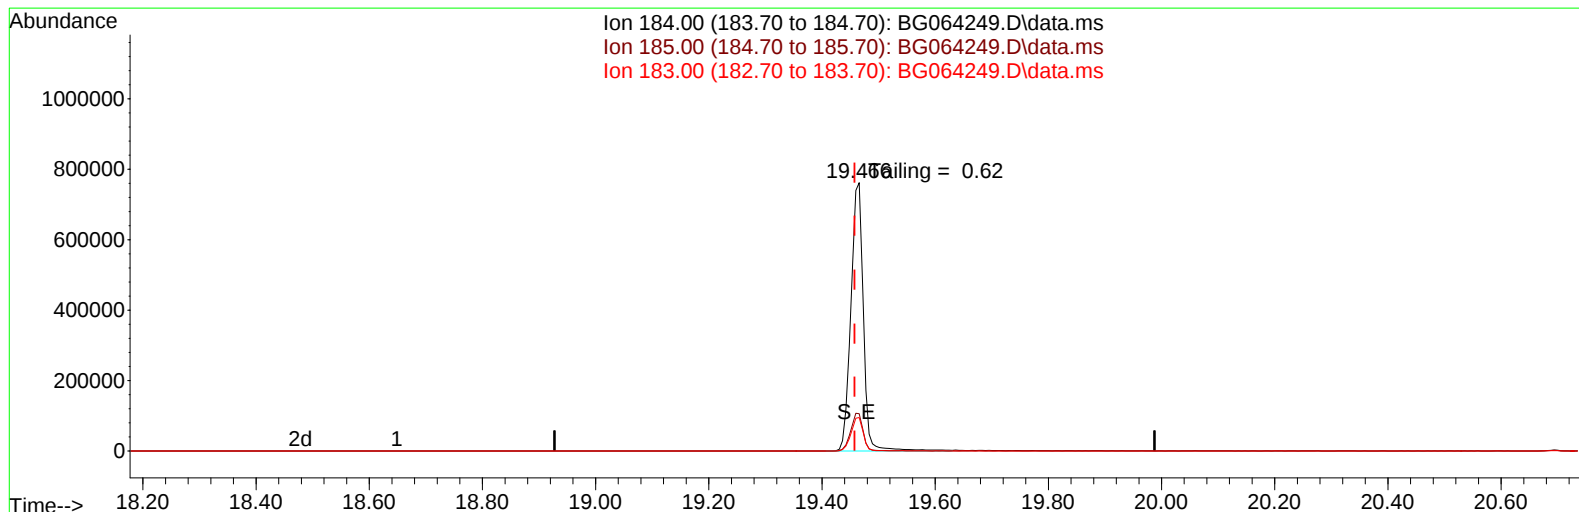

TIC: BG064249.D\data.ms

(77) Benzidine

19.466min (+ 0.008) 5991.08 ng m

response 1180283

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.90
183.00	12.10	12.48
0.00	0.00	0.00