
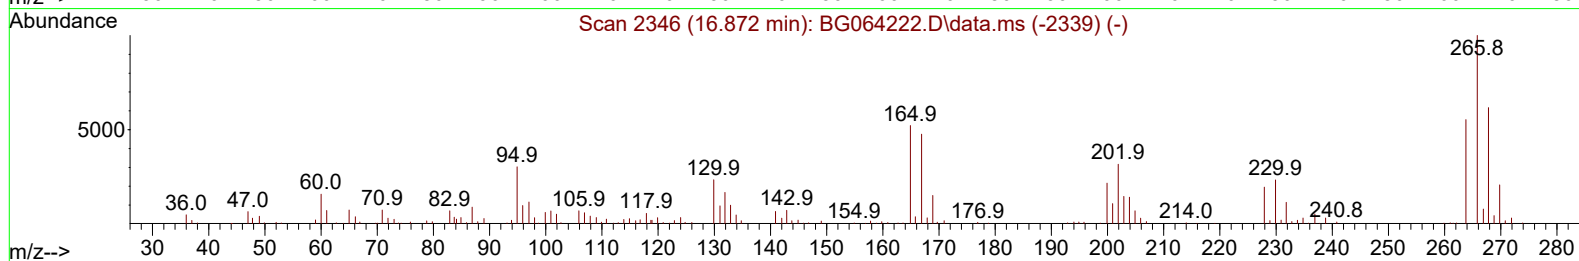
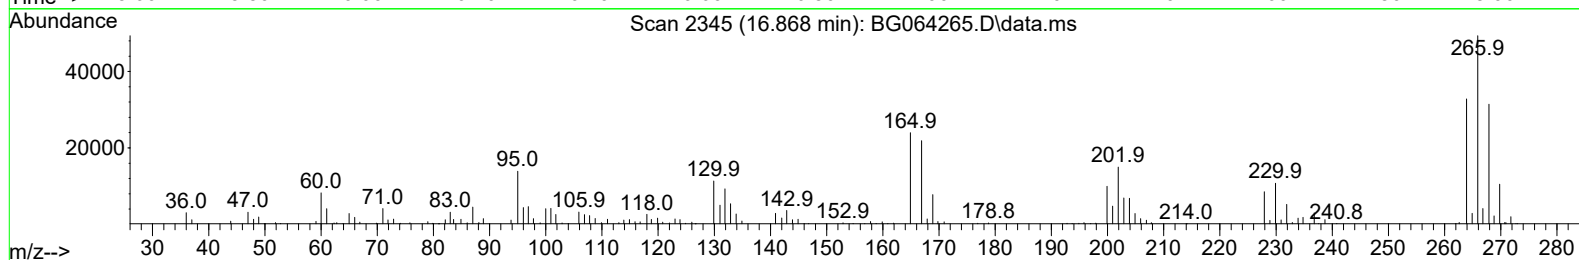


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG090325\  
Data File : BG064265.D  
Acq On : 3 Sep 2025 23:18  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 04 01:49:02 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG082825.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Aug 28 17:41:58 2025  
Response via : Initial Calibration

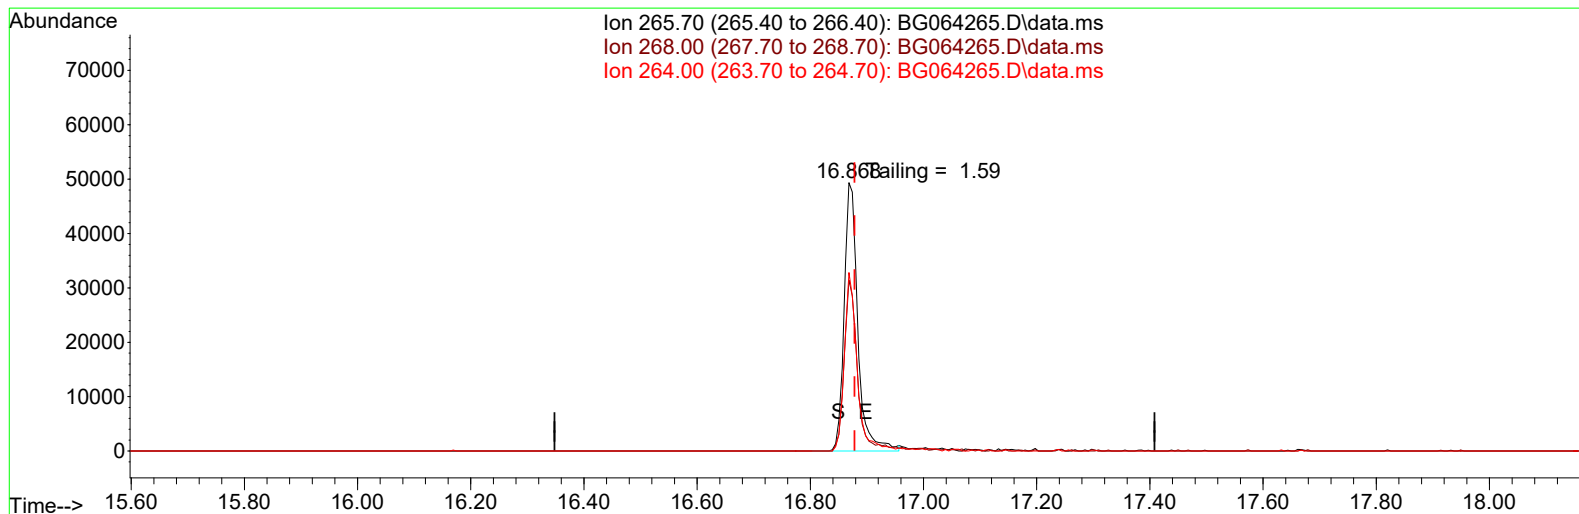

TIC: BG064265.D\data.ms

**(70) Pentachlorophenol (C)**




**16.868min (-0.010) 195043.33 ng**

**response 82298**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.70  | 63.66  |
| 264.00 | 55.40  | 66.46  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG090325\  
Data File : BG064265.D  
Acq On : 3 Sep 2025 23:18  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 04 01:49:02 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG082825.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Aug 28 17:41:58 2025  
Response via : Initial Calibration

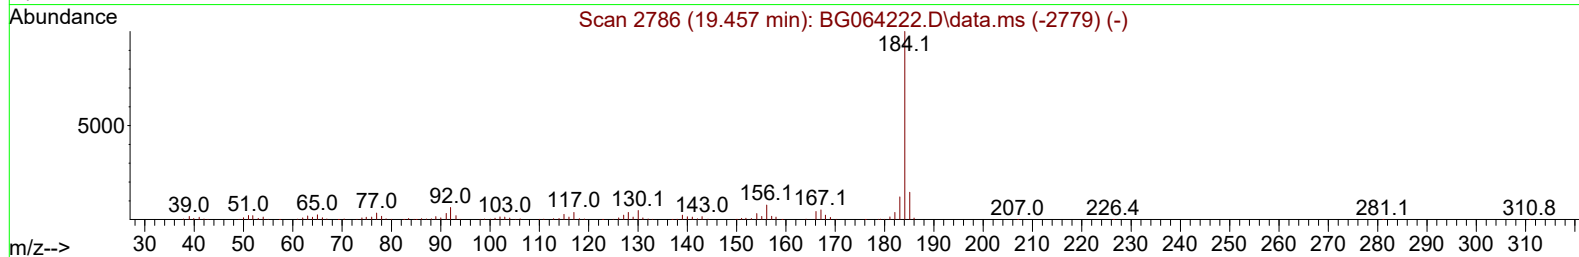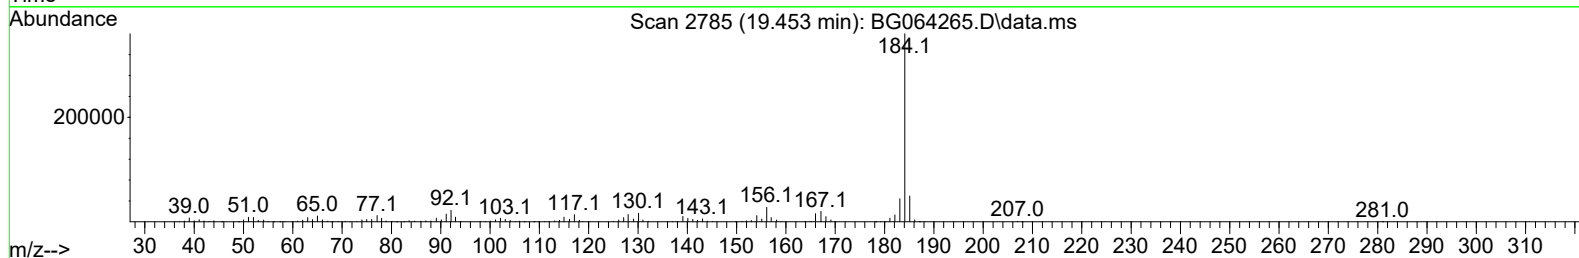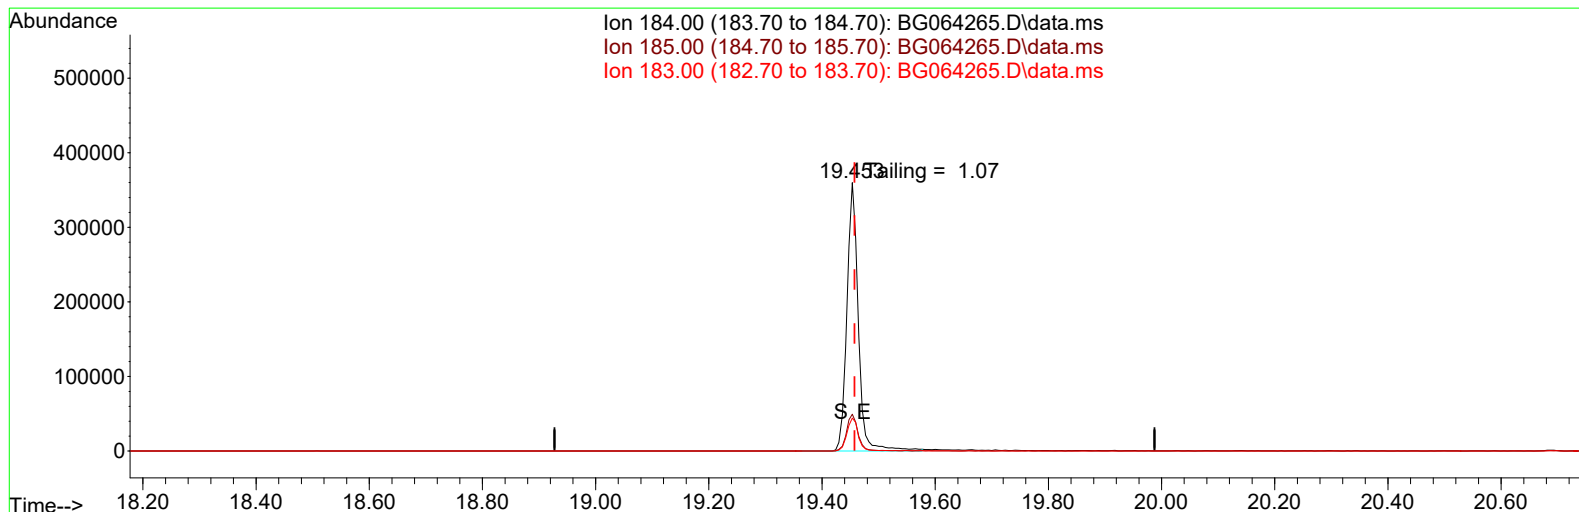

TIC: BG064265.D\data.ms

**(77) Benzidine****19.453min (-0.004) 359802.62 ng****response 499553**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.60  | 13.71  |
| 183.00 | 12.10  | 12.29  |
| 0.00   | 0.00   | 0.00   |