
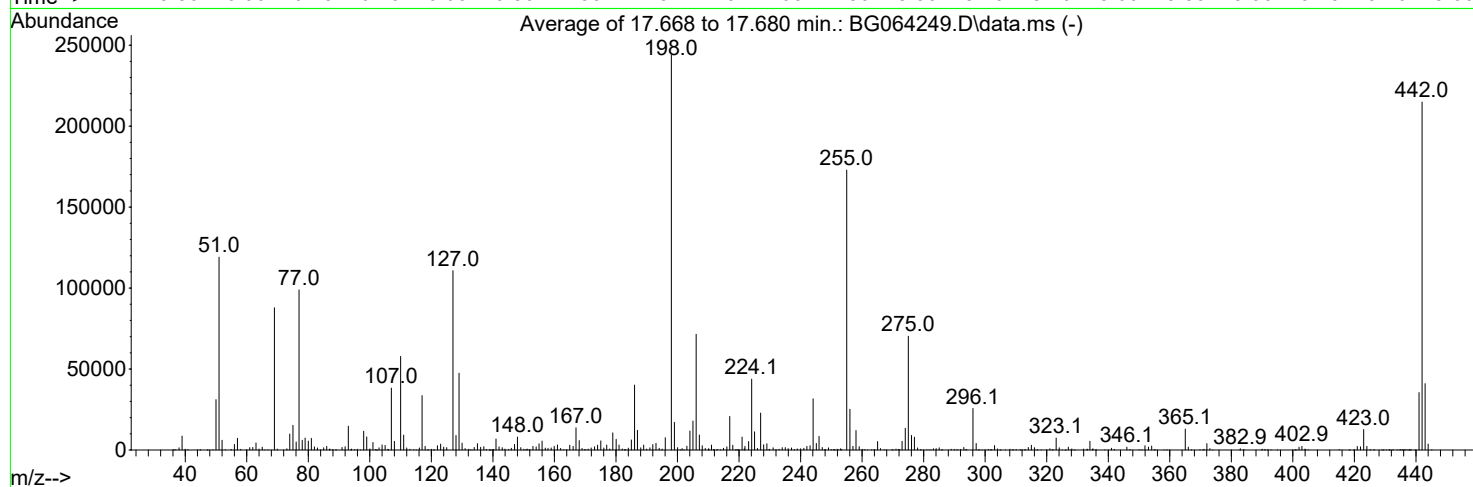


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090325\
Data File : BG064249.D
Acq On : 3 Sep 2025 11:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 28 17:41:58 2025

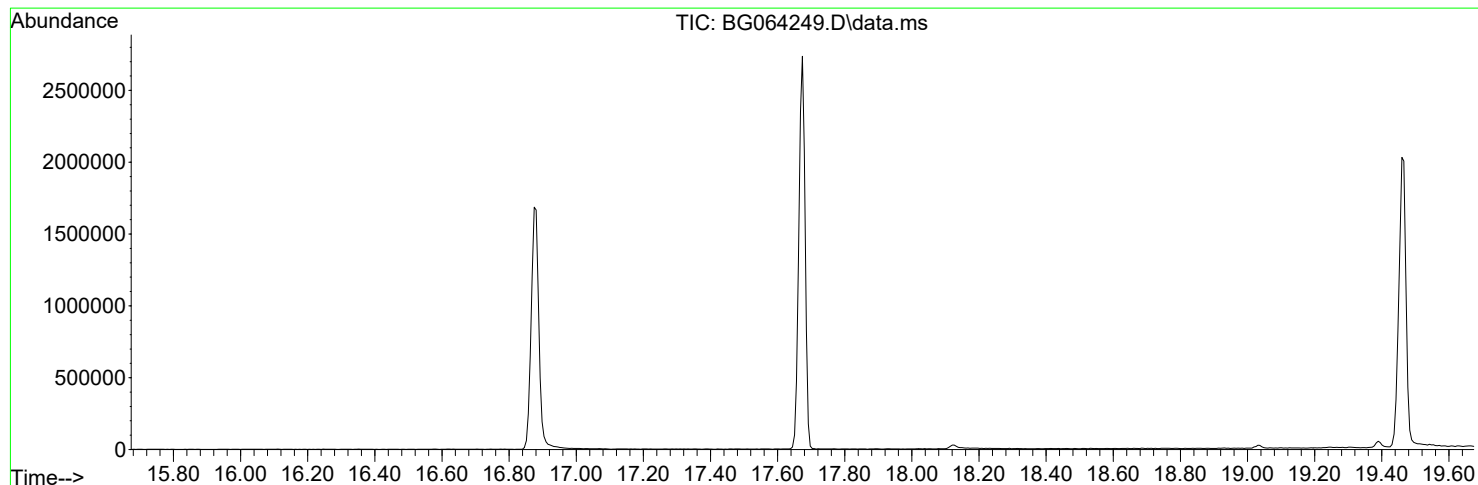

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	87883	PASS
70	69	0.00	2	0.6	570	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	243819	PASS
199	198	5	9	7.0	17148	PASS
365	198	1	100	5.3	12990	PASS
441	443	0.01	150	86.5	35437	PASS
442	442	100	100	100.0	214933	PASS
443	442	15	24	19.1	40989	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/2/2025	BNA_G	BG064239.D
Compound Name	Response	Retention Time
DDT	618340	20.694
DDD	14208	20.253
DDE	656	19.748
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14864	633204	2.35

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090325\
Data File : BG064249.D
Acq On : 3 Sep 2025 11:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 03 12:45:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

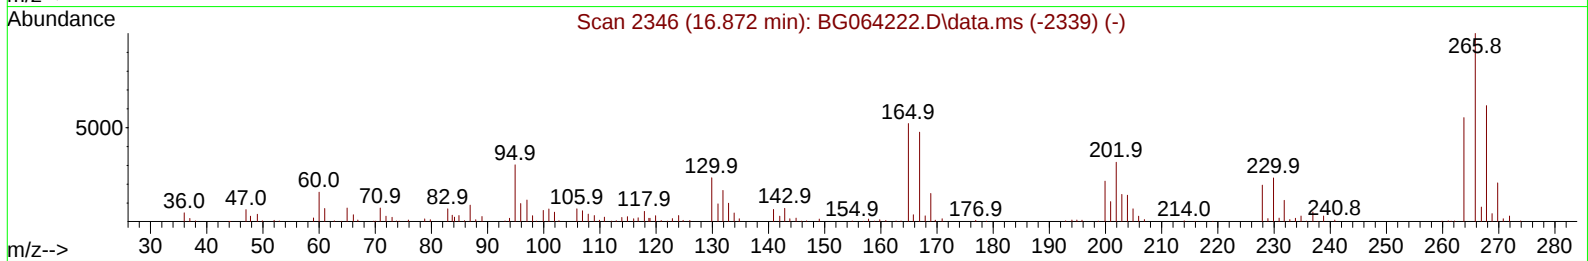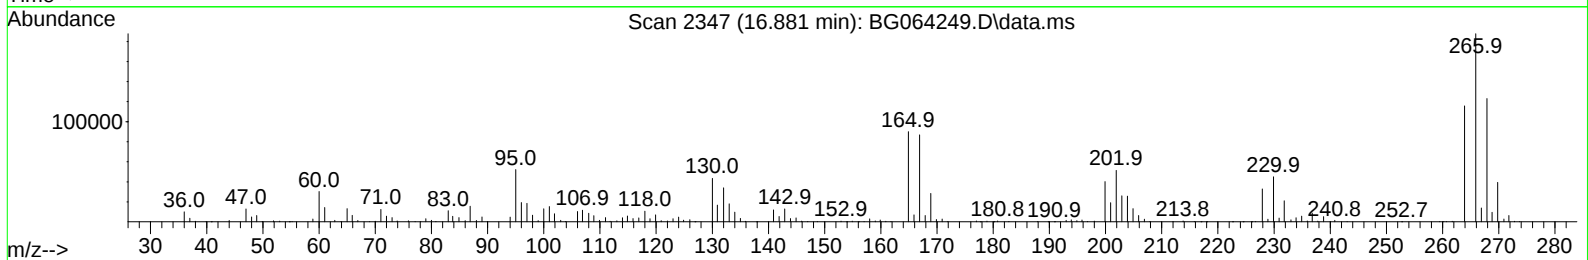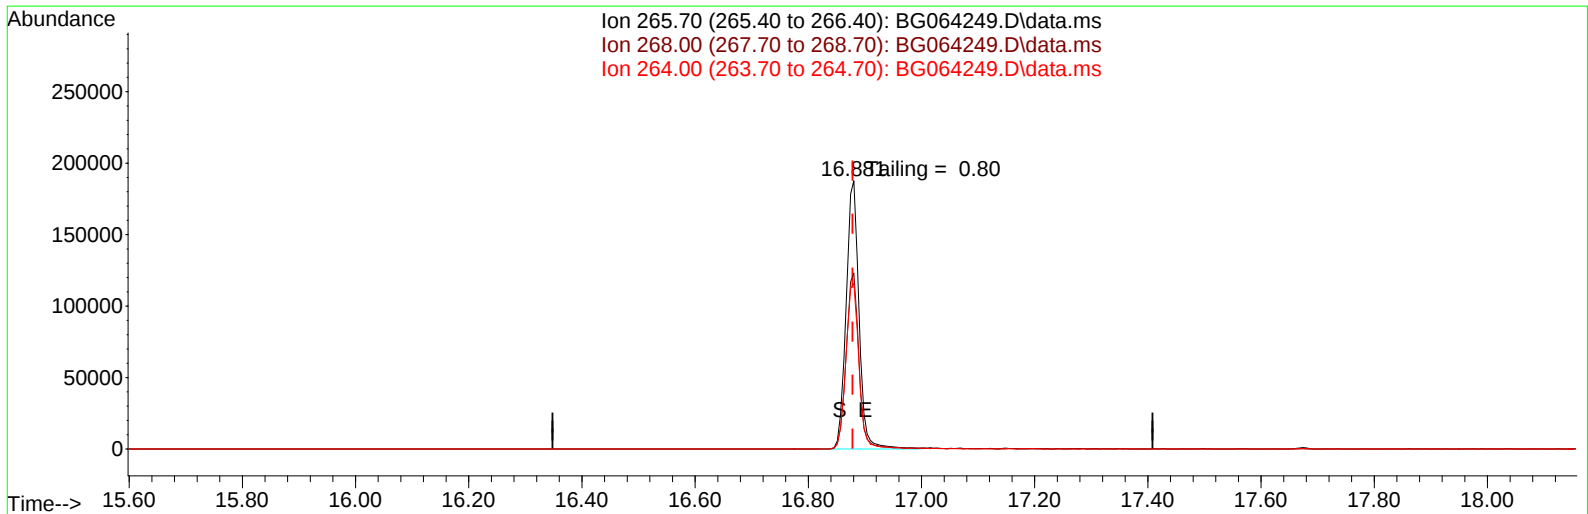

TIC: BG064249.D\data.ms

(70) Pentachlorophenol (C)

16.881min (+ 0.003) 612423.57 ng




response 297829

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	65.60
264.00	55.40	61.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG090325\
Data File : BG064249.D
Acq On : 3 Sep 2025 11:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 03 12:45:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 28 17:41:58 2025
Response via : Initial Calibration

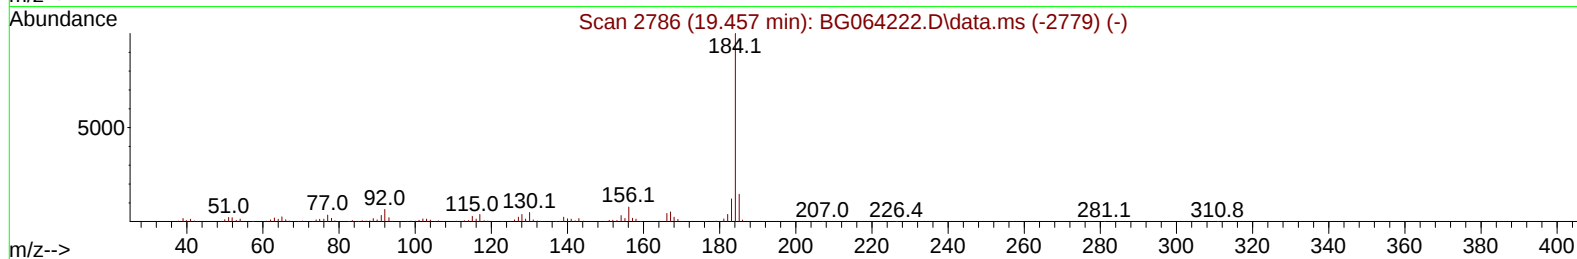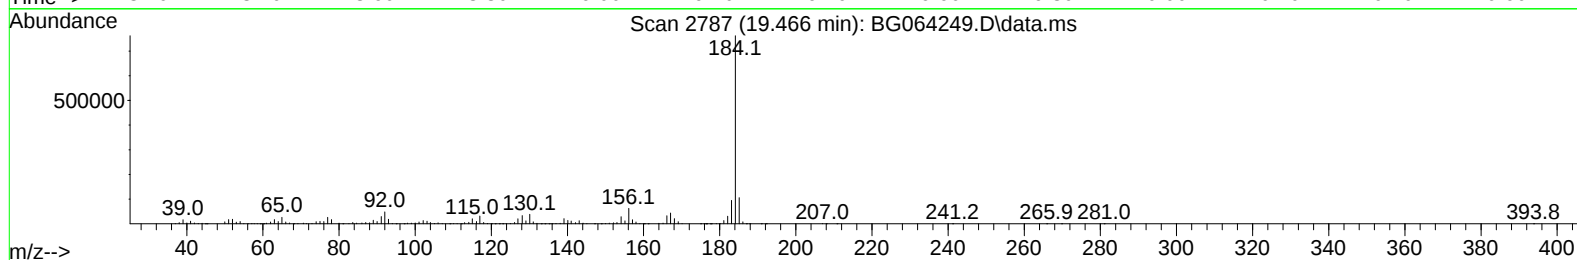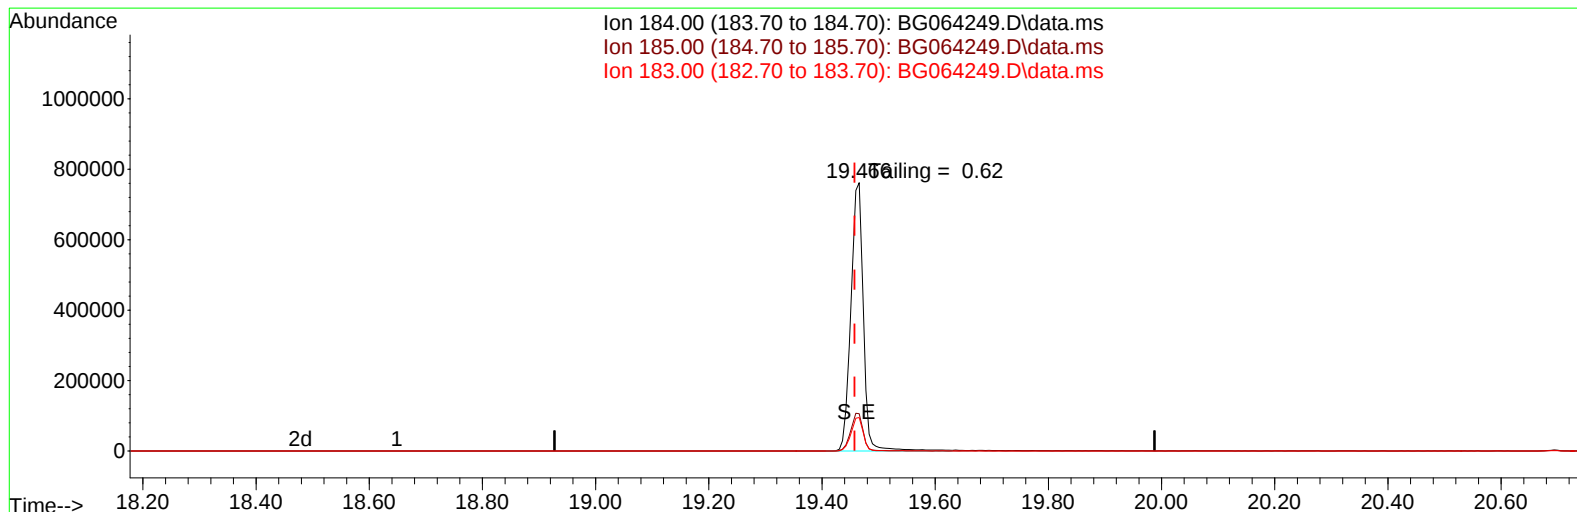

TIC: BG064249.D\data.ms

(77) Benzidine

19.466min (+ 0.008) 5991.08 ng m

response 1180283

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.90
183.00	12.10	12.48
0.00	0.00	0.00